

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
 Data File : VU026283.D
 Acq On : 23 Aug 2018 05:10
 Operator : MD/SY
 Sample : J4599-15 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOL5

Quant Time: Aug 23 07:48:24 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 23 07:46:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	285973	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	283643	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	134209	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	67879	38.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.84%
7) Chloroethane-d5	1.68	69	59620	41.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.84%
11) 1,1-Dichloroethene-d2	2.27	63	108870	31.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.52%
21) 2-Butanone-d5	4.18	46	131902	94.75	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.75%
24) Chloroform-d	4.65	84	172279	44.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.62%
26) 1,2-Dichloroethane-d4	5.31	65	115155	45.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.02%
32) Benzene-d6	5.35	84	326234	42.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.98%
36) 1,2-Dichloropropane-d6	6.33	67	109307	44.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.72%
41) Toluene-d8	7.57	98	295464	40.74	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.48%
43) trans-1,3-Dichloropropene-	7.85	79	50426	40.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.12%
47) 2-Hexanone-d5	8.31	63	92170	88.51	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.51%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	156641	43.44	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.88%
64) 1,2-Dichlorobenzene-d4	11.86	152	129844	45.59	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.18%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	11.49	75	14707	5.582 ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
Data File : VU026283.D
Acq On : 23 Aug 2018 05:10
Operator : MD/SY
Sample : J4599-15 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOL5

Quant Time: Aug 23 07:48:24 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 23 07:46:41 2018
Response via : Initial Calibration

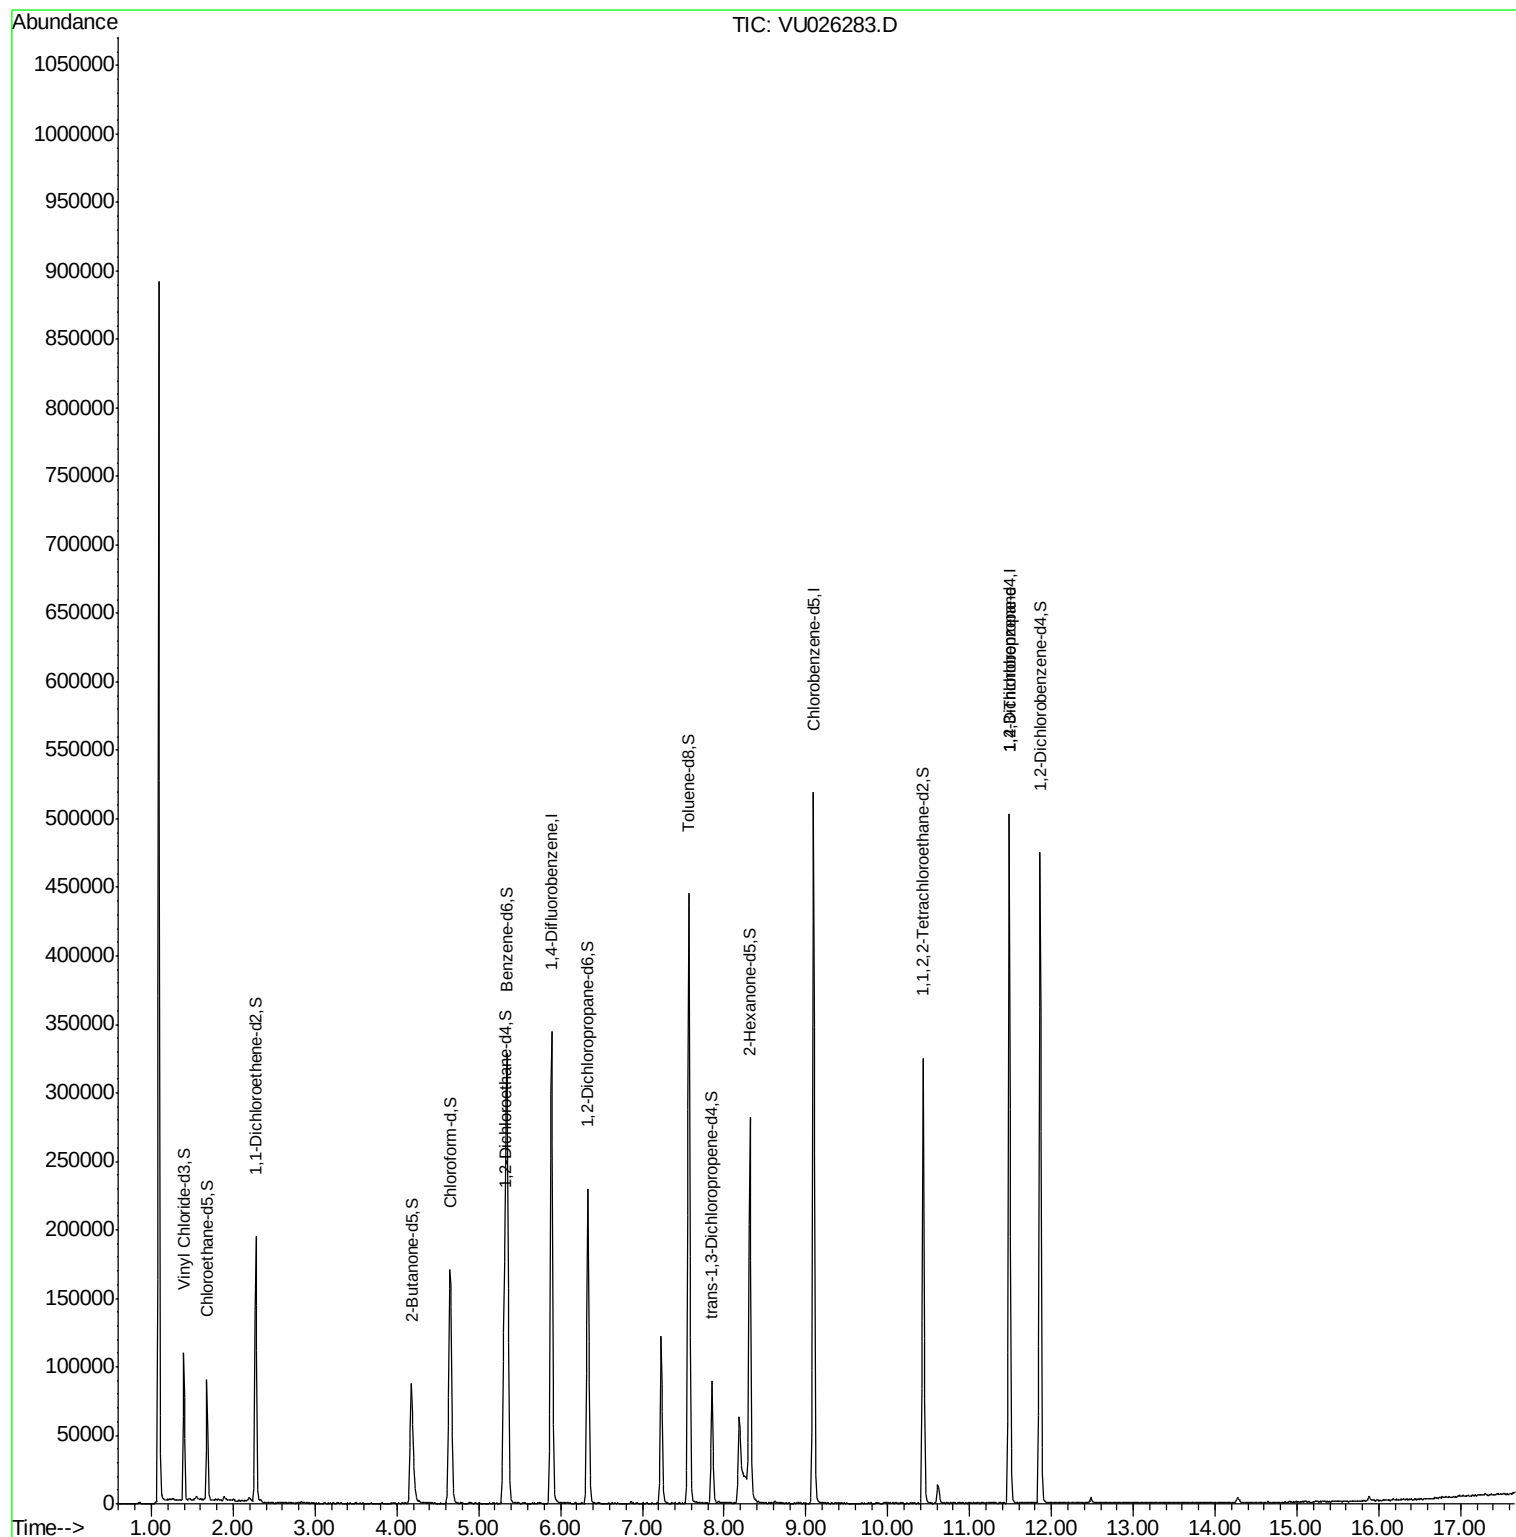

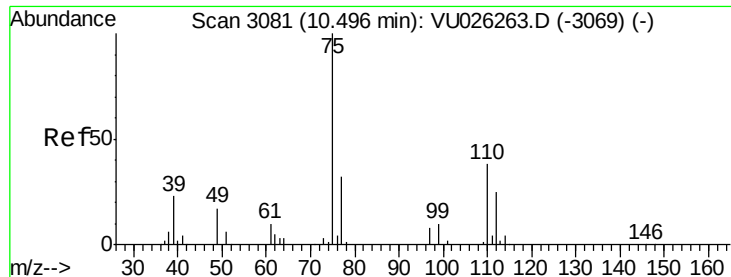

#59

1,2,3-Trichloropropane

Concen: 5.582 ug/L

RT: 11.49 min Scan# 3389

Delta R.T. 0.99 min

Lab File: VU026283.D

Acq: 23 Aug 2018 05:10

Instrument :

MSVOA_U

ClientSampleId :

ETOL5

Tgt Ion: 75 Resp: 14707

Ion Ratio Lower Upper

75 100

77 38.5 25.5 38.3#

