

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082218\
 Data File : VU026256.D
 Acq On : 22 Aug 2018 18:45
 Operator : MD/SY
 Sample : J4598-08 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.677	24	27	29	rBV	179	129	0.01%	0.001%
2	0.732	41	44	47	rBV2	300	171	0.02%	0.002%
3	0.751	47	50	52	rBV	165	129	0.01%	0.001%
4	0.777	56	58	60	rVB	138	60	0.01%	0.001%
5	0.799	61	65	66	rBV	155	111	0.01%	0.001%
6	0.834	72	76	79	rBV2	163	163	0.01%	0.002%
7	0.873	86	88	94	rVB	151	133	0.01%	0.001%
8	0.902	94	97	99	rBV	84	49	0.00%	0.001%
9	0.918	99	102	103	rBV	246	123	0.01%	0.001%
10	0.950	109	112	116	rBV2	244	218	0.02%	0.002%
11	0.995	123	126	127	rBV	258	144	0.01%	0.001%
12	1.024	132	135	138	rBV	275	197	0.02%	0.002%
13	1.088	146	155	173	rBV	808755	892402	80.61%	9.262%
14	1.397	245	251	263	rVB	127397	130765	11.81%	1.357%
15	1.680	332	339	354	rVB	102068	132096	11.93%	1.371%
16	2.272	513	523	536	rBV	222287	341561	30.85%	3.545%
17	2.699	652	656	665	rVB4	918	1365	0.12%	0.014%
18	2.838	692	699	702	rBV3	1183	1616	0.15%	0.017%
19	3.281	834	837	839	rBV	332	153	0.01%	0.002%
20	3.368	861	864	868	rBV2	249	220	0.02%	0.002%
21	3.477	891	898	901	rBV2	415	540	0.05%	0.006%
22	3.805	998	1000	1003	rBV	254	150	0.01%	0.002%
23	3.912	1030	1033	1035	rBV	262	170	0.02%	0.002%
24	4.053	1076	1077	1080	rBV	158	97	0.01%	0.001%
25	4.095	1086	1090	1096	rBV	278	356	0.03%	0.004%
26	4.178	1102	1116	1151	rBV2	101007	269297	24.32%	2.795%
27	4.474	1206	1208	1212	rBV2	336	178	0.02%	0.002%
28	4.522	1220	1223	1224	rBV2	238	148	0.01%	0.002%
29	4.555	1230	1233	1236	rBV2	255	225	0.02%	0.002%
30	4.651	1246	1263	1288	rBV2	191551	453656	40.98%	4.708%
31	4.886	1328	1336	1340	rBV3	681	981	0.09%	0.010%
32	4.928	1346	1349	1351	rBV2	190	107	0.01%	0.001%
33	4.953	1354	1357	1362	rVB2	586	504	0.05%	0.005%
34	4.979	1362	1365	1368	rBV2	385	238	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082218\
 Data File : VU026256.D
 Acq On : 22 Aug 2018 18:45
 Operator : MD/SY
 Sample : J4598-08 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

35	5.075	1392	1395	1397	rBV	266	170	0.02%	0.002%
36	5.095	1400	1401	1403	rBV	253	114	0.01%	0.001%
37	5.127	1409	1411	1413	rBV2	329	188	0.02%	0.002%
38	5.194	1429	1432	1437	rBV2	187	151	0.01%	0.002%
39	5.246	1447	1448	1451	rBV	146	75	0.01%	0.001%
40	5.346	1454	1479	1499	rBV2	374067	1107119	100.00%	11.490%
41	5.481	1520	1521	1522	rBV	210	60	0.01%	0.001%
42	5.503	1525	1528	1533	rBV3	260	272	0.02%	0.003%
43	5.603	1555	1559	1561	rBV2	338	263	0.02%	0.003%
44	5.657	1574	1576	1578	rBV	173	121	0.01%	0.001%
45	5.673	1578	1581	1586	rVB2	472	387	0.03%	0.004%
46	5.728	1595	1598	1599	rBV	161	72	0.01%	0.001%
47	5.754	1604	1606	1608	rVV	172	73	0.01%	0.001%
48	5.812	1622	1624	1626	rBB	131	68	0.01%	0.001%
49	5.828	1627	1629	1633	rVB2	183	121	0.01%	0.001%
50	5.889	1633	1648	1673	rBV	344910	674660	60.94%	7.002%
51	6.056	1698	1700	1703	rBV2	315	215	0.02%	0.002%
52	6.075	1704	1706	1709	rVB2	362	209	0.02%	0.002%
53	6.098	1710	1713	1717	rBV2	354	192	0.02%	0.002%
54	6.172	1732	1736	1737	rBV2	414	289	0.03%	0.003%
55	6.210	1746	1748	1751	rBV2	201	87	0.01%	0.001%
56	6.246	1756	1759	1761	rBV	280	207	0.02%	0.002%
57	6.275	1767	1768	1772	rBV	202	83	0.01%	0.001%
58	6.333	1772	1786	1806	rBV	253232	510383	46.10%	5.297%
59	6.503	1837	1839	1842	rVB2	303	150	0.01%	0.002%
60	6.529	1844	1847	1852	rBV2	373	306	0.03%	0.003%
61	6.554	1853	1855	1857	rBV	185	69	0.01%	0.001%
62	6.590	1862	1866	1867	rBV	187	133	0.01%	0.001%
63	6.654	1881	1886	1891	rVB2	334	304	0.03%	0.003%
64	6.677	1891	1893	1894	rBV	115	54	0.00%	0.001%
65	6.712	1901	1904	1905	rBV2	205	126	0.01%	0.001%
66	6.757	1913	1918	1922	rBV	373	354	0.03%	0.004%
67	6.860	1945	1950	1959	rBV4	916	1505	0.14%	0.016%
68	6.931	1969	1972	1974	rBV2	218	146	0.01%	0.002%
69	7.043	2000	2007	2008	rBV	317	322	0.03%	0.003%
70	7.075	2015	2017	2019	rBV	34	17	0.00%	0.000%
71	7.088	2019	2021	2023	rBV	304	195	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082218\
 Data File : VU026256.D
 Acq On : 22 Aug 2018 18:45
 Operator : MD/SY
 Sample : J4598-08 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

72	7.153	2038	2041	2043	rBV2	153	134	0.01%	0.001%
73	7.230	2053	2065	2084	rBV	143843	253294	22.88%	2.629%
74	7.410	2117	2121	2123	rBV3	441	255	0.02%	0.003%
75	7.426	2123	2126	2130	rVB2	221	136	0.01%	0.001%
76	7.567	2155	2170	2188	rBV	512608	878077	79.31%	9.113%
77	7.763	2229	2231	2233	rVB	265	97	0.01%	0.001%
78	7.850	2246	2258	2280	rBV	106306	182414	16.48%	1.893%
79	8.101	2333	2336	2341	rBV3	553	530	0.05%	0.006%
80	8.185	2350	2362	2374	rBV2	53546	132032	11.93%	1.370%
81	8.313	2394	2402	2425	rVB	331355	551151	49.78%	5.720%
82	8.574	2480	2483	2486	rBV2	334	220	0.02%	0.002%
83	8.670	2511	2513	2514	rBV	260	112	0.01%	0.001%
84	8.776	2541	2546	2549	rBV2	383	483	0.04%	0.005%
85	9.091	2631	2644	2667	rBV	509593	836032	75.51%	8.677%
86	9.313	2709	2713	2718	rBV2	433	337	0.03%	0.003%
87	9.773	2848	2856	2859	rBV3	413	688	0.06%	0.007%
88	9.956	2908	2913	2920	rVB2	746	796	0.07%	0.008%
89	10.027	2931	2935	2936	rBV	393	251	0.02%	0.003%
90	10.082	2949	2952	2957	rVB	431	326	0.03%	0.003%
91	10.120	2961	2964	2966	rBV2	293	238	0.02%	0.002%
92	10.432	3048	3061	3082	rBV	364015	582736	52.64%	6.048%
93	10.615	3106	3118	3132	rBV2	13070	25262	2.28%	0.262%
94	11.049	3251	3253	3255	rBV	335	177	0.02%	0.002%
95	11.487	3377	3389	3408	rBV	511081	796355	71.93%	8.265%
96	11.747	3467	3470	3473	rBV	298	202	0.02%	0.002%
97	11.863	3492	3506	3525	rBV	543440	865436	78.17%	8.982%


Sum of corrected areas: 9635483

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082218\
Data File : VU026256.D
Acq On : 22 Aug 2018 18:45
Operator : MD/SY
Sample : J4598-08 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBM7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

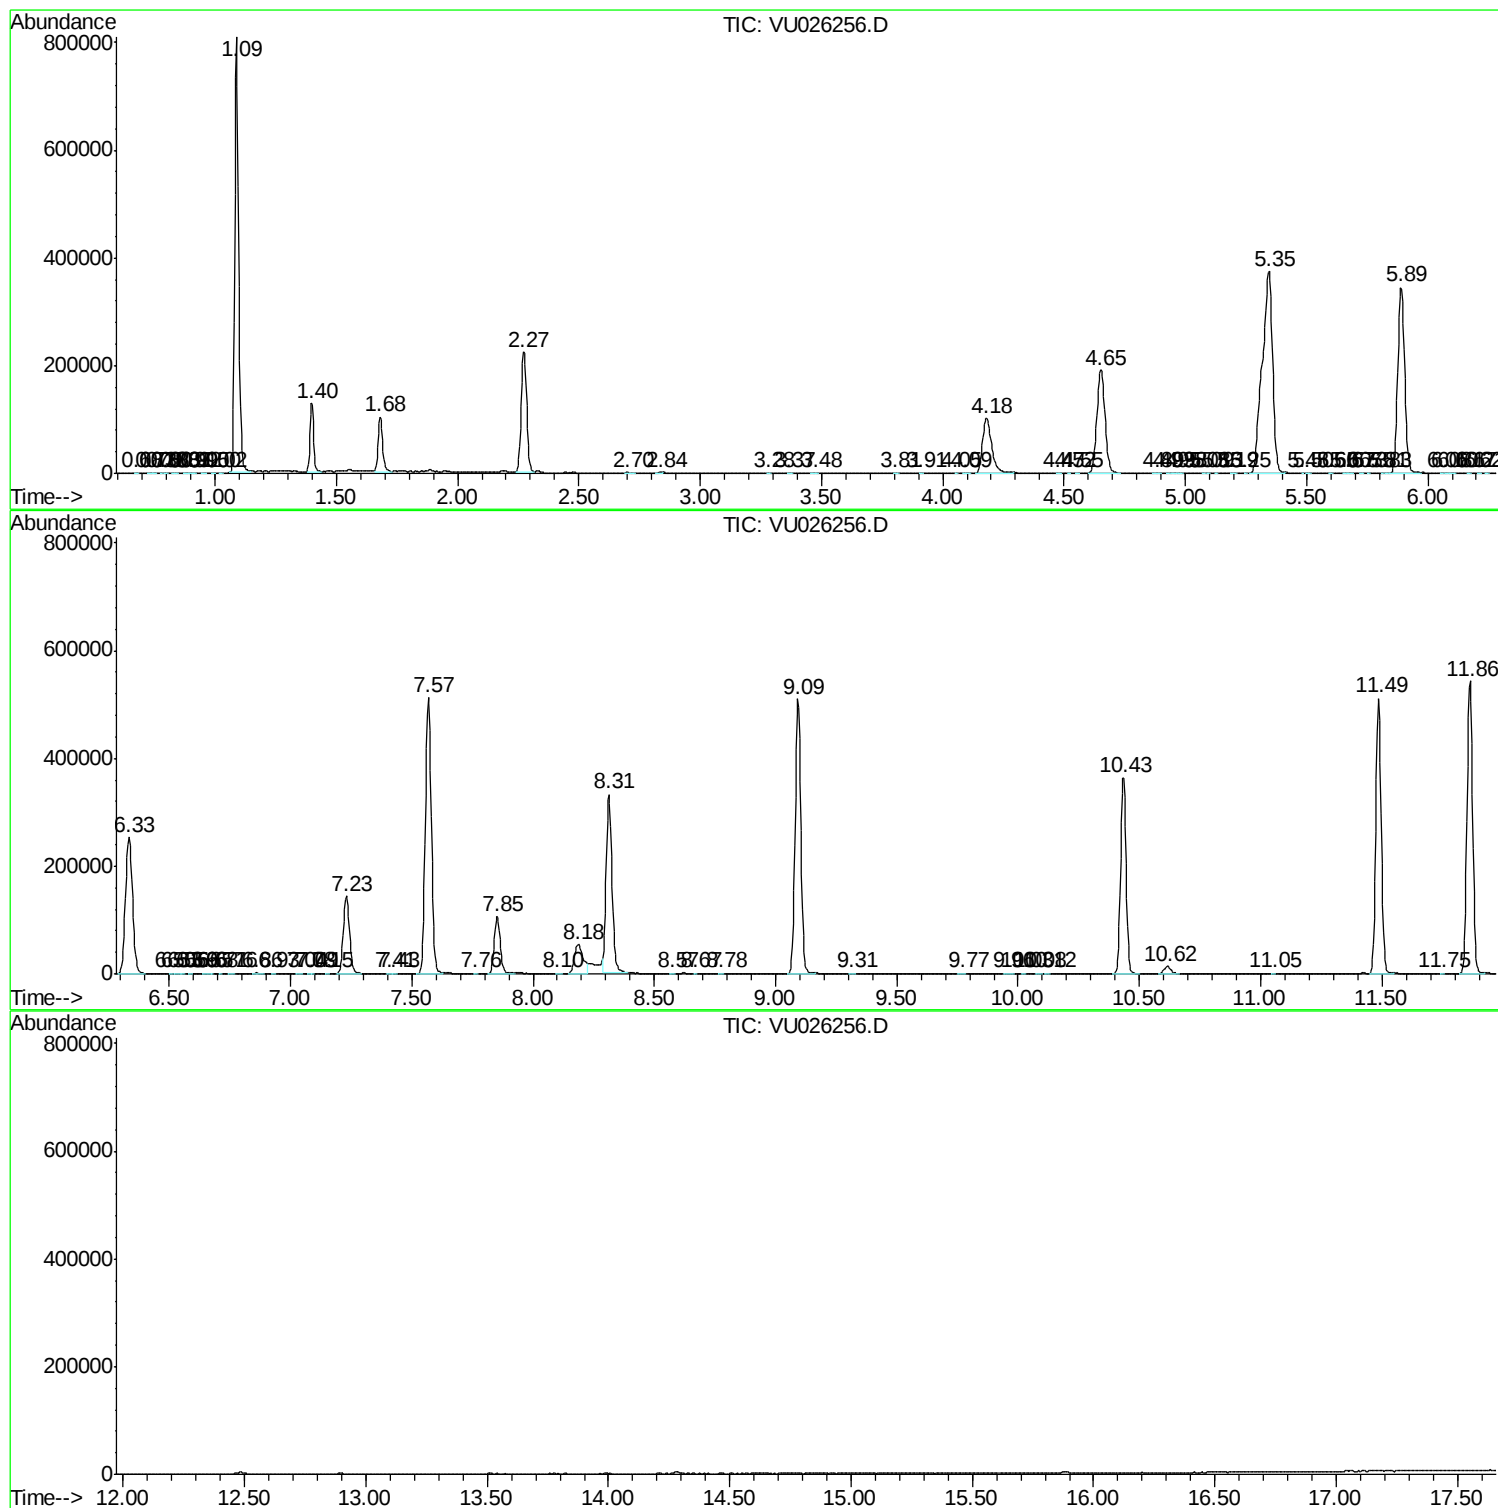

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
Data File : VU026256.D
Acq On : 22 Aug 2018 18:45
Operator : MD/SY
Sample : J4598-08 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBM7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
Data File : VU026256.D
Acq On : 22 Aug 2018 18:45
Operator : MD/SY
Sample : J4598-08 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBM7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
