


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082218\
Data File : VU026238.D
Acq On : 22 Aug 2018 10:43
Operator : MD/SY
Sample : BFB40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Title : VOC Analysis
Last Update : Thu Aug 23 07:46:41 2018

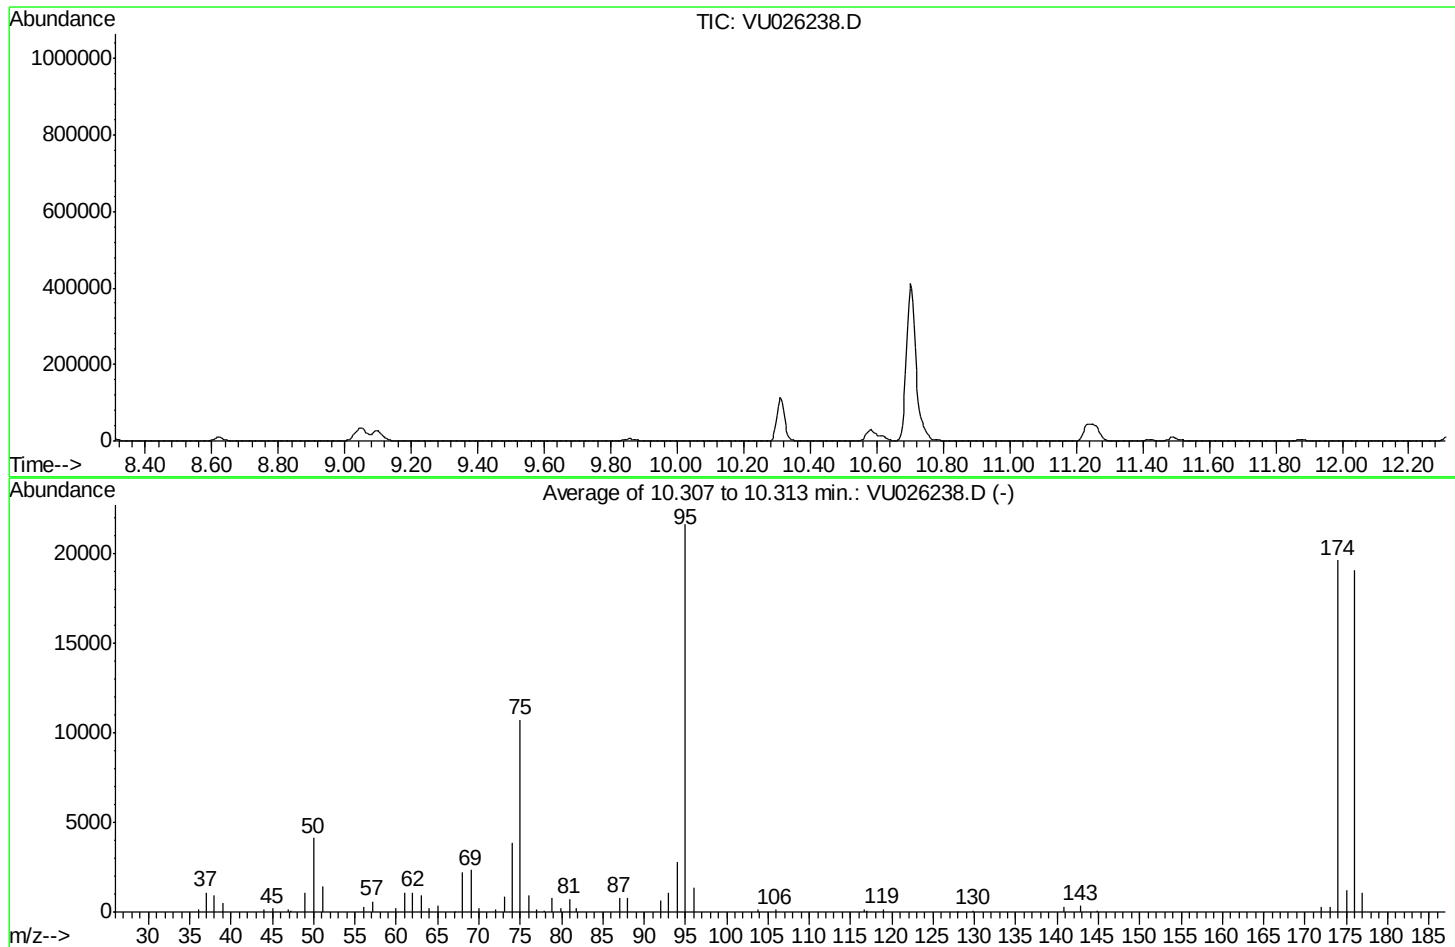

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	4142	PASS
75	95	30	80	49.6	10733	PASS
95	95	100	100	100.0	21656	PASS
96	95	5	9	6.3	1371	PASS
173	174	0.00	2	1.6	305	PASS
174	95	50	120	90.7	19645	PASS
175	174	5	9	6.3	1235	PASS
176	174	95	101	97.3	19122	PASS
177	176	5	9	5.5	1058	PASS

Scan 3012 (10.275 min): VU026238.D
BFB40

m/z	Abundance
39.80	159.0
43.90	345.0
206.90	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	211.0
37.00	1027.0
38.00	879.0
39.10	584.0
39.90	152.0
44.00	527.0
45.10	206.0
46.90	268.0
49.00	1041.0
50.00	4026.0
51.00	1367.0
56.00	275.0
57.10	612.0
59.90	189.0
61.00	1002.0
62.00	1010.0
63.00	941.0
64.00	224.0
65.00	392.0
68.00	2180.0
69.00	2166.0
69.90	235.0
72.00	187.0
73.00	865.0
74.00	3727.0
75.00	10292.0
76.00	967.0
76.90	107.0
78.90	829.0
79.90	198.0
80.90	672.0
81.90	238.0
87.00	861.0
88.00	845.0
92.00	606.0
93.00	1007.0
94.00	2663.0
95.00	20712.0
96.00	1356.0
103.80	114.0
105.90	124.0
116.70	237.0
118.90	160.0
140.80	297.0
142.80	276.0
144.90	157.0
171.90	327.0
173.00	281.0
174.00	18552.0
175.00	1261.0
176.00	17744.0
177.00	1094.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	168.0
37.00	1151.0
38.00	979.0
39.10	578.0
40.00	118.0
44.00	523.0
45.00	200.0
47.00	257.0
49.00	1122.0
50.00	4286.0
51.00	1527.0
56.00	329.0
57.10	627.0
59.90	210.0
61.00	1121.0
62.00	1143.0
63.00	940.0
64.00	245.0
65.00	406.0
67.00	104.0
68.00	2343.0
69.00	2449.0
70.00	253.0
72.00	178.0
73.10	874.0
74.00	3976.0
75.00	11037.0
76.00	935.0
76.90	124.0
77.90	117.0
78.90	824.0
79.90	195.0
80.90	725.0
81.90	224.0
87.00	820.0
88.00	755.0
92.00	678.0
93.00	1079.0
94.00	2887.0
95.00	22552.0
96.00	1404.0
103.80	131.0
105.90	130.0
116.70	224.0
118.90	172.0
129.90	106.0
140.90	317.0
142.90	335.0
144.90	106.0
171.90	315.0
173.00	326.0
174.00	20256.0
175.00	1259.0
176.00	19768.0
177.00	1074.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	133.0
37.00	1131.0
38.00	965.0
39.00	445.0
40.10	109.0
44.00	523.0
45.00	189.0
47.20	260.0
49.00	1013.0
50.00	4116.0
51.10	1408.0
56.00	341.0
57.10	544.0
59.90	197.0
61.00	1074.0
62.00	1150.0
63.00	928.0
64.00	206.0
65.00	296.0
68.00	2192.0
69.00	2420.0
70.00	236.0
72.00	145.0
73.10	777.0
74.00	3981.0
75.00	10871.0
76.00	851.0
76.90	140.0
77.80	157.0
78.90	770.0
79.90	187.0
81.00	760.0
81.80	214.0
87.10	681.0
88.00	747.0
92.00	699.0
93.00	1062.0
94.00	2809.0
95.00	21704.0
96.00	1354.0
103.70	107.0
105.90	126.0
116.90	197.0
118.90	163.0
128.00	104.0
129.80	116.0
140.90	318.0
142.90	370.0
171.90	313.0
173.00	310.0
174.00	20128.0
175.00	1187.0
176.00	19856.0
177.00	1008.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40