

Data File : VU033913.D
Acq On : 22 Aug 2019 20:42
Operator : JC/SP
Sample : K4454-04DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B87DL

Quant Time: Aug 23 03:05:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 23 02:53:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	620016	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	619268	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	263384	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	195042	35.87	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.74%
7) Chloroethane-d5	1.67	69	175298	40.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.28%
11) 1,1-Dichloroethene-d2	2.25	63	292233	29.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.58%#
21) 2-Butanone-d5	4.15	46	363975	99.48	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.48%
24) Chloroform-d	4.62	84	387519	43.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.56%
26) 1,2-Dichloroethane-d4	5.28	65	262149	45.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.66%
32) Benzene-d6	5.31	84	757191	43.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.08%
36) 1,2-Dichloropropane-d6	6.31	67	261972	45.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.78%
41) Toluene-d8	7.54	98	645326	40.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.20%
43) trans-1,3-Dichloropropene-	7.83	79	104287	39.59	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.18%
47) 2-Hexanone-d5	8.29	63	237040	99.86	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.86%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	374020	46.01	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.02%
64) 1,2-Dichlorobenzene-d4	11.84	152	252054	46.90	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.80%

Target Compounds


						Qvalue
20) cis-1,2-Dichloroethene	4.20	96	110840	22.420	ug/L	99
34) Trichloroethene	6.16	95	198698	40.895	ug/L	99
46) Tetrachloroethene	8.21	164	52199	13.824	ug/L	97
48) 2-Hexanone	8.29	43	28427	4.990	ug/L #	71
59) 1,2,3-Trichloropropane	11.47	75	32099	4.903	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU033913.D
Acq On : 22 Aug 2019 20:42
Operator : JC/SP
Sample : K4454-04DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B87DL

Quant Time: Aug 23 03:05:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 23 02:53:44 2019
Response via : Initial Calibration

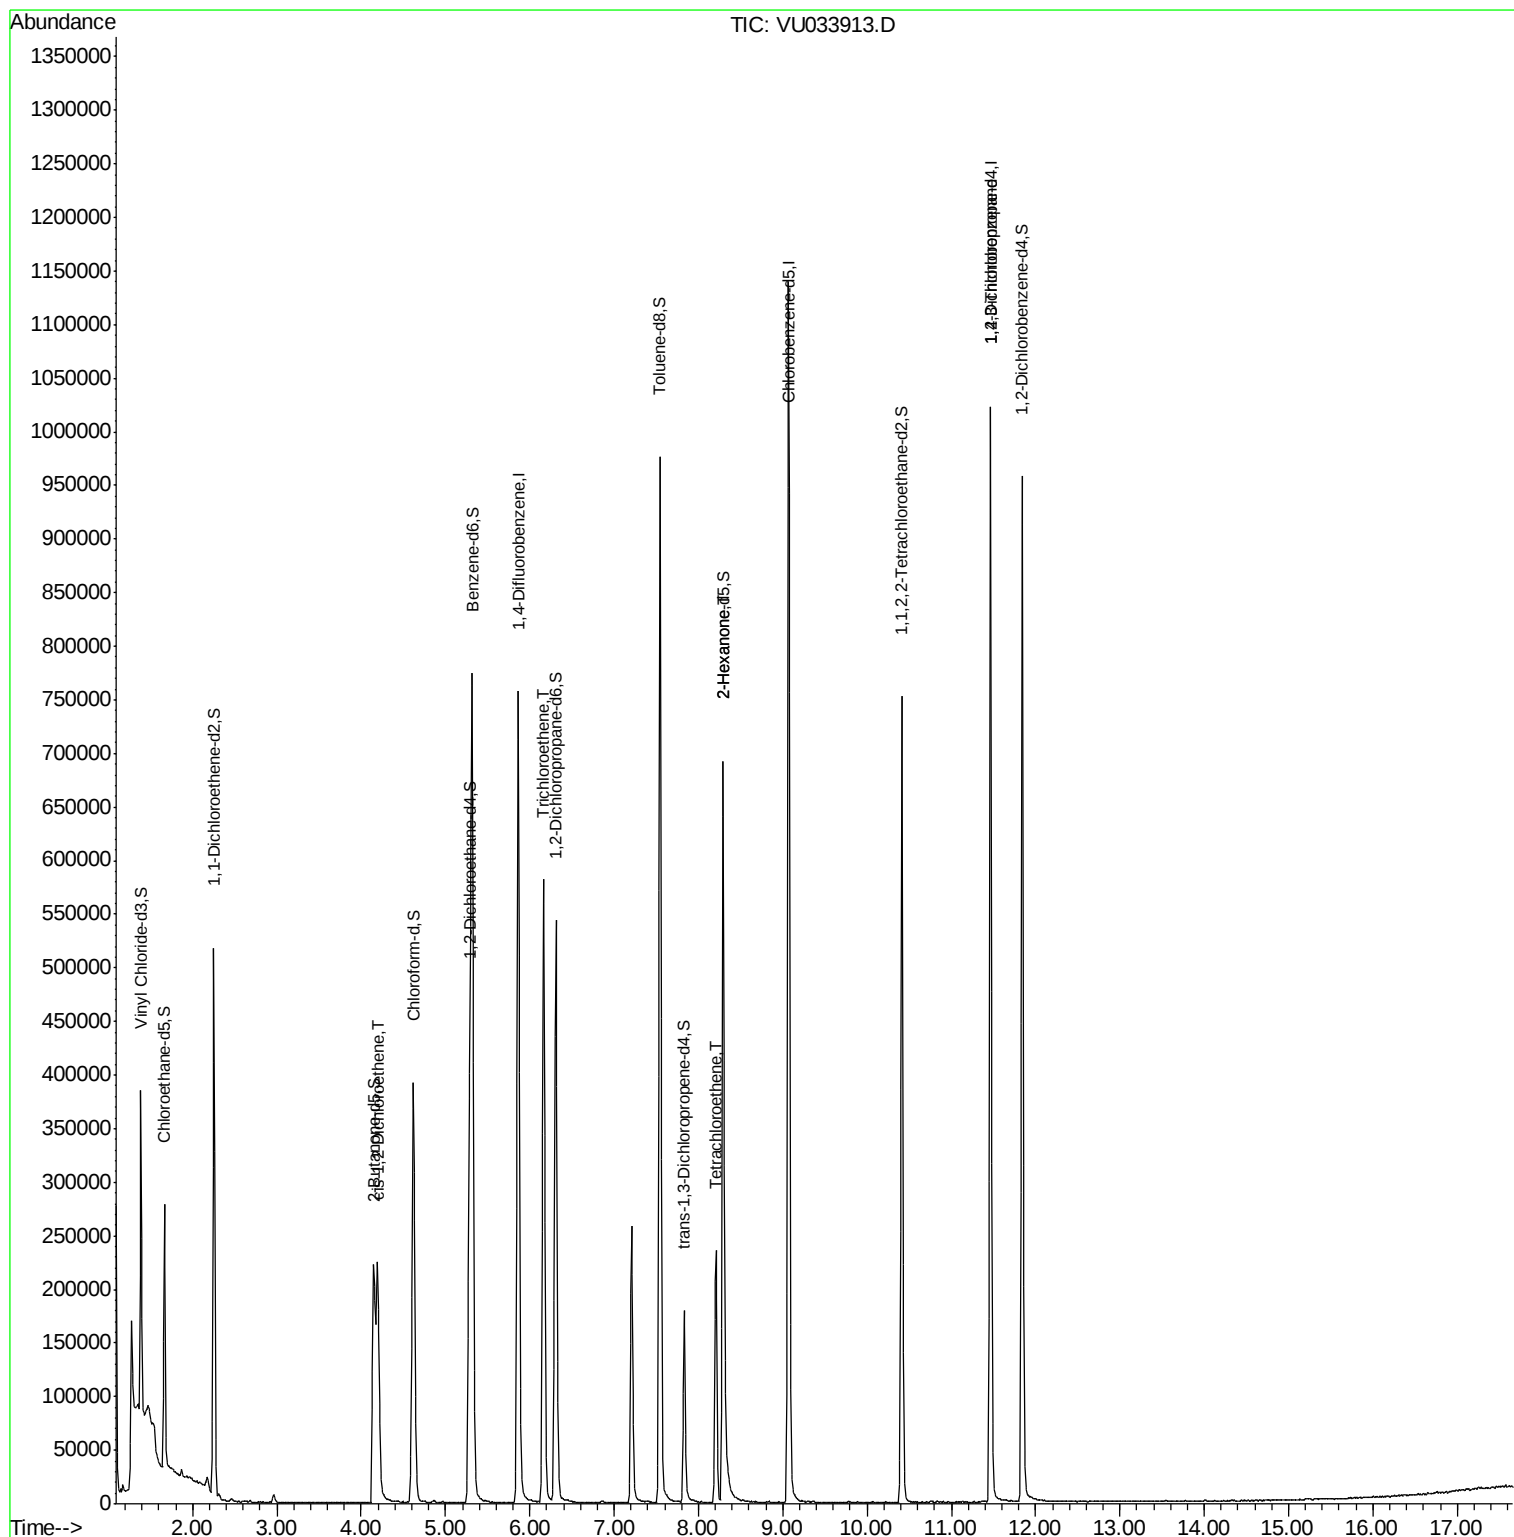

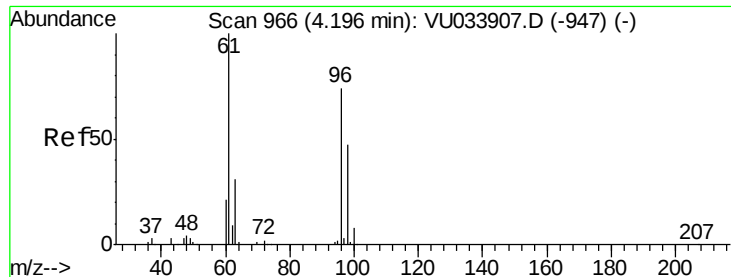

#20

cis-1,2-Dichloroethene

Concen: 22.420 ug/L

RT: 4.20 min Scan# 966

Delta R.T. -0.00 min

Lab File: VU033913.D

Acq: 22 Aug 2019 20:42

Instrument :

MSVOA_U

ClientSampleId :

F2B87DL


Tgt Ion: 96 Resp: 110840

Ion Ratio Lower Upper

96 100

61 135.7 95.5 177.4




68 0.0 0.0 0.0

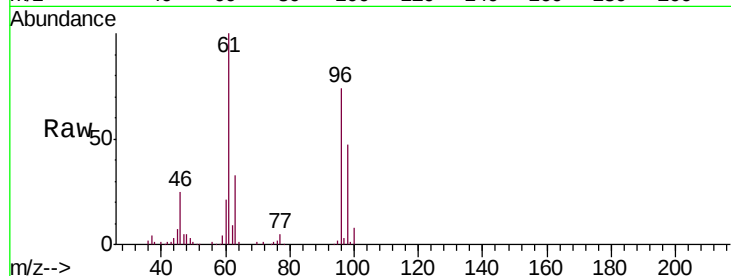

Abundance Ion 96.00 (95.70 to 96.70): VU033913.D (-873) (-)

Ion 61.00 (60.70 to 61.70): VU033913.D (-873) (-)

Ion 68.00 (67.70 to 68.70): VU033913.D (-873) (-)

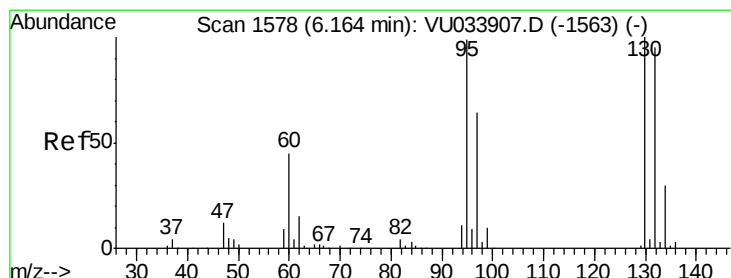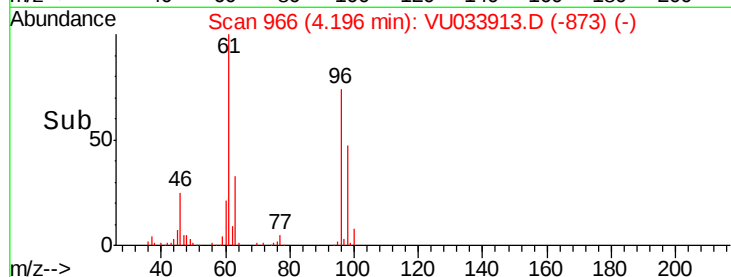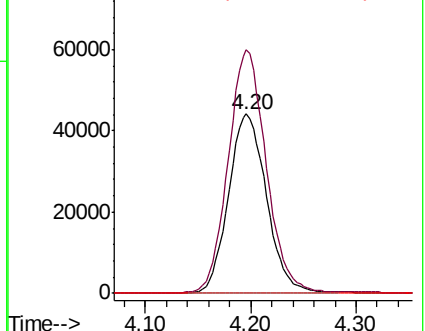

#34

Trichloroethene

Concen: 40.895 ug/L

RT: 6.16 min Scan# 1578

Delta R.T. -0.00 min

Lab File: VU033913.D

Acq: 22 Aug 2019 20:42

Tgt Ion: 95 Resp: 198698


Ion Ratio Lower Upper

95 100

97 64.2 44.7 82.9

132 96.3 65.7 122.1

130 99.3 70.0 130.0


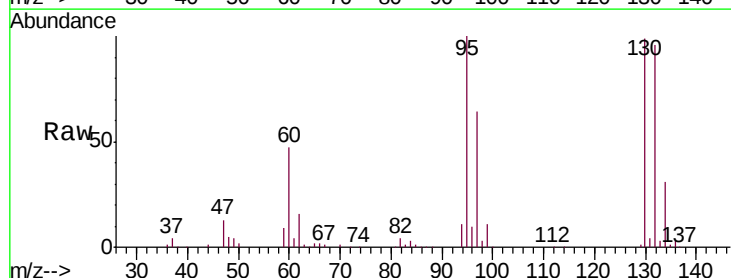



Abundance Ion 95.00 (94.70 to 95.70): VU033913.D (-1485) (-)

Ion 97.00 (96.70 to 97.70): VU033913.D (-1485) (-)

Ion 132.00 (131.70 to 132.70): VU033913.D (-1485) (-)

Ion 130.00 (129.70 to 130.70): VU033913.D (-1485) (-)

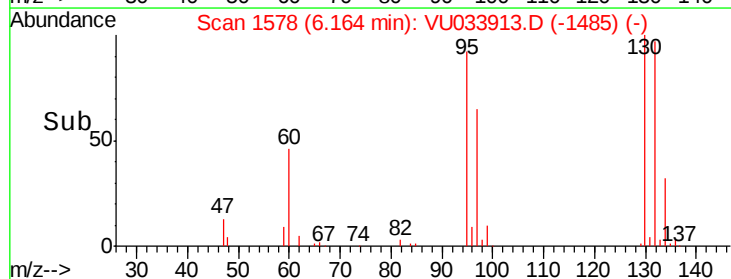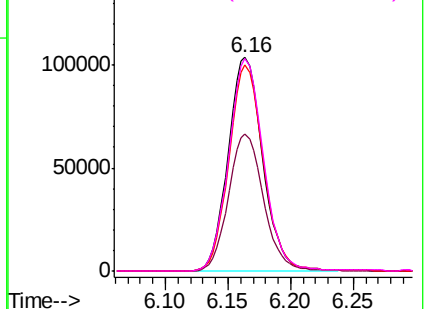

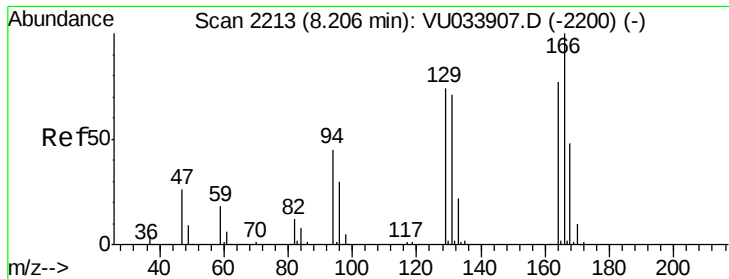

#46

Tetrachloroethene

Concen: 13.824 ug/L

RT: 8.21 min Scan# 2214

Delta R.T. 0.00 min

Lab File: VU033913.D

Acq: 22 Aug 2019 20:42

Instrument :

MSVOA_U

ClientSampleId :

F2B87DL

Tgt Ion:164 Resp: 52199


Ion Ratio Lower Upper

164 100

129 95.4 63.9 118.7

131 89.4 62.5 116.1

166 130.1 87.3 162.1



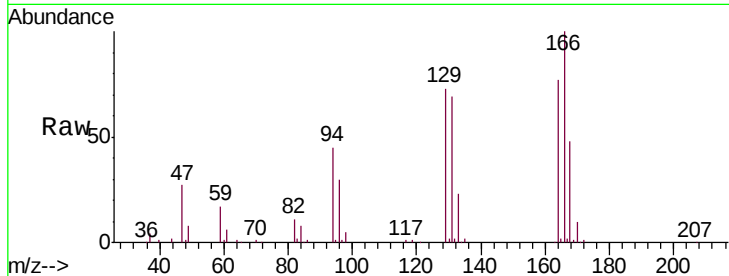


Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

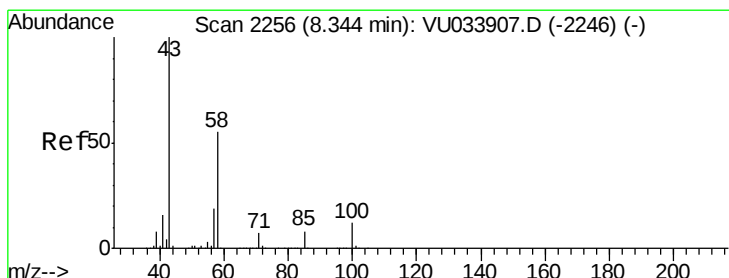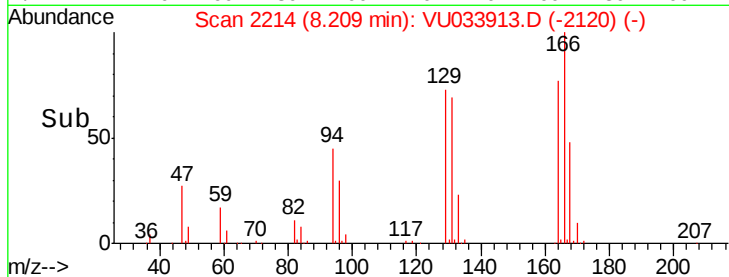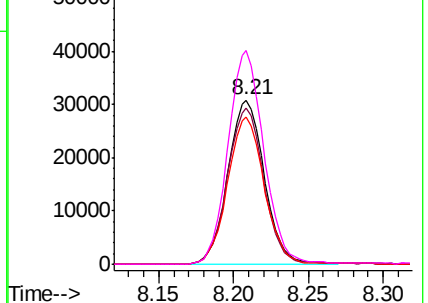

#48

2-Hexanone

Concen: 4.990 ug/L

RT: 8.29 min Scan# 2240

Delta R.T. -0.05 min

Lab File: VU033913.D

Acq: 22 Aug 2019 20:42

Tgt Ion: 43 Resp: 28427


Ion Ratio Lower Upper

43 100

58 33.0 44.3 66.5#

57 31.0 15.3 22.9#

100 1.8 9.4 14.2#


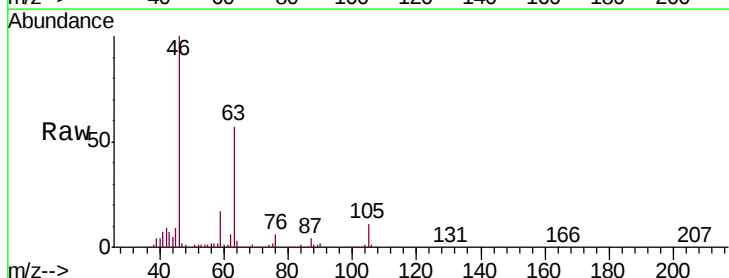



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

Ion 57.00 (56.70 to 57.70): VU0

Ion 100.00 (99.70 to 100.70): VU0

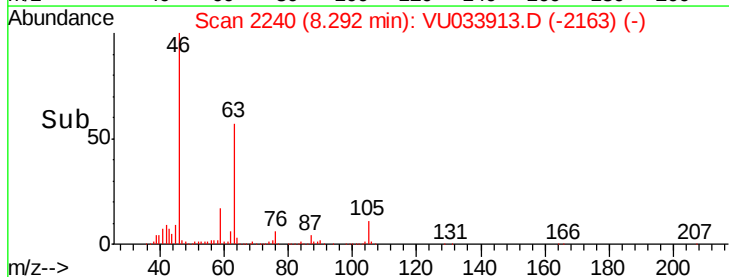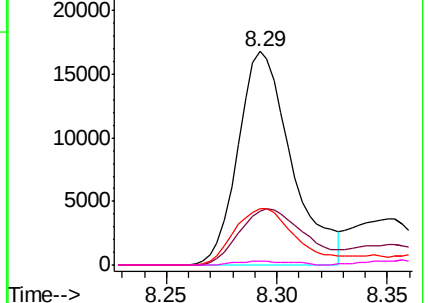

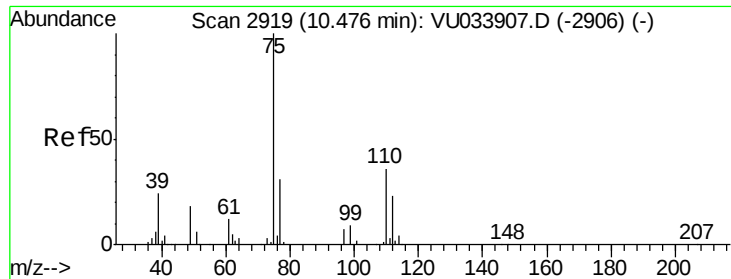

#59

1,2,3-Trichloropropane

Concen: 4.903 ug/L

RT: 11.47 min Scan# 3227

Delta R.T. 0.99 min

Lab File: VU033913.D

Acq: 22 Aug 2019 20:42

Instrument :

MSVOA_U

ClientSampleId :

F2B87DL

Tgt Ion: 75 Resp: 32099

Ion Ratio Lower Upper

75 100

77 38.0 25.8 38.8

