


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082219\
Data File : VU033898.D
Acq On : 22 Aug 2019 14:18
Operator : JC/SP
Sample : BFB60
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082219WMA.M
Title : VOC Analysis
Last Update : Fri Aug 23 02:53:44 2019

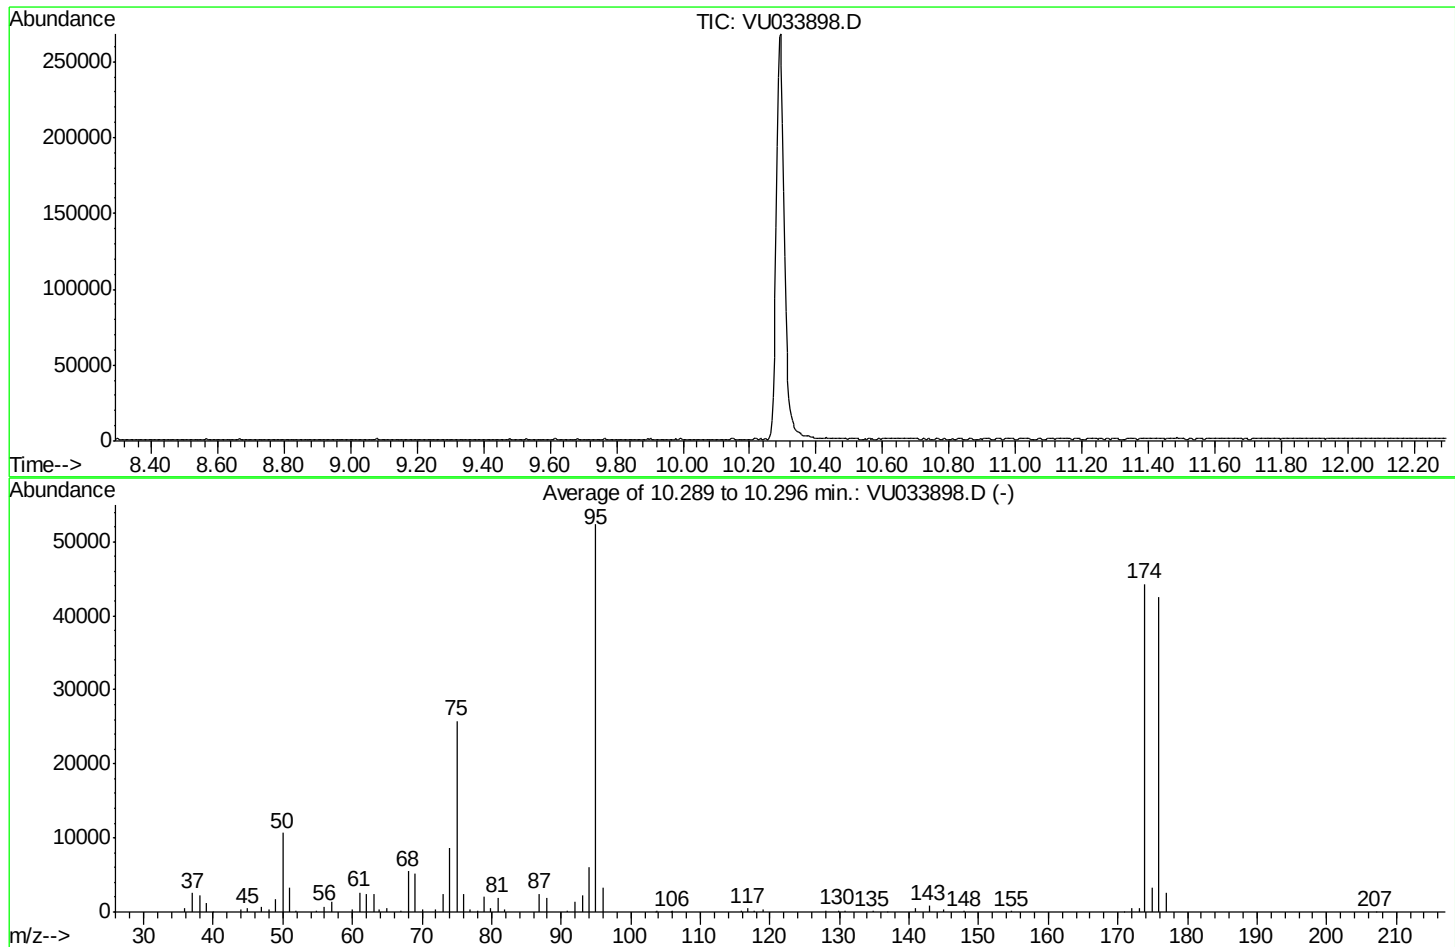

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	10713	PASS
75	95	30	80	49.2	25768	PASS
95	95	100	100	100.0	52344	PASS
96	95	5	9	6.2	3240	PASS
173	174	0.00	2	1.2	532	PASS
174	95	50	120	84.6	44301	PASS
175	174	5	9	7.6	3350	PASS
176	174	95	101	96.2	42602	PASS
177	176	5	9	6.1	2592	PASS

m/z	Abundance
36.00	521.0
37.00	2637.0
38.00	2295.0
39.00	1146.0
40.00	343.0
43.90	1101.0
45.00	512.0
47.00	724.0
47.90	380.0
49.00	1934.0
50.00	11221.0
51.00	3380.0
51.90	144.0
54.90	137.0
56.00	760.0
57.00	1422.0
60.00	395.0
61.00	2854.0
62.00	2637.0
63.00	2503.0
63.90	489.0
65.00	519.0
66.90	130.0
68.00	5546.0
69.00	5415.0
70.00	407.0
72.00	303.0
73.00	2430.0
74.00	9029.0
75.00	27088.0
76.00	2537.0
76.90	339.0
78.00	222.0
78.90	2007.0
79.90	437.0
80.90	2071.0
81.90	362.0
86.90	2666.0
87.90	1977.0
90.90	276.0
92.00	1389.0
93.00	2386.0
94.00	6365.0
95.00	53872.0
96.00	3292.0
103.60	157.0
106.00	184.0
115.90	153.0
116.80	430.0
117.80	258.0
118.90	300.0
128.00	146.0
129.90	240.0
130.80	147.0
136.90	102.0
140.90	492.0
142.90	832.0
144.90	325.0
147.90	144.0
154.70	133.0
170.90	108.0
172.00	437.0
173.00	554.0
173.90	44080.0
174.90	3382.0
175.90	42472.0
176.90	2547.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	467.0
37.00	2677.0
38.00	2300.0
38.90	1279.0
40.00	358.0
43.90	1113.0
44.90	509.0
46.90	651.0
48.00	371.0
49.00	1777.0
50.00	11174.0
51.00	3463.0
51.90	139.0
54.80	126.0
56.00	745.0
57.00	1425.0
60.00	375.0
61.00	2734.0
62.00	2548.0
63.00	2431.0
63.90	444.0
65.00	487.0
66.90	148.0
68.00	5642.0
69.00	5253.0
70.00	333.0
72.00	347.0
73.00	2535.0
74.00	8920.0
75.00	26504.0
76.00	2432.0
76.90	302.0
77.90	257.0
78.90	2087.0
79.90	512.0
80.90	1955.0
81.90	346.0
86.90	2540.0
87.90	1935.0
90.90	252.0
92.00	1414.0
93.00	2246.0
94.00	6171.0
95.00	54032.0
96.00	3327.0
103.80	186.0
106.00	151.0
115.90	148.0
116.90	460.0
117.80	253.0
118.90	300.0
128.00	160.0
129.90	219.0
130.80	178.0
134.80	152.0
140.90	523.0
142.90	864.0
144.90	391.0
147.90	163.0
154.70	191.0
171.90	524.0
173.00	557.0
173.90	45752.0
174.90	3473.0
175.90	43792.0
177.00	2691.0
207.00	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
35.90	434.0
37.00	2394.0
38.00	2138.0
38.90	1310.0
40.00	397.0
43.90	1002.0
44.90	416.0
46.90	556.0
48.00	358.0
49.00	1620.0
50.00	9744.0
51.00	3174.0
51.90	135.0
54.80	157.0
56.00	662.0
57.00	1359.0
60.00	392.0
61.00	2408.0
62.00	2335.0
63.10	2233.0
63.90	376.0
65.00	455.0
66.90	149.0
68.00	5185.0
69.00	4703.0
70.00	276.0
72.00	340.0
73.00	2400.0
74.00	8136.0
75.00	23712.0
76.00	2262.0
76.80	236.0
77.90	249.0
78.90	1925.0
79.90	593.0
80.90	1735.0
81.90	294.0
86.90	2072.0
88.00	1887.0
90.80	201.0
92.00	1243.0
93.00	1940.0
94.00	5580.0
95.00	49128.0
96.00	3101.0
103.80	206.0
105.70	113.0
106.00	116.0
115.90	136.0
116.90	458.0
117.80	243.0
119.00	291.0
128.00	159.0
129.80	197.0
130.90	177.0
134.80	162.0
140.90	484.0
142.80	887.0
144.90	402.0
147.90	179.0
154.70	185.0
172.00	624.0
173.00	486.0
173.90	43072.0
174.90	3197.0
175.90	41544.0
176.90	2540.0
207.10	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

Scan 2849 (10.251 min): VU033898.D
BFB60

m/z	Abundance
40.00	319.0
44.00	746.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60