

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082222\
 Data File : VU050393.D
 Acq On : 22 Aug 2022 11:24
 Operator : SY/MD
 Sample : VU0822WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0822WBL01

Quant Time: Aug 23 08:20:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Aug 23 08:18:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	31503	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	8078	0.753	ug/l	0.00
Spiked Amount 1.000			Recovery	=	75.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	9837	0.776	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082222\
Data File : VU050393.D
Acq On : 22 Aug 2022 11:24
Operator : SY/MD
Sample : VU0822WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0822WBL01

Quant Time: Aug 23 08:20:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Aug 23 08:18:20 2022
Response via : Initial Calibration




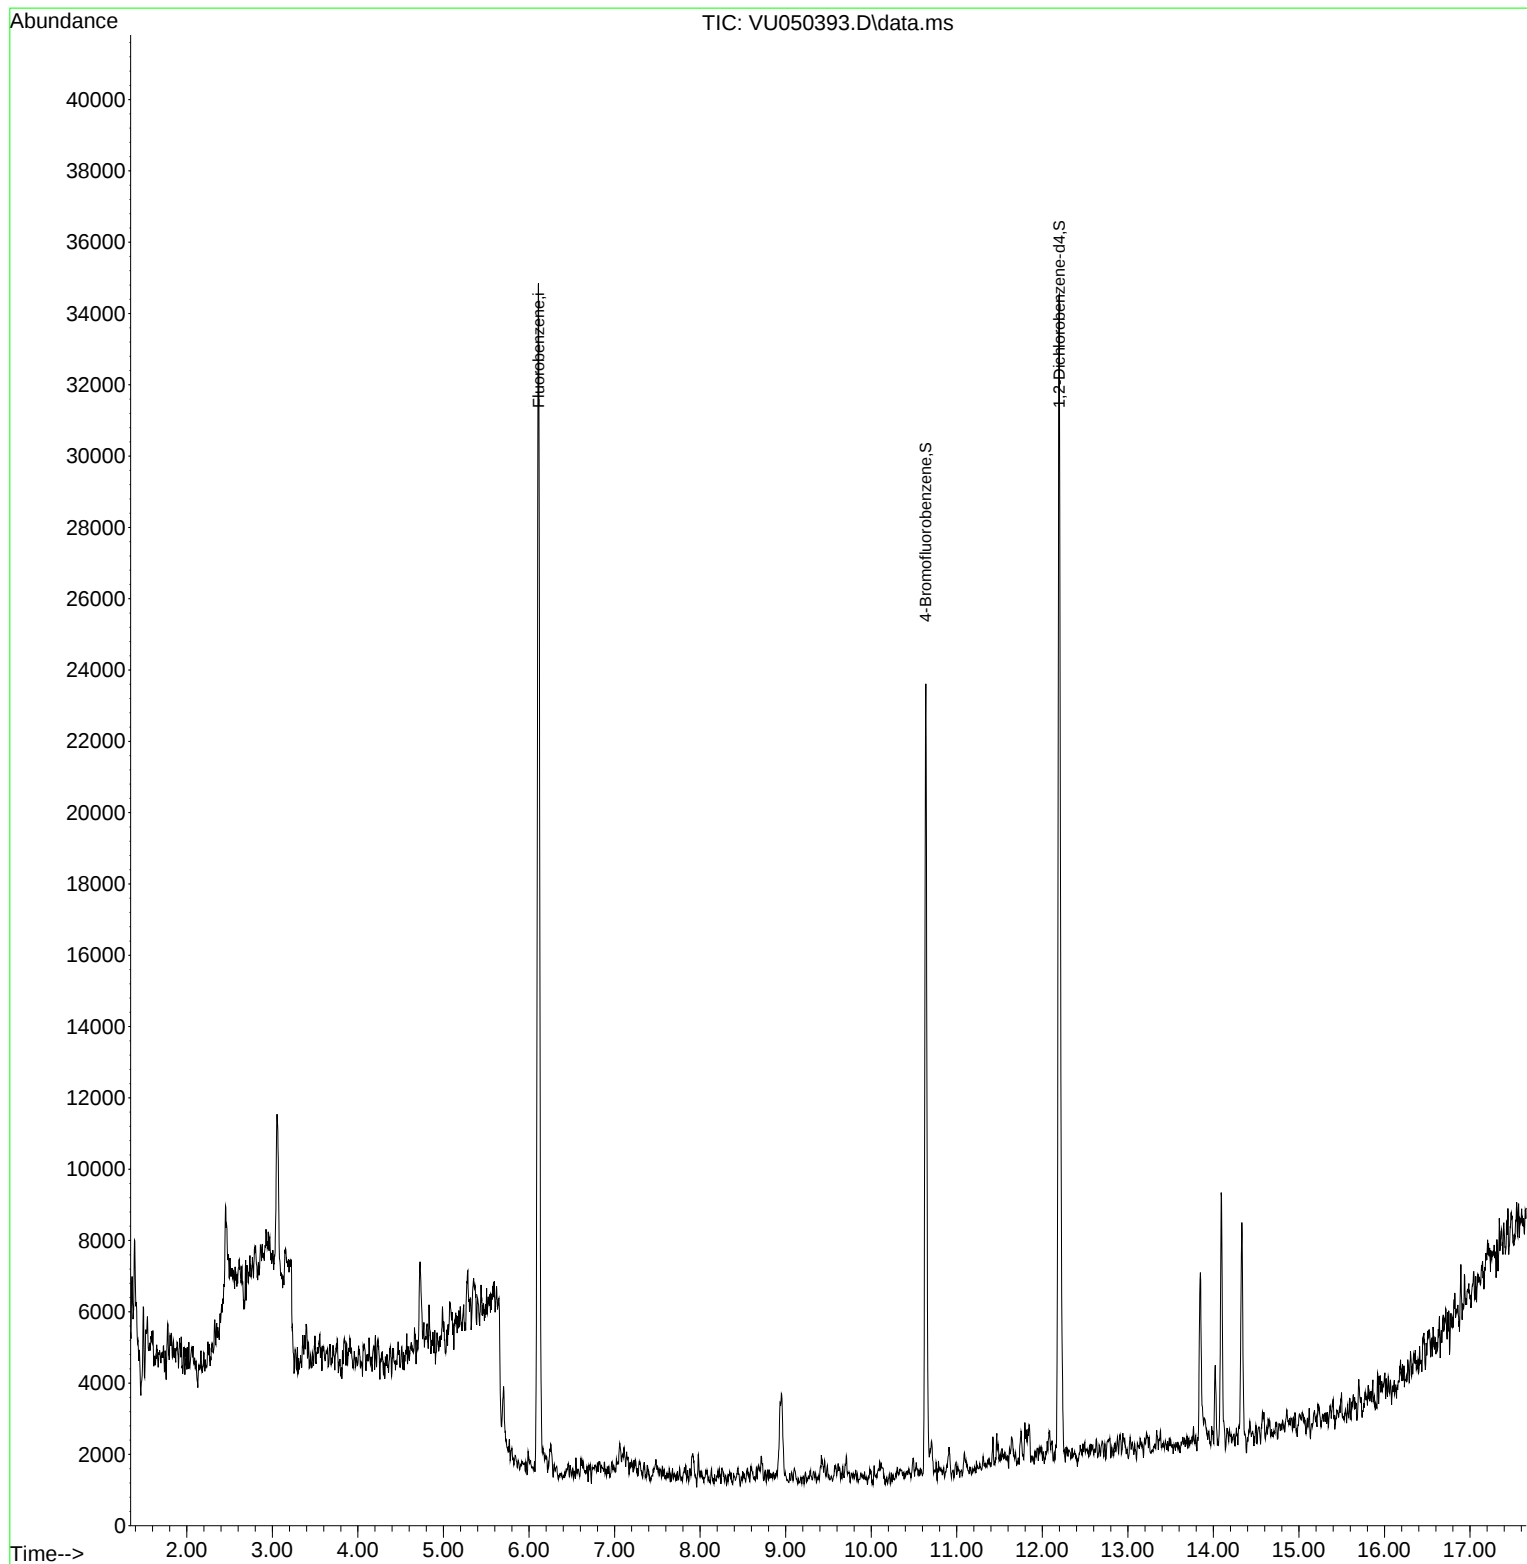


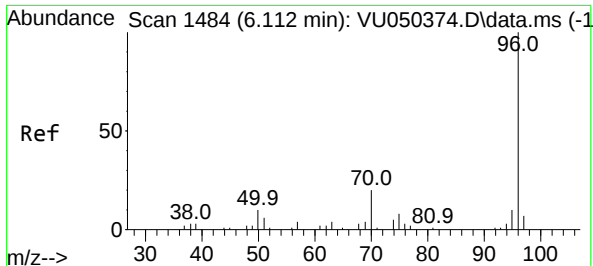

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1484
Delta R.T. -0.003 min
Lab File: VU050393.D
Acq: 22 Aug 2022 11:24




Instrument :
MSVOA_U
ClientSampleId :
VU0822WBL01


Tgt Ion: 96	Resp: 31503
Ion Ratio	Lower Upper
96 100	
70 18.9	16.7 25.1
95 9.6	7.4 11.0
97 6.6	0.0 0.0#

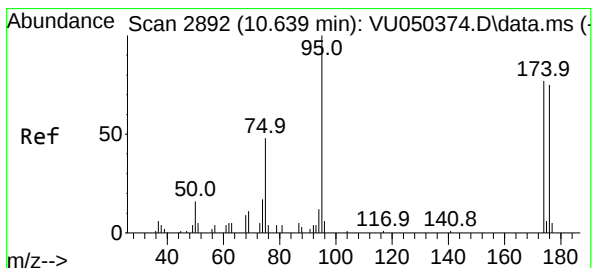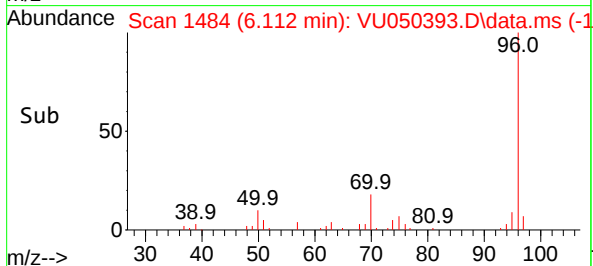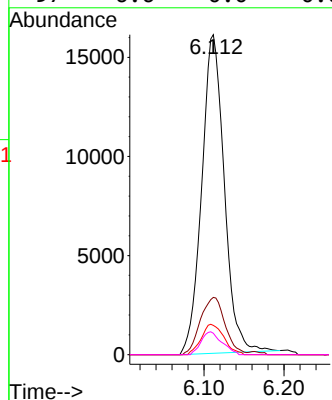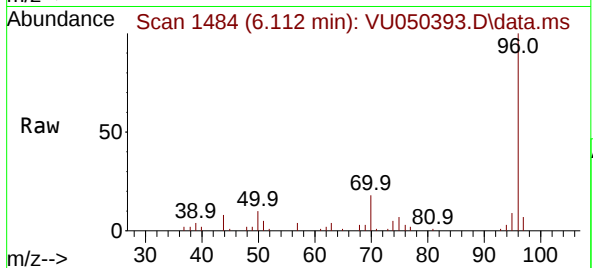

#57
4-Bromofluorobenzene
Concen: 0.753 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.007 min
Lab File: VU050393.D
Acq: 22 Aug 2022 11:24


Tgt Ion: 95	Resp: 8078
Ion Ratio	Lower Upper
95 100	
174 84.0	62.4 93.6
176 75.6	56.2 84.2

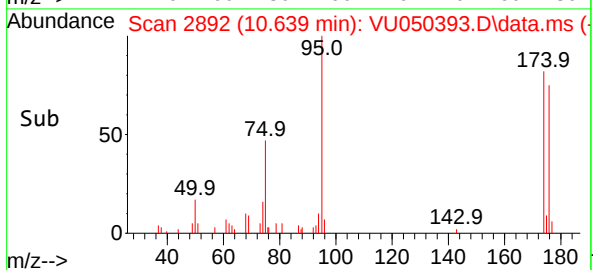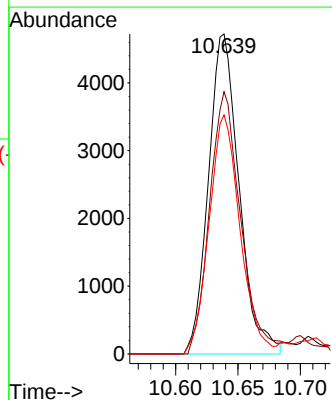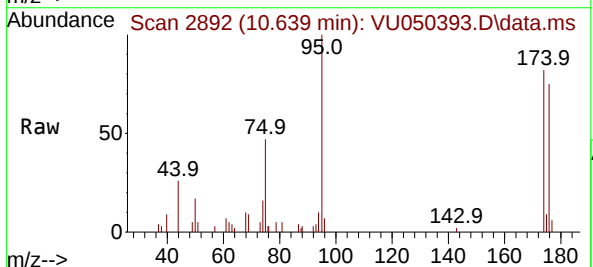

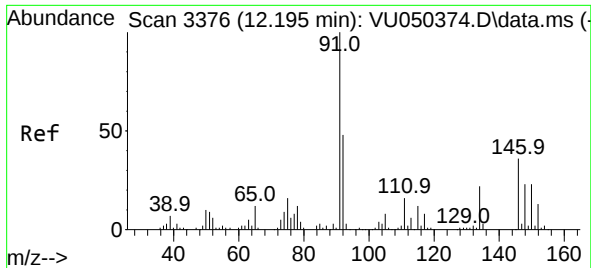

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.776 ug/l
 RT: 12.198 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU050393.D
 Acq: 22 Aug 2022 11:24

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0822WBL01

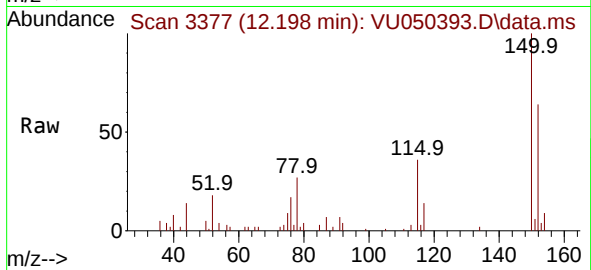

Tgt Ion:	152	Resp:	9837
Ion Ratio	Lower	Upper	
152	100		
115	62.3	0.0	254.6
150	156.5	0.0	623.6

