


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082222\
Data File : VU050391.D
Acq On : 22 Aug 2022 09:20
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Aug 23 08:18:20 2022

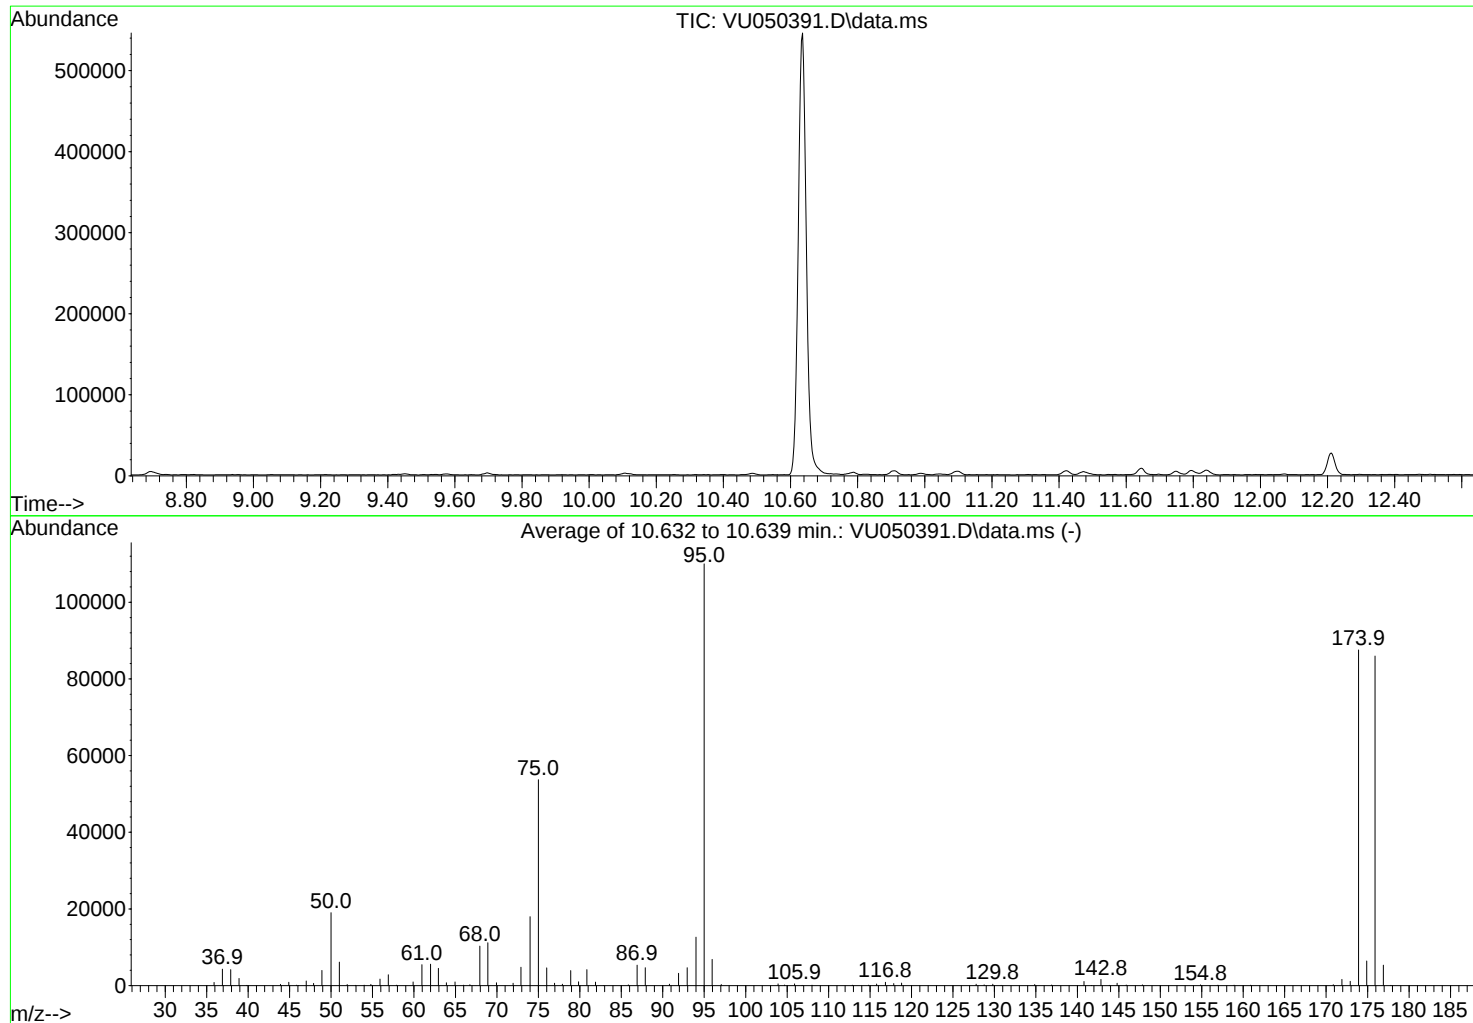

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	19032	PASS
75	95	30	60	48.8	53707	PASS
95	95	100	100	100.0	110008	PASS
96	95	5	9	6.2	6857	PASS
173	174	0.00	2	1.3	1145	PASS
174	95	50	100	79.6	87536	PASS
175	174	5	9	7.3	6423	PASS
176	174	95	101	98.2	85963	PASS
177	176	5	9	6.2	5349	PASS