

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082318\
Quantitation Report (LSC Reviewed)


Data File : VU026322.D
Acq On : 24 Aug 2018 00:28
Operator : MD/SY
Sample : J4622-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Aug 24 10:24:11 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 02:06:29 2018
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
ETBK0

Manual Integrations
APPROVED

sam
8/24/2018 2:44:15 PM

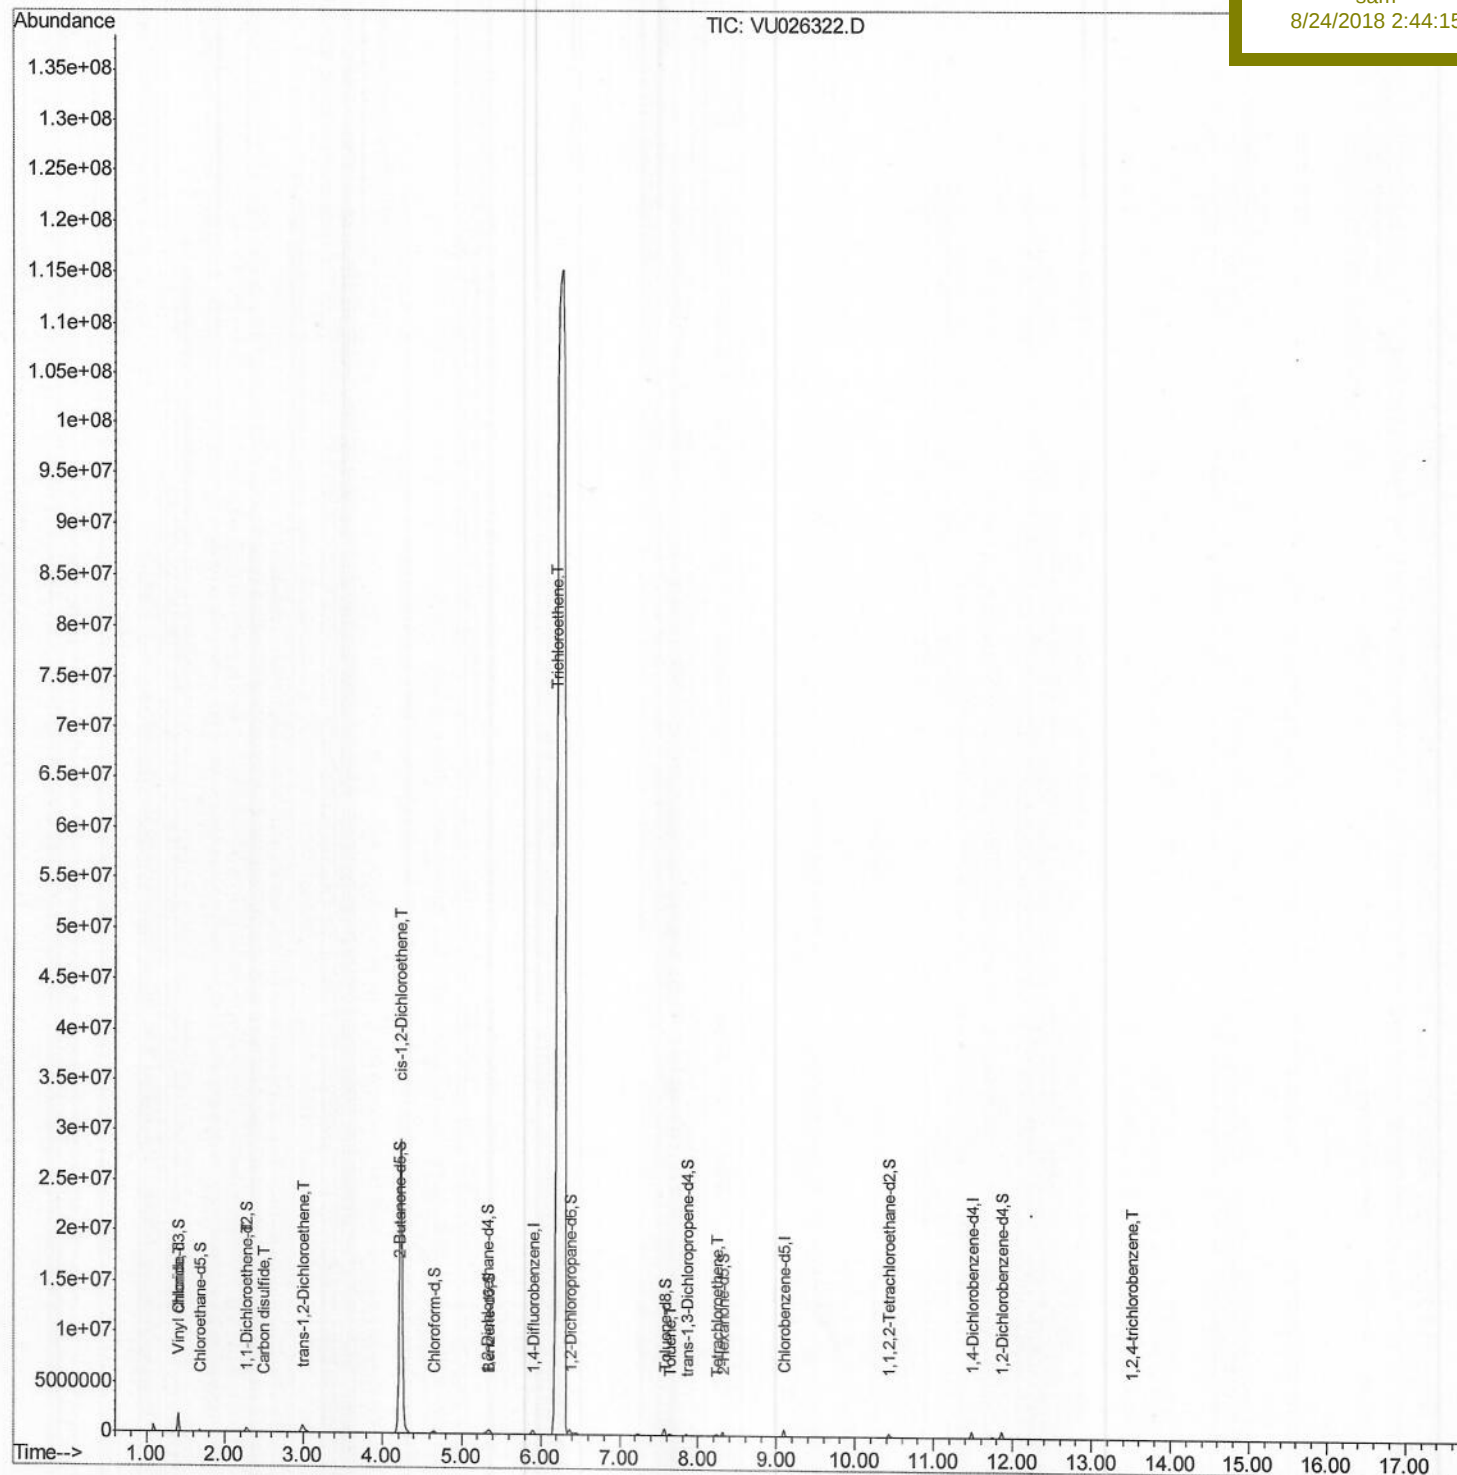

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082318\

Data File : VU026322.D

Acq On : 24 Aug 2018 00:28

Operator : MD/SY

Sample : J4622-08

Misc : 5.0mL/MSVOA U/WATER

ALS Vial : 37 Sample Multiplier: 1

Quant Time: Aug 24 02:09:27 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M

Quant Title : VOC Analysis

QLast Update : Fri Aug 24 02:06:29 2018

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :




ETBK0

Manual Integrations

APPROVED

sam

8/24/2018 2:44:15 PM

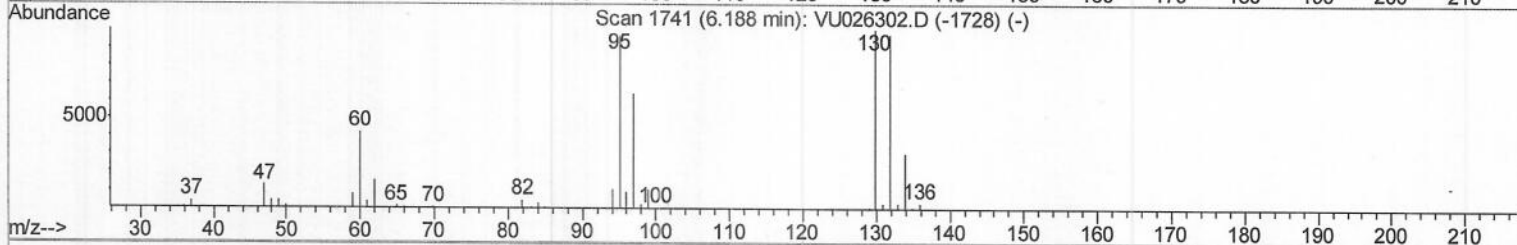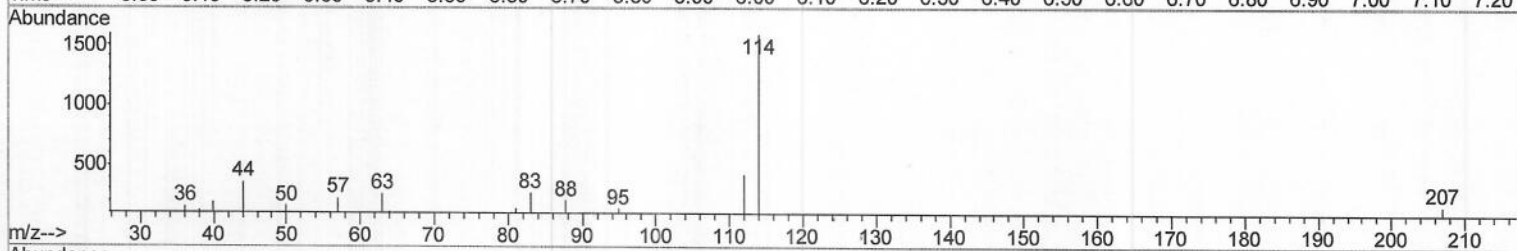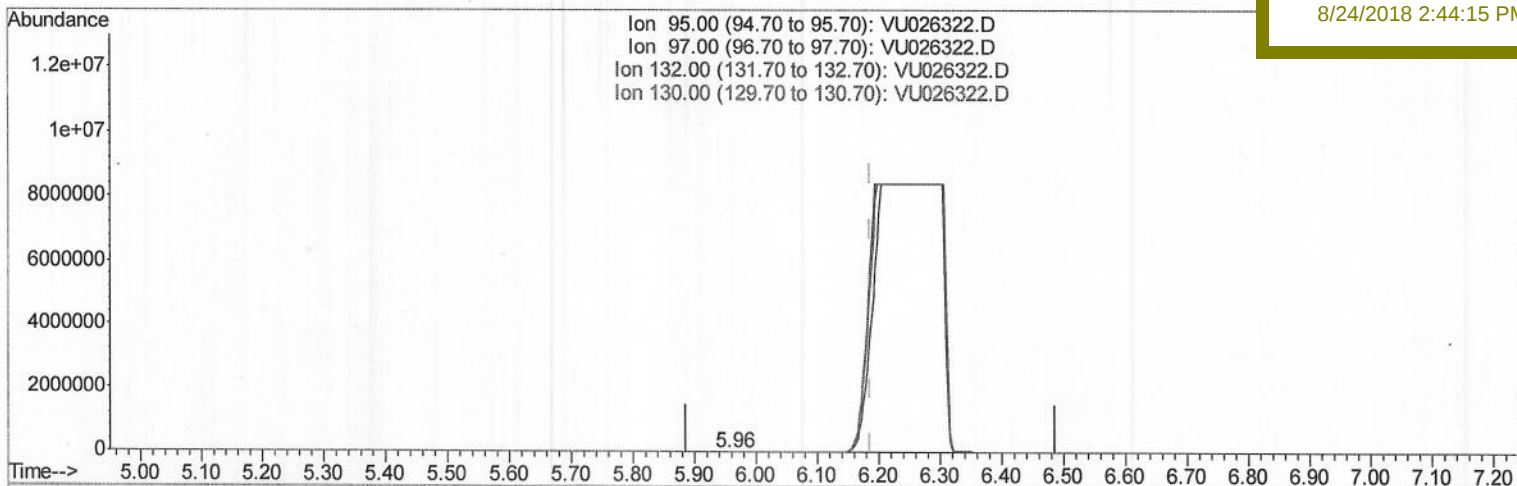

TIC: VU026322.D

(34) Trichloroethene (T)

5.957min (-0.231) 0.03ug/L

response 74

Ion	Exp%	Act%
95.00	100	100
97.00	67.40	0.00#
132.00	100.30	0.00#
130.00	104.90	0.00#

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082318\

Data File : VU026322.D

Acq On : 24 Aug 2018 00:28

Operator : MD/SY

Sample : J4622-08

Misc : 5.0mL/MSVOA U/WATER

ALS Vial : 37 Sample Multiplier: 1

Quant Time: Aug 24 02:09:27 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M

Quant Title : VOC Analysis

QLast Update : Fri Aug 24 02:06:29 2018

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :




ETBK0

Manual Integrations

APPROVED

sam

8/24/2018 2:44:15 PM

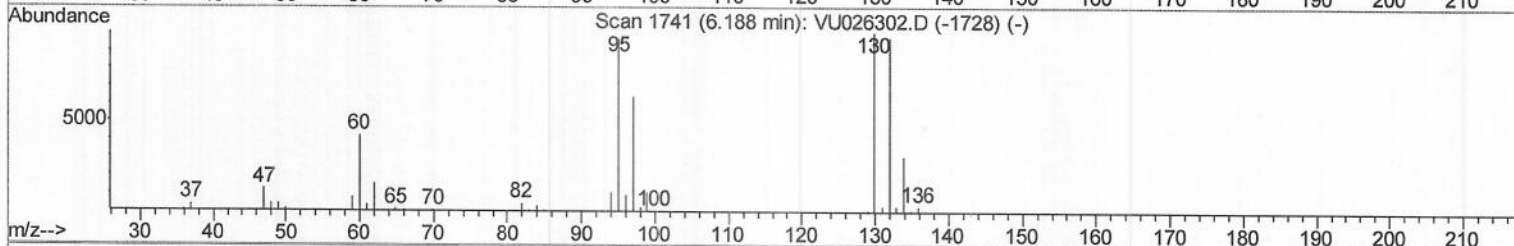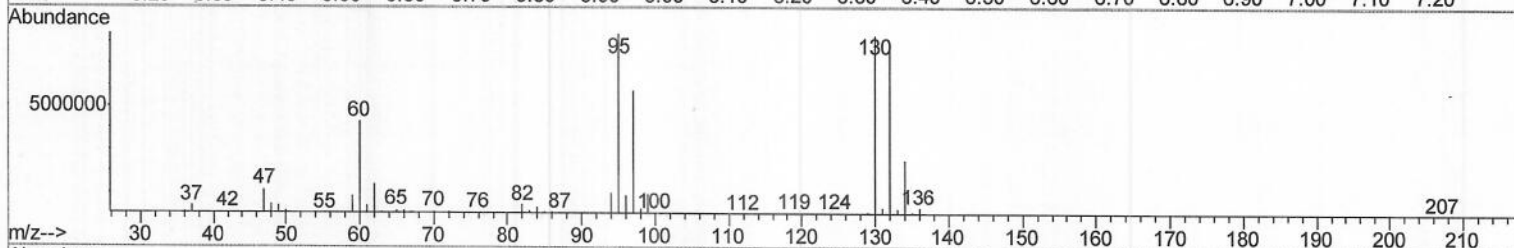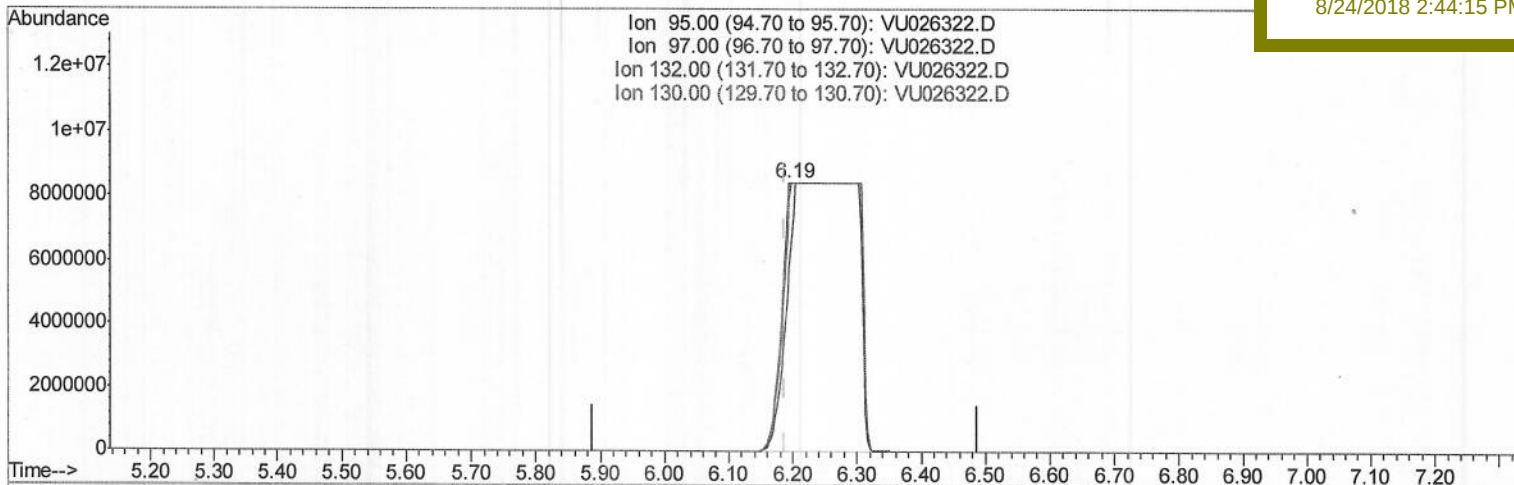

TIC: VU026322.D

(34) Trichloroethene (T)

6.194min (+0.007) 26917.31ug/L m MD 08/30/18

response 65976363

Ion	Exp%	Act%
95.00	100	100
97.00	67.40	68.49
132.00	100.30	93.75
130.00	104.90	99.13

Data File : VU026322.D
Acq On : 24 Aug 2018 00:28
Operator : MD/SY
Sample : J4622-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Aug 24 10:24:11 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 02:06:29 2018
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
ETBK0

Manual Integrations
APPROVED

sam
8/24/2018 2:44:15 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.90	114	332763	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	339999	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	173495	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	93267	45.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.90%
7) Chloroethane-d5	1.68	69	72697	43.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.84%
11) 1,1-Dichloroethene-d2	2.28	63	183617	46.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.06%
21) 2-Butanone-d5	4.20	46	157510	97.24	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.24%
24) Chloroform-d	4.65	84	201691	44.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.16%
26) 1,2-Dichloroethane-d4	5.31	65	131070	44.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.04%
32) Benzene-d6	5.35	84	404042	44.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.84%
36) 1,2-Dichloropropane-d6	6.37	67	142169	48.68	ug/L	0.03
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.36%
41) Toluene-d8	7.57	98	393103	45.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.44%
43) trans-1,3-Dichloropropene-	7.85	79	67996	45.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.12%
47) 2-Hexanone-d5	8.31	63	113710	91.10	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.10%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	186769	43.21	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.42%
64) 1,2-Dichlorobenzene-d4	11.86	152	164457	44.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.34%

Target Compounds

						Qvalue
5) Vinyl chloride	1.40	62	1077208	443.812	ug/L	96
12) 1,1-Dichloroethene	2.29	96	94152	53.758	ug/L	93
14) Carbon disulfide	2.49	76	12292	1.829	ug/L	99
17) trans-1,2-Dichloroethene	2.99	96	460709	213.412	ug/L	98
20) cis-1,2-Dichloroethene	4.23	96	17901652	7512.626	ug/L	96
34) Trichloroethene	6.19	95	65976363m)	26917.308	ug/L	
42) Toluene	7.64	91	71549	7.255	ug/L	96
46) Tetrachloroethene	8.23	164	21983	10.423	ug/L	96
68) 1,2,4-trichlorobenzene	13.51	180	17960	5.125	ug/L	97

JMD08/30/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed