

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082318\
 Data File : VU026290.D
 Acq On : 23 Aug 2018 11:58
 Operator : MD/SY
 Sample : J4598-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.613	3	7	11	rBV3	237	196	0.002%	0.0002%
2	0.818	69	71	74	rVB2	303	125	0.001%	0.0001%
3	0.834	74	76	79	rVB2	157	83	0.001%	0.0001%
4	0.899	93	96	101	rVB	359	268	0.002%	0.0003%
5	0.924	101	104	106	rBV2	279	181	0.002%	0.0002%
6	0.957	113	114	117	rBV	273	142	0.001%	0.0002%
7	0.976	117	120	125	rVV2	174	217	0.002%	0.0002%
8	1.088	146	155	172	rBV	836940	908205	84.27%	10.250%
9	1.397	245	251	261	rBV	134843	138264	12.83%	1.560%
10	1.680	332	339	354	rVB	104280	134406	12.47%	1.517%
11	2.275	513	524	535	rBV	232010	351142	32.58%	3.963%
12	2.699	653	656	658	rBV3	791	584	0.005%	0.0007%
13	2.918	721	724	726	rBV2	313	191	0.002%	0.0002%
14	3.088	769	777	781	rBV2	411	593	0.006%	0.0007%
15	3.121	784	787	793	rVV2	425	354	0.003%	0.0004%
16	3.188	806	808	811	rVB	332	141	0.001%	0.0002%
17	3.230	817	821	824	rBV2	227	203	0.002%	0.0002%
18	3.413	876	878	881	rBV	230	163	0.002%	0.0002%
19	3.449	886	889	895	rBV3	645	678	0.006%	0.0008%
20	3.522	909	912	917	rBV2	183	147	0.001%	0.0002%
21	3.606	937	938	940	rBV2	218	106	0.001%	0.0001%
22	3.641	944	949	953	rBV2	321	385	0.004%	0.0004%
23	3.706	966	969	974	rBV2	274	266	0.002%	0.0003%
24	3.773	988	990	991	rBV	181	94	0.001%	0.0001%
25	3.818	1001	1004	1007	rVB	306	220	0.002%	0.0002%
26	3.844	1007	1012	1015	rBV2	335	327	0.003%	0.0004%
27	3.860	1015	1017	1021	rVB2	496	271	0.003%	0.0003%
28	3.899	1026	1029	1031	rBV	138	97	0.001%	0.0001%
29	3.918	1031	1035	1036	rBV	187	115	0.001%	0.0001%
30	3.973	1049	1052	1058	rBV2	209	233	0.002%	0.0003%
31	4.178	1102	1116	1150	rBV	88402	246978	22.92%	2.787%
32	4.484	1210	1211	1213	rBV	197	94	0.001%	0.0001%
33	4.651	1246	1263	1286	rBV	187268	441270	40.95%	4.980%
34	4.860	1326	1328	1329	rBV	230	80	0.001%	0.0001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082318\
 Data File : VU026290.D
 Acq On : 23 Aug 2018 11:58
 Operator : MD/SY
 Sample : J4598-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

35	5.050	1382	1387	1388	rBV2	323	306	0.03%	0.003%
36	5.072	1391	1394	1397	rBV2	272	218	0.02%	0.002%
37	5.259	1448	1452	1453	rBV	557	347	0.03%	0.004%
38	5.342	1455	1478	1500	rVV2	368227	1077681	100.00%	12.163%
39	5.513	1527	1531	1534	rBV2	557	369	0.03%	0.004%
40	5.545	1539	1541	1542	rVV	118	44	0.00%	0.000%
41	5.558	1543	1545	1550	rVB2	273	157	0.01%	0.002%
42	5.767	1608	1610	1611	rBV2	124	49	0.00%	0.001%
43	5.783	1611	1615	1616	rBV	228	116	0.01%	0.001%
44	5.889	1633	1648	1673	rBV	328847	642015	59.57%	7.246%
45	6.095	1710	1712	1715	rBV	194	139	0.01%	0.002%
46	6.185	1737	1740	1747	rVB4	646	451	0.04%	0.005%
47	6.223	1750	1752	1755	rVV3	551	222	0.02%	0.003%
48	6.333	1770	1786	1806	rBV	245826	490108	45.48%	5.531%
49	6.487	1832	1834	1837	rVB	352	159	0.01%	0.002%
50	6.503	1837	1839	1841	rBV	302	134	0.01%	0.002%
51	6.532	1846	1848	1853	rBV3	317	323	0.03%	0.004%
52	6.596	1866	1868	1870	rVB	200	109	0.01%	0.001%
53	6.616	1870	1874	1879	rBV2	354	316	0.03%	0.004%
54	6.654	1883	1886	1887	rBV	156	98	0.01%	0.001%
55	6.786	1925	1927	1928	rBV	184	85	0.01%	0.001%
56	6.825	1933	1939	1942	rBV3	1115	1419	0.13%	0.016%
57	6.895	1959	1961	1963	rBV	280	168	0.02%	0.002%
58	6.911	1963	1966	1971	rVV4	737	728	0.07%	0.008%
59	6.937	1971	1974	1977	rVB2	227	119	0.01%	0.001%
60	6.950	1977	1978	1980	rVB2	102	34	0.00%	0.000%
61	6.963	1980	1982	1984	rBV	132	57	0.01%	0.001%
62	6.976	1984	1986	1987	rBV	186	56	0.01%	0.001%
63	7.072	2012	2016	2020	rBV2	453	397	0.04%	0.004%
64	7.136	2034	2036	2041	rBV2	222	193	0.02%	0.002%
65	7.169	2041	2046	2049	rBV2	456	387	0.04%	0.004%
66	7.230	2053	2065	2090	rBV	141416	250369	23.23%	2.826%
67	7.432	2122	2128	2129	rBV3	1238	1030	0.10%	0.012%
68	7.497	2146	2148	2155	rBV3	299	289	0.03%	0.003%
69	7.567	2156	2170	2190	rBV	497356	862596	80.04%	9.735%
70	7.763	2226	2231	2233	rBV3	459	438	0.04%	0.005%
71	7.850	2247	2258	2277	rBV	101516	173267	16.08%	1.956%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082318\
 Data File : VU026290.D
 Acq On : 23 Aug 2018 11:58
 Operator : MD/SY
 Sample : J4598-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

72	8.188	2349	2363	2371	rBV	64528	155222	14.40%	1.752%
73	8.554	2475	2477	2480	rBV2	283	188	0.02%	0.002%
74	8.747	2534	2537	2540	rVB2	442	213	0.02%	0.002%
75	8.773	2541	2545	2551	rBV3	474	631	0.06%	0.007%
76	8.866	2572	2574	2578	rBV2	299	257	0.02%	0.003%
77	8.895	2578	2583	2585	rBV	431	413	0.04%	0.005%
78	8.956	2598	2602	2605	rBV2	360	364	0.03%	0.004%
79	9.091	2631	2644	2670	rBV	489931	792709	73.56%	8.947%
80	9.255	2689	2695	2698	rBV4	630	793	0.07%	0.009%
81	9.323	2714	2716	2718	rBV2	218	132	0.01%	0.001%
82	9.374	2728	2732	2739	rBV6	535	775	0.07%	0.009%
83	9.538	2781	2783	2786	rBV2	217	143	0.01%	0.002%
84	9.670	2822	2824	2825	rBV	288	119	0.01%	0.001%
85	9.950	2908	2911	2912	rBV2	474	228	0.02%	0.003%
86	10.014	2929	2931	2933	rBV	346	221	0.02%	0.002%
87	10.146	2969	2972	2974	rBV2	423	301	0.03%	0.003%
88	10.435	3050	3062	3083	rVB	338360	535074	49.65%	6.039%
89	10.619	3106	3119	3134	rBV2	25708	54007	5.01%	0.610%
90	10.802	3173	3176	3180	rBV2	313	274	0.03%	0.003%
91	10.873	3193	3198	3207	rBV3	800	1184	0.11%	0.013%
92	11.487	3376	3389	3406	rBV	469330	740544	68.72%	8.358%
93	11.738	3465	3467	3468	rBV	417	146	0.01%	0.002%
94	11.860	3493	3505	3530	rVB	511224	820651	76.15%	9.262%
95	12.483	3688	3699	3711	rBV2	7571	13561	1.26%	0.153%
96	14.278	4249	4257	4270	rVB2	6130	10398	0.96%	0.117%


Sum of corrected areas: 8860360

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082318\
Data File : VU026290.D
Acq On : 23 Aug 2018 11:58
Operator : MD/SY
Sample : J4598-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
ETBM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

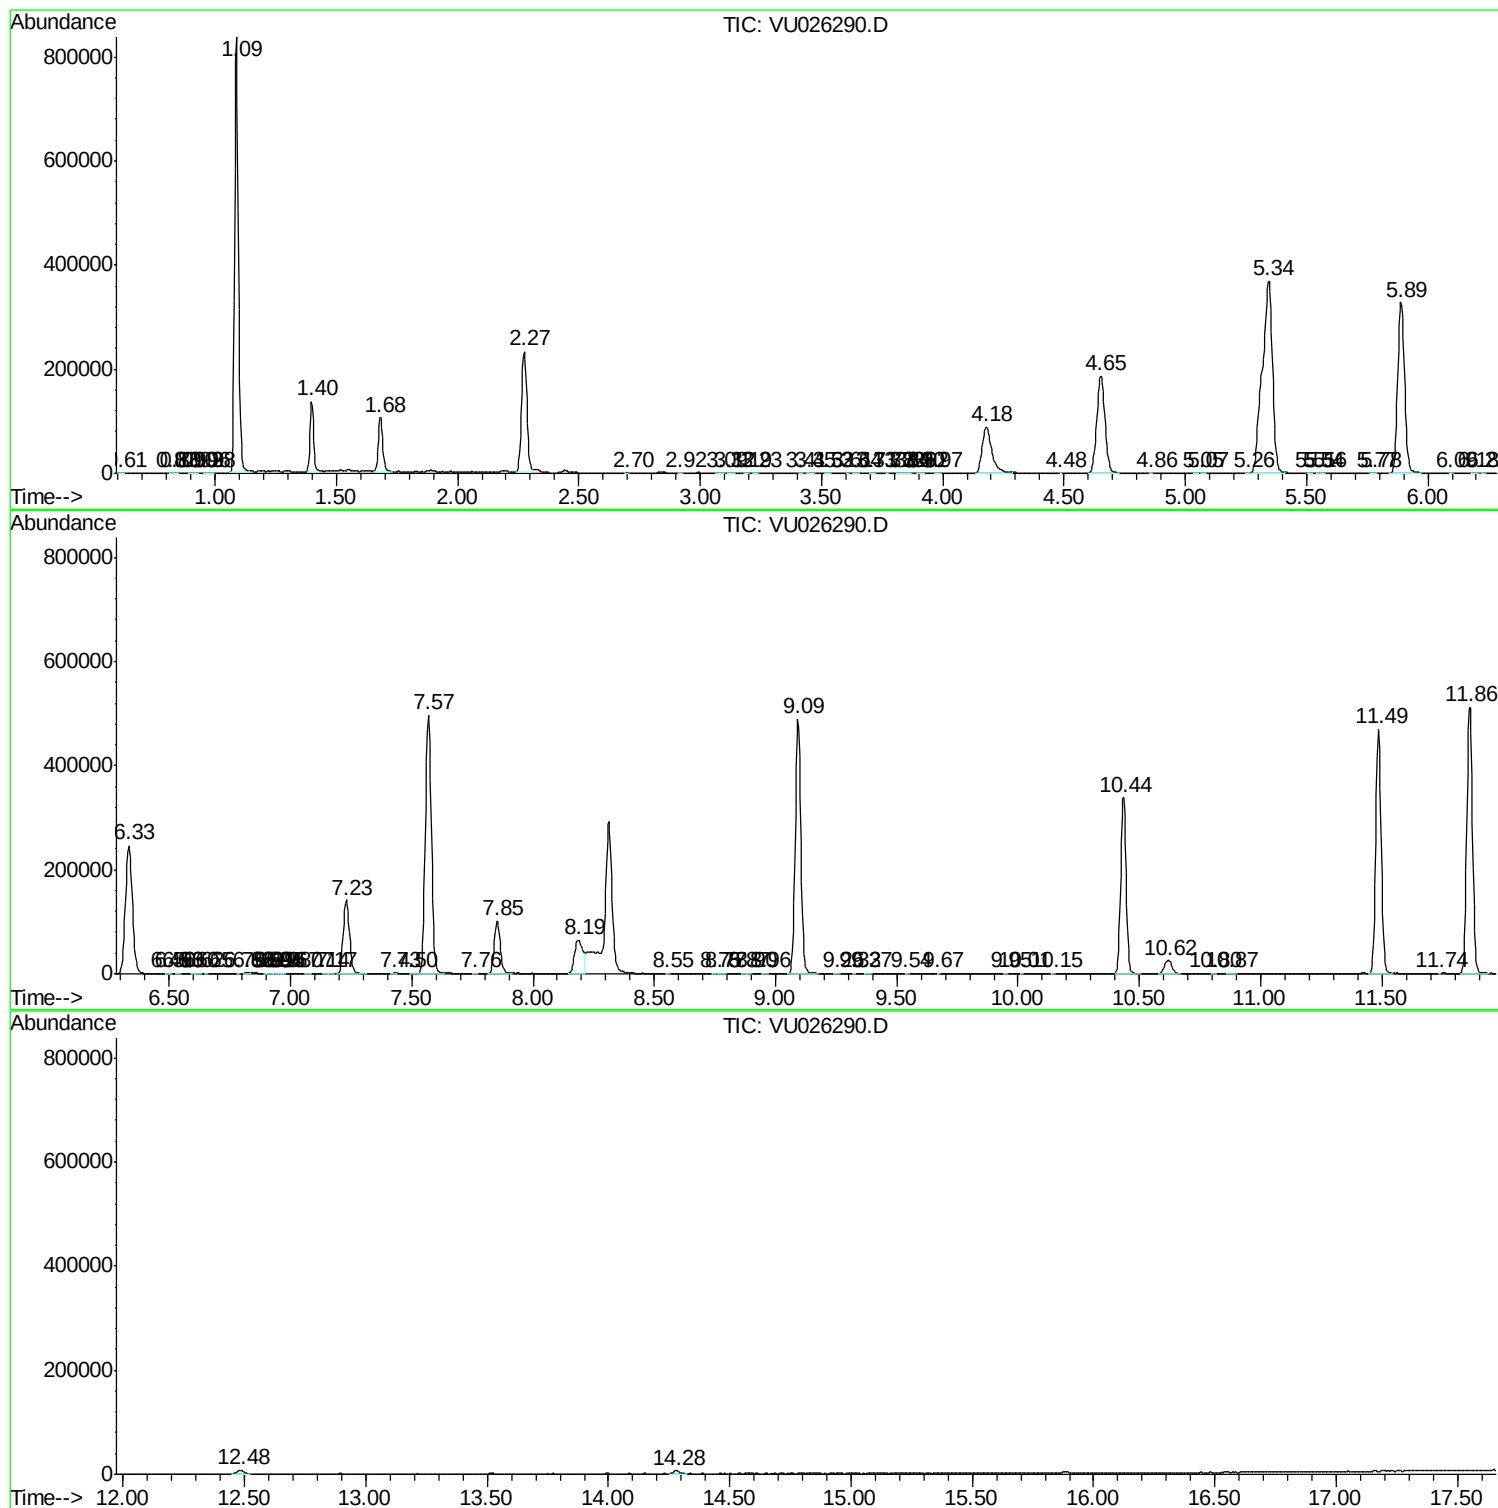

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082318\
Data File : VU026290.D
Acq On : 23 Aug 2018 11:58
Operator : MD/SY
Sample : J4598-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082318\
Data File : VU026290.D
Acq On : 23 Aug 2018 11:58
Operator : MD/SY
Sample : J4598-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc