


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082318\
Data File : VU026286.D
Acq On : 23 Aug 2018 08:21
Operator : MD/SY
Sample : BFB41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Title : VOC Analysis
Last Update : Fri Aug 24 02:06:29 2018

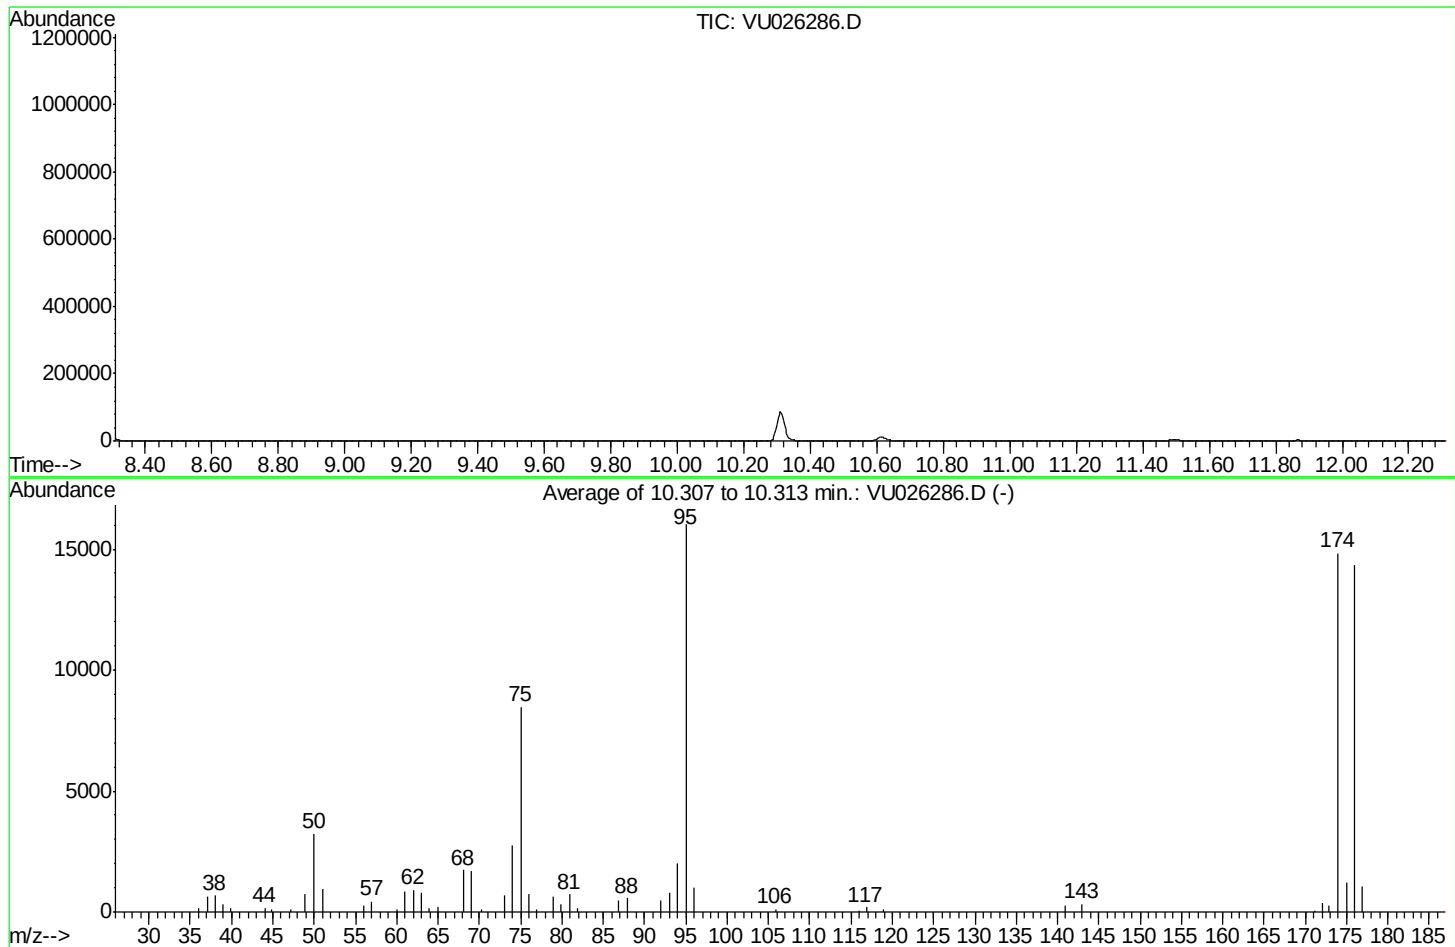

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	3239	PASS
75	95	30	80	53.0	8493	PASS
95	95	100	100	100.0	16026	PASS
96	95	5	9	6.2	988	PASS
173	174	0.00	2	1.7	257	PASS
174	95	50	120	92.6	14843	PASS
175	174	5	9	8.1	1204	PASS
176	174	95	101	96.6	14335	PASS
177	176	5	9	7.2	1039	PASS

m/z	Abundance
44.00	344.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	166.0
37.10	653.0
38.00	584.0
38.90	316.0
39.90	105.0
44.00	535.0
44.90	131.0
47.20	140.0
48.90	665.0
50.00	3250.0
51.00	924.0
56.10	229.0
56.90	467.0
60.10	119.0
61.00	860.0
62.00	953.0
63.00	772.0
64.00	172.0
65.00	185.0
68.10	1652.0
69.00	1686.0
73.00	666.0
74.10	2668.0
75.00	8250.0
76.10	794.0
76.80	116.0
79.00	624.0
80.00	331.0
81.00	735.0
81.90	147.0
86.90	504.0
87.90	691.0
92.00	408.0
93.00	719.0
94.00	1907.0
95.00	15232.0
96.00	949.0
105.90	141.0
115.90	112.0
116.90	150.0
118.90	128.0
140.90	169.0
143.00	309.0
172.10	286.0
172.90	280.0
174.00	14373.0
175.00	1137.0
176.00	13789.0
176.90	1020.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	162.0
37.00	683.0
38.00	695.0
38.90	304.0
40.00	138.0
44.00	511.0
44.90	127.0
47.20	134.0
49.00	778.0
50.00	3338.0
51.10	950.0
56.10	279.0
57.00	471.0
60.10	121.0
61.00	842.0
62.00	940.0
63.00	805.0
63.90	171.0
65.00	202.0
68.00	1769.0
69.00	1757.0
70.20	114.0
73.00	754.0
74.00	2811.0
75.10	8743.0
76.10	767.0
76.90	126.0
79.00	663.0
79.90	329.0
80.90	747.0
81.90	169.0
86.80	499.0
87.90	594.0
92.00	494.0
93.00	811.0
94.00	2110.0
95.00	16472.0
96.00	1031.0
105.90	120.0
115.90	122.0
116.90	209.0
118.90	131.0
140.80	257.0
143.00	333.0
172.00	357.0
172.90	276.0
174.00	15283.0
175.00	1238.0
176.00	14912.0
176.90	1047.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	143.0
37.00	645.0
38.00	764.0
39.00	278.0
40.00	165.0
44.00	519.0
44.90	113.0
47.10	118.0
49.00	796.0
50.00	3129.0
51.10	985.0
56.00	256.0
57.00	403.0
60.00	114.0
61.00	811.0
62.00	830.0
63.00	863.0
63.80	137.0
65.00	209.0
68.00	1751.0
69.00	1650.0
70.20	132.0
73.00	718.0
74.00	2805.0
75.10	8488.0
76.00	665.0
76.90	136.0
79.00	587.0
79.80	313.0
80.90	719.0
81.90	133.0
86.90	460.0
87.90	444.0
92.00	527.0
93.00	846.0
94.00	2096.0
95.00	16374.0
96.00	984.0
105.90	104.0
116.90	269.0
118.90	127.0
140.80	321.0
143.00	331.0
171.10	108.0
172.00	398.0
172.90	215.0
174.00	14873.0
175.00	1239.0
176.00	14306.0
177.00	1050.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41