


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082319\
 Data File : VU033931.D
 Acq On : 23 Aug 2019 10:14
 Operator : JC/SP
 Sample : BFB31
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB31

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082219WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 26 06:54:44 2019

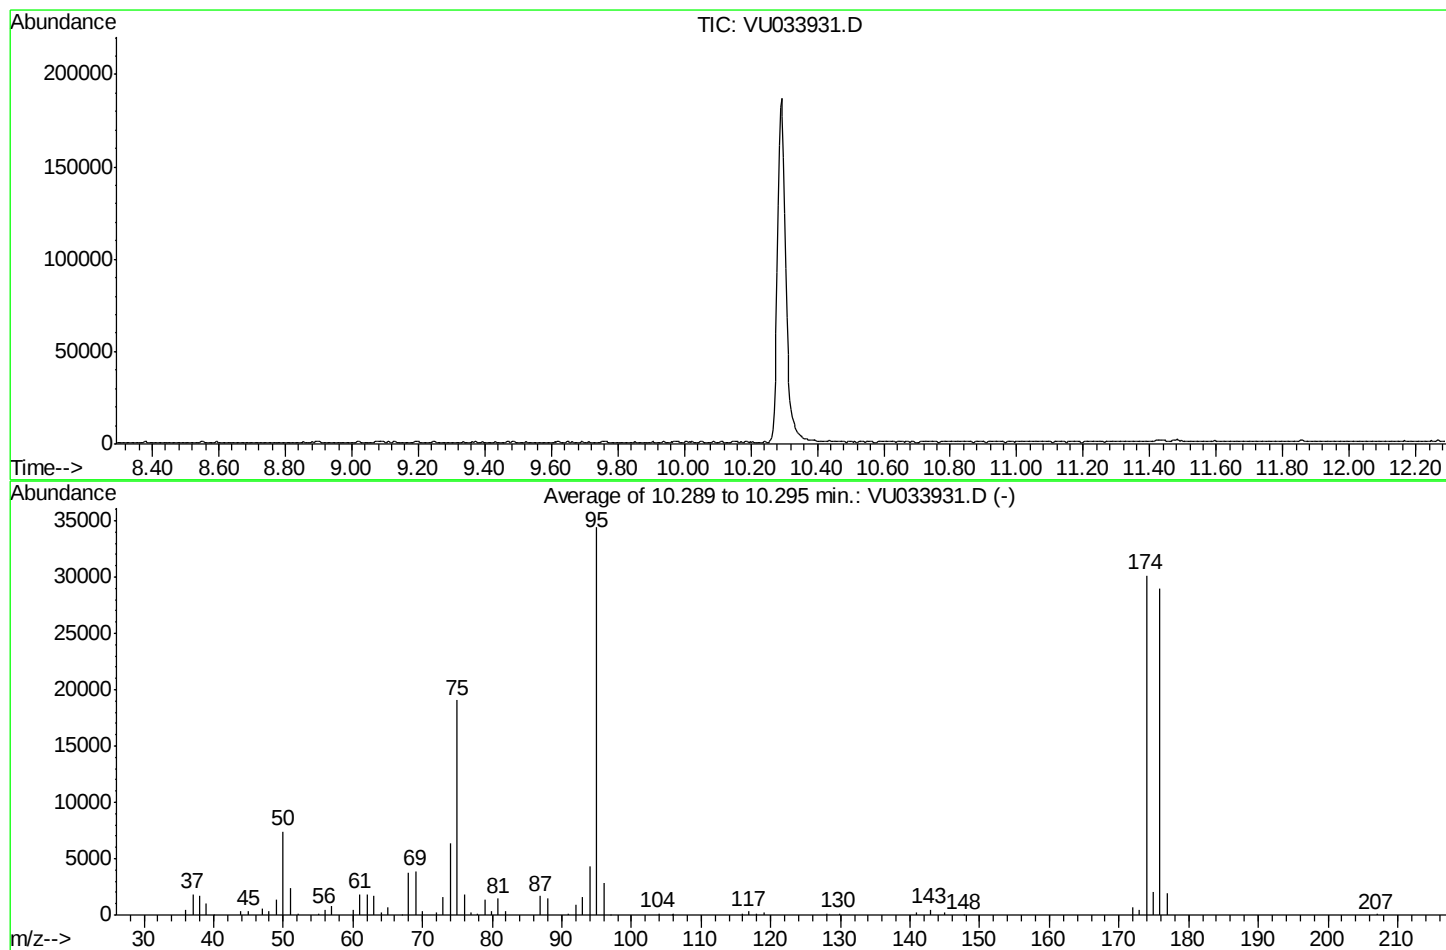

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	7431	PASS
75	95	30	80	55.3	19045	PASS
95	95	100	100	100.0	34413	PASS
96	95	5	9	8.3	2866	PASS
173	174	0.00	2	1.7	507	PASS
174	95	50	120	87.6	30141	PASS
175	174	5	9	6.9	2072	PASS
176	174	95	101	96.2	28992	PASS
177	176	5	9	6.7	1949	PASS

m/z	Abundance
36.10	443.0
37.00	1813.0
38.00	1757.0
39.00	948.0
39.90	289.0
44.00	861.0
45.00	377.0
47.00	577.0
48.00	312.0
49.00	1457.0
50.00	7590.0
51.00	2423.0
52.10	126.0
55.00	110.0
56.00	573.0
57.00	906.0
60.00	555.0
61.00	1913.0
62.00	1775.0
63.00	1680.0
64.00	262.0
65.00	658.0
67.00	110.0
68.00	3713.0
69.00	4108.0
70.00	322.0
72.00	290.0
73.00	1701.0
74.00	6603.0
75.00	19544.0
76.00	1727.0
76.90	188.0
78.00	116.0
78.90	1262.0
80.00	295.0
80.90	1486.0
81.90	258.0
86.90	1735.0
88.00	1521.0
91.90	956.0
92.90	1655.0
94.00	4463.0
95.00	34096.0
96.00	2955.0
97.00	103.0
103.90	139.0
106.00	178.0
115.90	164.0
116.90	350.0
119.10	262.0
128.10	132.0
129.80	156.0
140.90	267.0
142.90	540.0
144.90	261.0
147.80	134.0
171.90	708.0
172.90	461.0
173.90	29096.0
174.90	2087.0
175.90	28424.0
176.90	1840.0
207.00	193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	411.0
37.00	1884.0
38.00	1724.0
39.00	1042.0
40.00	349.0
44.00	974.0
45.00	380.0
47.00	607.0
47.90	345.0
49.00	1435.0
50.00	7625.0
51.00	2410.0
52.00	139.0
55.00	133.0
56.00	522.0
57.00	844.0
60.00	493.0
61.00	1923.0
62.00	1827.0
63.00	1721.0
64.00	261.0
65.00	766.0
68.00	3853.0
69.00	4055.0
70.00	409.0
72.00	279.0
73.00	1574.0
74.00	6598.0
75.00	19696.0
76.00	1859.0
76.90	193.0
77.90	145.0
78.90	1342.0
79.90	296.0
80.90	1517.0
82.00	321.0
86.90	1675.0
87.90	1456.0
90.90	121.0
91.90	937.0
93.00	1635.0
94.00	4359.0
95.00	35296.0
96.00	2960.0
103.90	120.0
106.10	146.0
115.90	132.0
116.90	331.0
117.90	130.0
119.10	252.0
128.10	150.0
129.80	169.0
140.90	235.0
142.90	517.0
144.90	262.0
172.00	730.0
172.90	508.0
173.90	30864.0
175.00	2099.0
175.90	29984.0
176.90	2034.0
207.00	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	425.0
37.00	1819.0
38.00	1596.0
39.00	1015.0
40.00	379.0
44.00	1044.0
45.00	342.0
47.00	550.0
47.90	329.0
49.00	1373.0
50.00	7078.0
51.00	2188.0
52.00	129.0
55.00	119.0
56.00	435.0
56.90	752.0
60.00	396.0
61.00	1754.0
62.00	1828.0
63.00	1601.0
64.00	269.0
65.00	777.0
68.00	3653.0
69.00	3581.0
70.00	437.0
72.00	204.0
73.00	1377.0
74.00	5872.0
75.00	17896.0
76.00	1778.0
76.90	208.0
77.80	168.0
78.90	1368.0
79.90	304.0
80.90	1430.0
82.00	343.0
87.00	1578.0
87.90	1308.0
90.90	178.0
92.00	985.0
93.00	1548.0
94.00	4101.0
95.00	33848.0
96.00	2683.0
103.90	124.0
105.80	123.0
116.90	281.0
117.90	159.0
119.00	206.0
128.10	114.0
129.90	142.0
140.80	242.0
142.80	480.0
145.00	202.0
172.00	707.0
173.00	553.0
173.90	30464.0
175.00	2032.0
175.90	28568.0
176.90	1975.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Scan 2850 (10.254 min): VU033931.D
BFB31

m/z	Abundance
40.00	338.0
43.90	670.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31