

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
 Data File : VU044504.D
 Acq On : 23 Aug 2021 15:53
 Operator : SY/MD
 Sample : M3519-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG9

Quant Time: Aug 24 04:00:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 24 03:56:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	119573	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	119526	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	54392	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	40169	4.154	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.000%
7) Chloroethane-d5	1.916	69	38589	4.591	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.800%
11) 1,1-Dichloroethene-d2	2.571	65	18150	4.412	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.200%
20) 2-Butanone-d5	4.639	46	137240	51.313	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.620%
24) Chloroform-d	5.073	84	80587	4.713	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
26) 1,2-Dichloroethane-d4	5.710	65	45916	4.924	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	5.735	84	162420	4.826	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%
36) 1,2-Dichloropropane-d6	6.697	67	54047	5.019	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.906	98	136141	4.562	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	8.185	79	17719	4.582	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.600%
46) 2-Hexanone-d5	8.642	63	110999	53.081	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.160%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	42760	4.715	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.400%
66) 1,2-Dichlorobenzene-d4	12.198	152	47430	5.161	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%
Target Compounds						
13) Acetone	2.645	43	3060	1.378	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044504.D
Acq On : 23 Aug 2021 15:53
Operator : SY/MD
Sample : M3519-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG9


Quant Time: Aug 24 04:00:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 24 03:56:17 2021
Response via : Initial Calibration

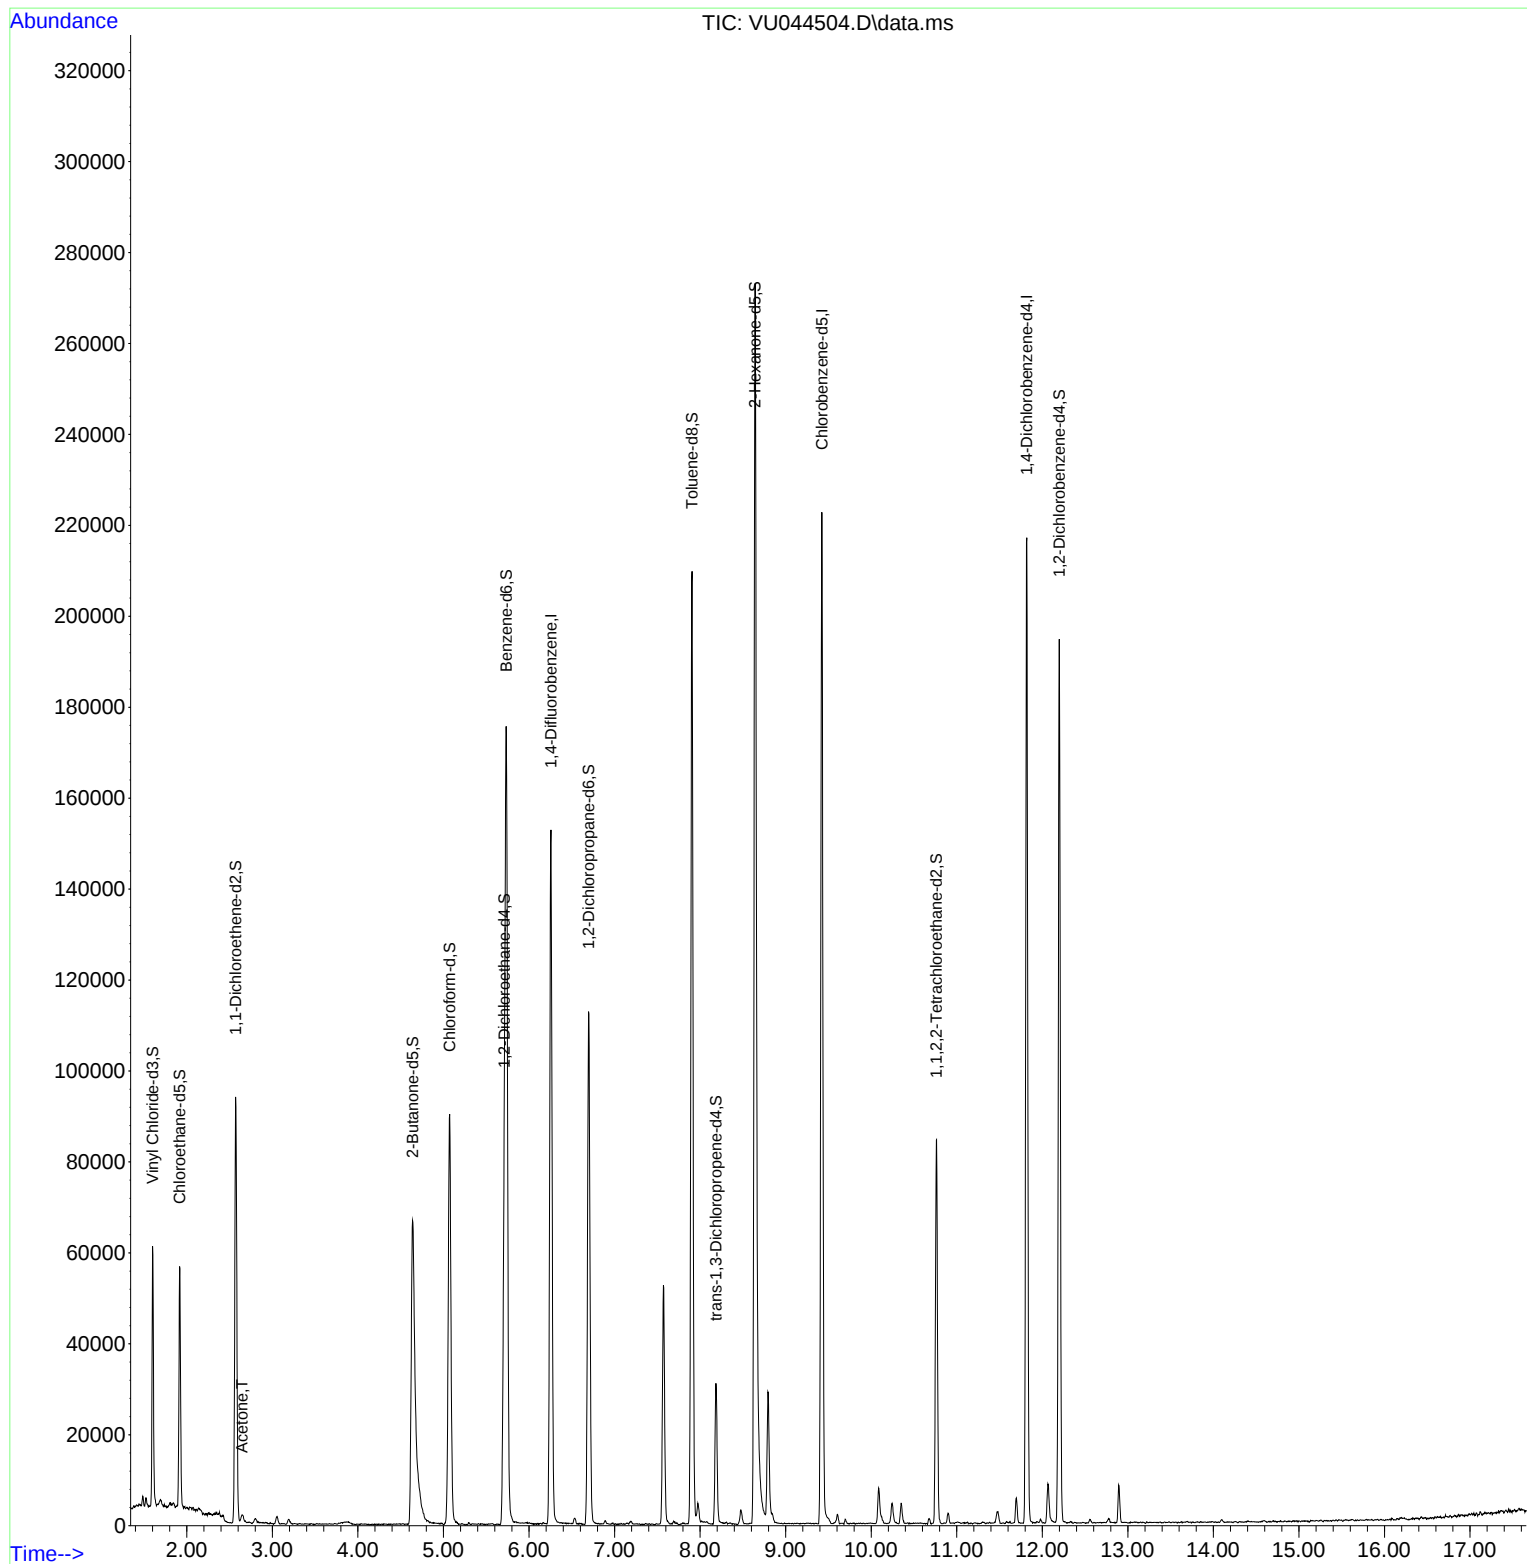

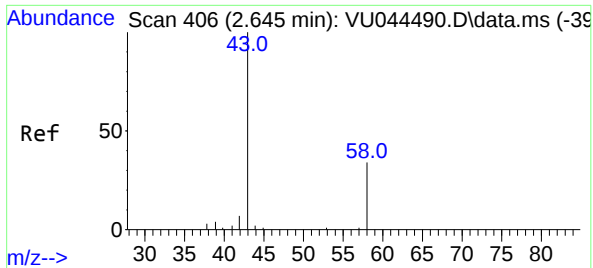

#13
 Acetone
 Concen: 1.378 ug/L
 RT: 2.645 min Scan# 406
 Delta R.T. 0.000 min
 Lab File: VU044504.D
 Acq: 23 Aug 2021 15:53

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG9

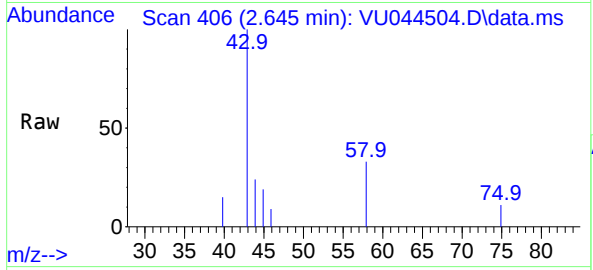

Tgt Ion: 43 Resp: 3060

Ion	Ratio	Lower	Upper
43	100		
58	22.5	0.0	45.4

