

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
 Data File : VU044499.D
 Acq On : 23 Aug 2021 13:52
 Operator : SY/MD
 Sample : M3515-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4558

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	10	17	26	rBV	88198	92709	13.53%	1.953%
2	1.523	50	57	66	rVB	25742	29782	4.35%	0.627%
3	1.601	74	81	90	rBV	52358	59764	8.72%	1.259%
4	1.916	172	179	192	rVB	50546	66548	9.71%	1.402%
5	2.572	372	383	397	rBV	90811	149265	21.78%	3.144%
6	3.372	617	632	660	rBV	37670	90154	13.16%	1.899%
7	4.639	1011	1026	1085	rBV	59816	227867	33.25%	4.799%
8	5.070	1145	1160	1182	rBV	83633	190357	27.78%	4.009%
9	5.732	1343	1366	1393	rBV2	168685	445350	64.99%	9.380%
10	6.256	1514	1529	1551	rBV	144360	276245	40.31%	5.818%
11	6.549	1605	1620	1637	rVB2	40111	74951	10.94%	1.579%
12	6.697	1653	1666	1692	rBV	107182	212738	31.05%	4.481%
13	7.571	1920	1938	1957	rBV	50248	89745	13.10%	1.890%
14	7.906	2028	2042	2056	rBV	203000	352455	51.44%	7.424%
15	8.186	2119	2129	2146	rBV	30672	51373	7.50%	1.082%
16	8.558	2232	2245	2259	rBV	404854	685227	100.00%	14.433%
17	8.645	2260	2272	2304	rVB	260227	538534	78.59%	11.343%
18	9.423	2501	2514	2532	rBV	217718	357039	52.11%	7.520%
19	10.761	2917	2930	2947	rBV	84253	135610	19.79%	2.856%
20	11.819	3246	3259	3275	rBV	203185	326917	47.71%	6.886%
21	12.198	3365	3377	3394	rBV	182125	295115	43.07%	6.216%




Sum of corrected areas: 4747745

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044499.D
Acq On : 23 Aug 2021 13:52
Operator : SY/MD
Sample : M3515-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4558

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

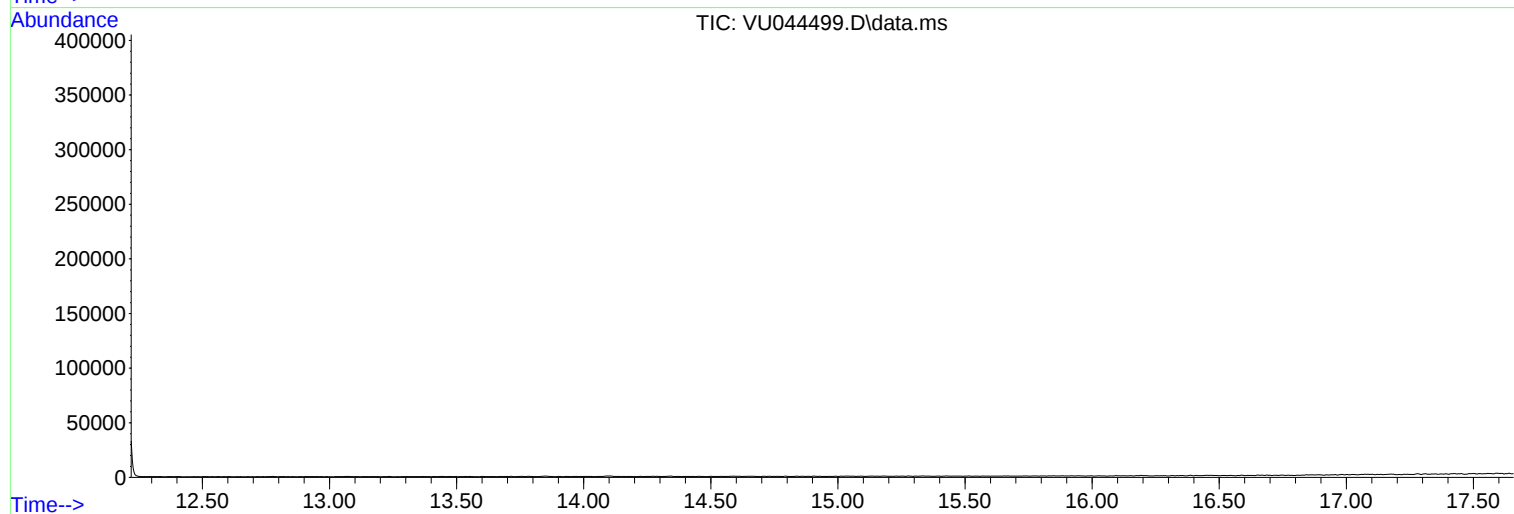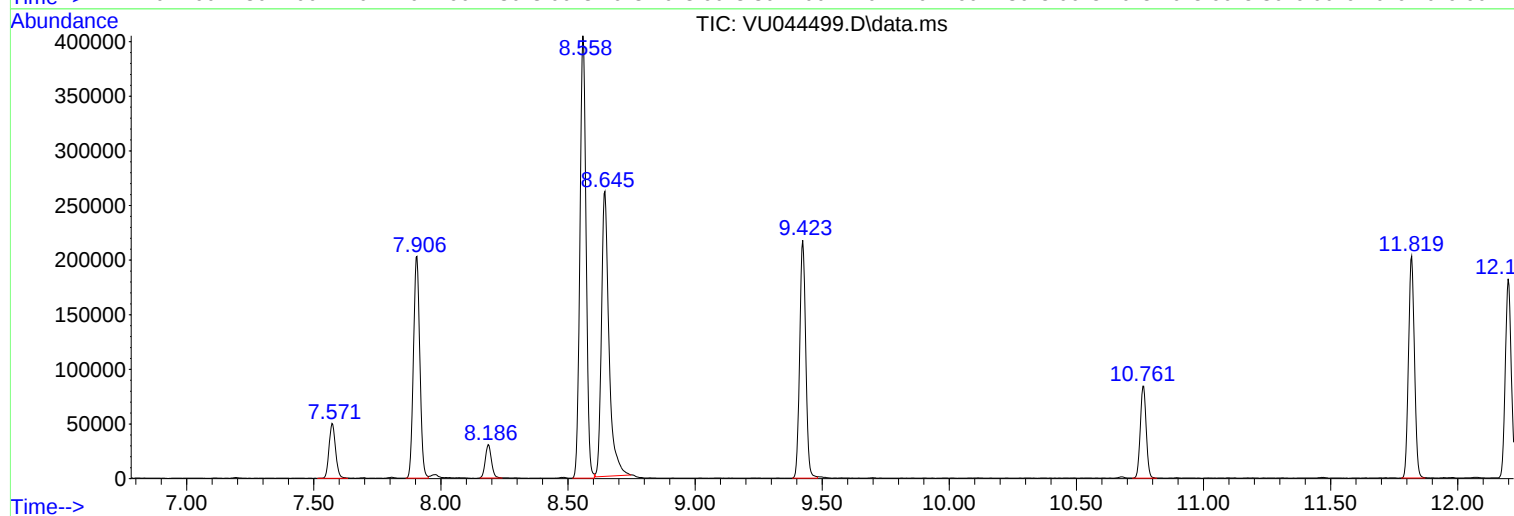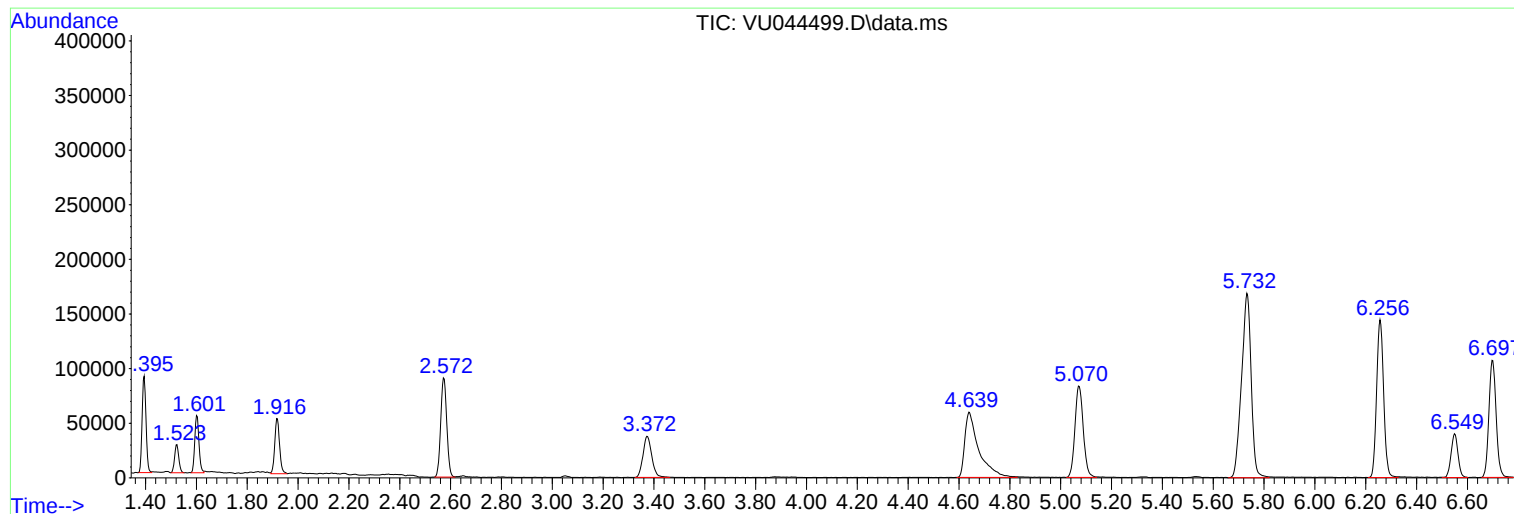

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044499.D
Acq On : 23 Aug 2021 13:52
Operator : SY/MD
Sample : M3515-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4558

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044499.D
Acq On : 23 Aug 2021 13:52
Operator : SY/MD
Sample : M3515-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4558

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
