

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
 Data File : VU044501.D
 Acq On : 23 Aug 2021 14:40
 Operator : SY/MD
 Sample : M3515-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4560

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	11	17	28	rVB	23200	24244	3.32%	0.539%
2	1.523	51	57	70	rVB2	8124	10471	1.44%	0.233%
3	1.600	74	81	95	rBV	50037	56103	7.69%	1.248%
4	1.919	172	180	196	rVB	47963	63248	8.67%	1.407%
5	2.572	369	383	398	rBV	88895	149076	20.44%	3.317%
6	3.372	616	632	649	rVB4	3262	8340	1.14%	0.186%
7	4.642	1012	1027	1053	rBV2	43915	158993	21.80%	3.538%
8	5.073	1144	1161	1187	rBV	82118	184667	25.32%	4.109%
9	5.732	1345	1366	1397	rBV2	160802	427018	58.56%	9.502%
10	6.256	1515	1529	1552	rBV	146976	281653	38.62%	6.267%
11	6.549	1605	1620	1639	rVB2	38450	71969	9.87%	1.601%
12	6.697	1650	1666	1692	rBV2	103843	206871	28.37%	4.603%
13	7.571	1926	1938	1959	rBV	47273	84716	11.62%	1.885%
14	7.906	2029	2042	2057	rBV	190653	335480	46.01%	7.465%
15	8.185	2118	2129	2149	rBV	28536	48465	6.65%	1.078%
16	8.558	2232	2245	2260	rBV	430864	729207	100.00%	16.227%
17	8.645	2260	2272	2326	rVB	221753	535864	73.49%	11.924%
18	9.423	2502	2514	2535	rBV	218312	364987	50.05%	8.122%
19	10.764	2918	2931	2949	rVB	80747	131826	18.08%	2.933%
20	11.819	3245	3259	3279	rBV	209965	334071	45.81%	7.434%
21	12.198	3365	3377	3394	rBV	175981	286619	39.31%	6.378%




Sum of corrected areas: 4493888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044501.D
Acq On : 23 Aug 2021 14:40
Operator : SY/MD
Sample : M3515-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4560

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

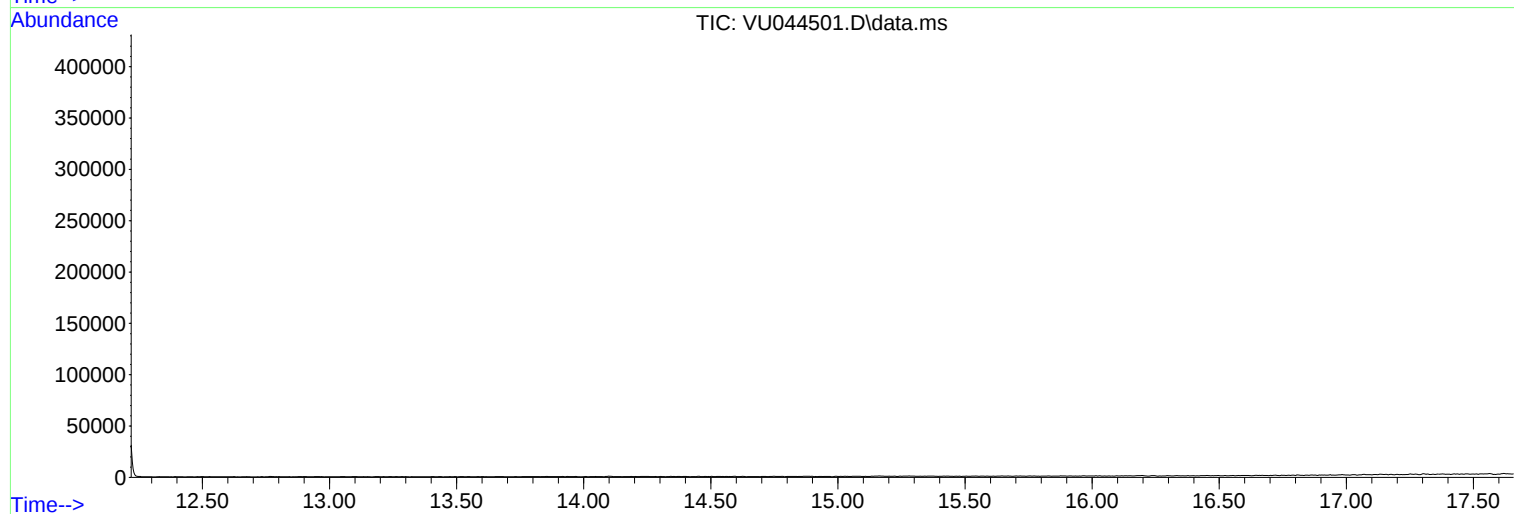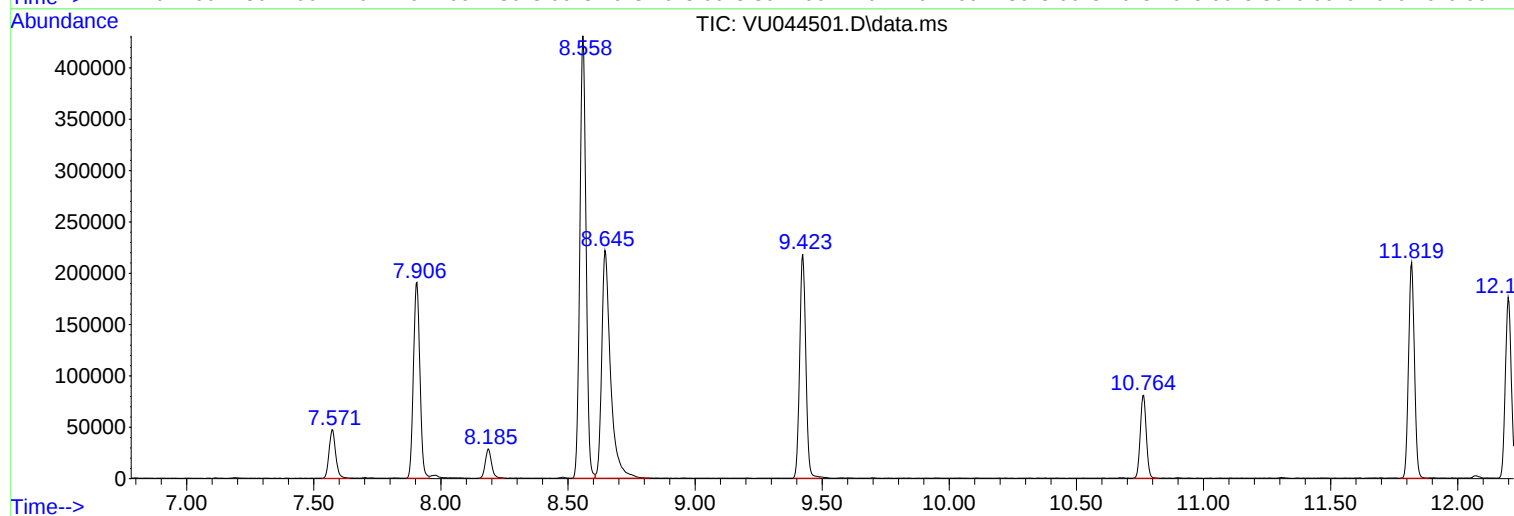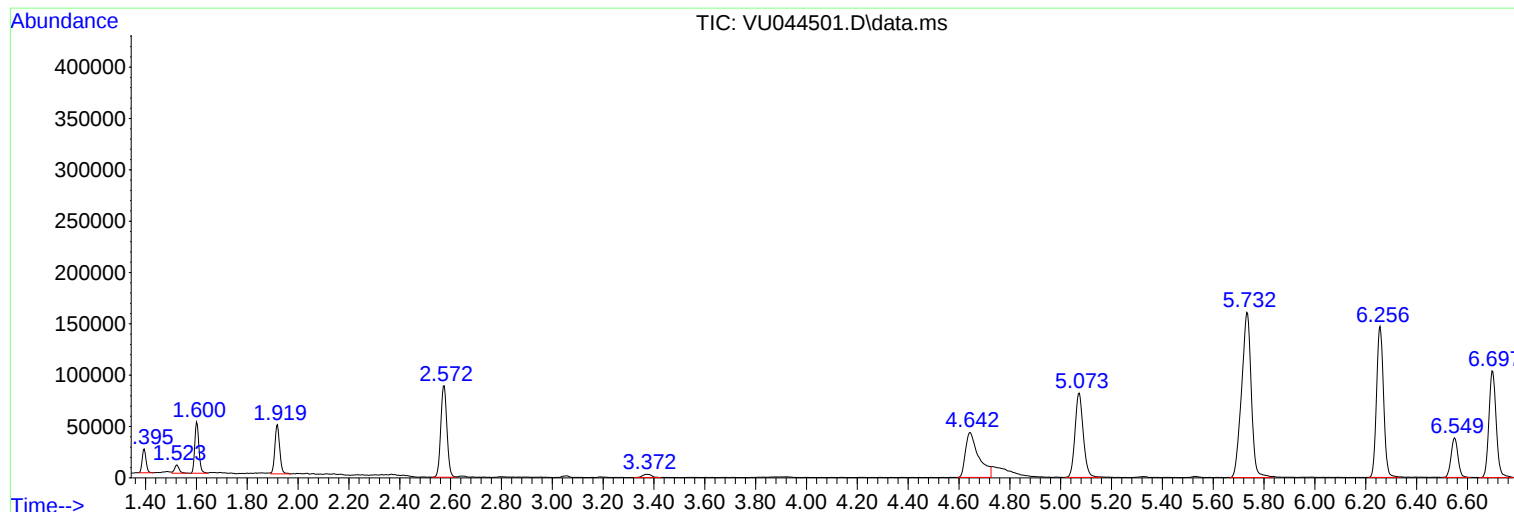

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044501.D
Acq On : 23 Aug 2021 14:40
Operator : SY/MD
Sample : M3515-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4560

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044501.D
Acq On : 23 Aug 2021 14:40
Operator : SY/MD
Sample : M3515-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4560

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
