

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
 Data File : VU044513.D
 Acq On : 23 Aug 2021 20:20
 Operator : SY/MD
 Sample : M3517-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AB9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU044513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	17	rVB2	16461	15822	2.95%	0.414%
2	1.475	37	42	52	rBV3	7985	11038	2.05%	0.289%
3	1.600	72	81	94	rBV2	62267	74325	13.84%	1.945%
4	1.916	171	179	193	rVB	49879	65879	12.26%	1.724%
5	2.208	264	270	281	rVB2	4668	6165	1.15%	0.161%
6	2.571	371	383	400	rBV	89082	144524	26.90%	3.782%
7	4.639	1011	1026	1079	rBV	60214	219015	40.77%	5.732%
8	5.073	1145	1161	1184	rBV	81922	187152	34.84%	4.898%
9	5.732	1345	1366	1390	rBV2	167900	439488	81.82%	11.502%
10	6.256	1514	1529	1551	rBV	140466	266428	49.60%	6.973%
11	6.549	1609	1620	1632	rVB4	12152	22910	4.26%	0.600%
12	6.697	1653	1666	1685	rBV	107171	209190	38.94%	5.475%
13	7.571	1926	1938	1954	rBV	48929	84560	15.74%	2.213%
14	7.906	2028	2042	2057	rBV	198120	345424	64.30%	9.040%
15	7.976	2058	2064	2077	rVB5	4183	6943	1.29%	0.182%
16	8.185	2117	2129	2144	rBV	28436	49262	9.17%	1.289%
17	8.558	2236	2245	2255	rBV2	19339	31853	5.93%	0.834%
18	8.642	2255	2271	2312	rBV	260880	537168	100.00%	14.058%
19	9.423	2502	2514	2540	rBV	209018	345795	64.37%	9.050%
20	10.761	2919	2930	2949	rVB	82819	133102	24.78%	3.483%
21	11.819	3246	3259	3272	rBV	192224	312054	58.09%	8.167%
22	12.069	3327	3337	3350	rBV3	9146	16551	3.08%	0.433%
23	12.198	3365	3377	3398	rVB	185371	296414	55.18%	7.757%




Sum of corrected areas: 3821062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044513.D
Acq On : 23 Aug 2021 20:20
Operator : SY/MD
Sample : M3517-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

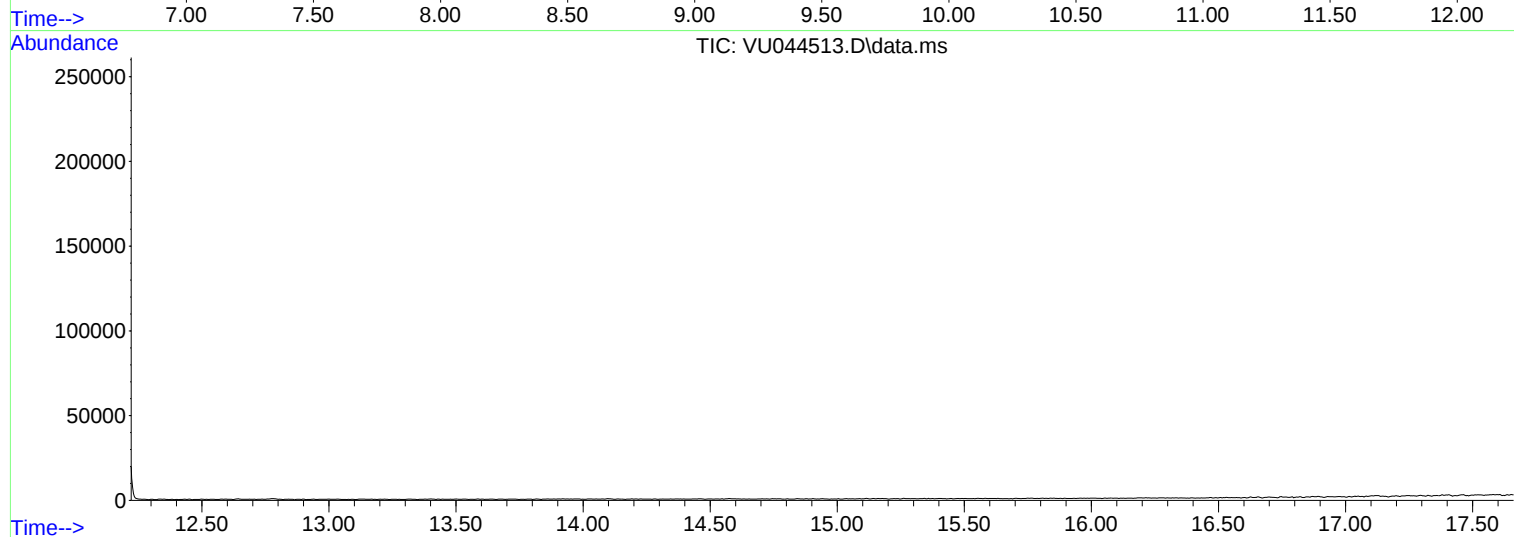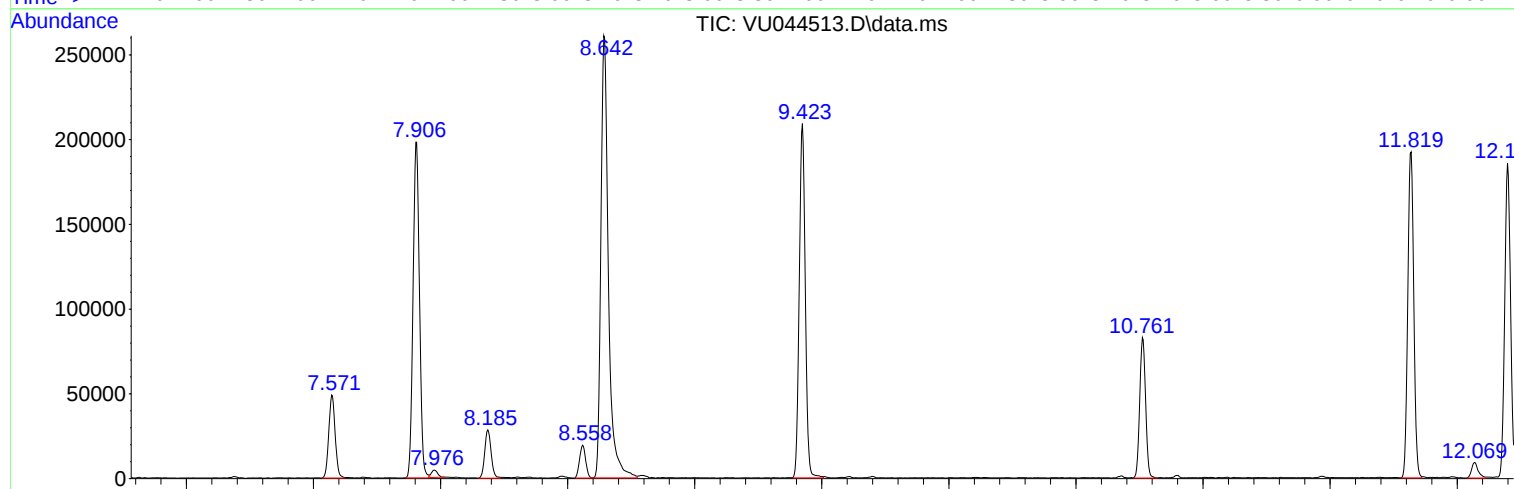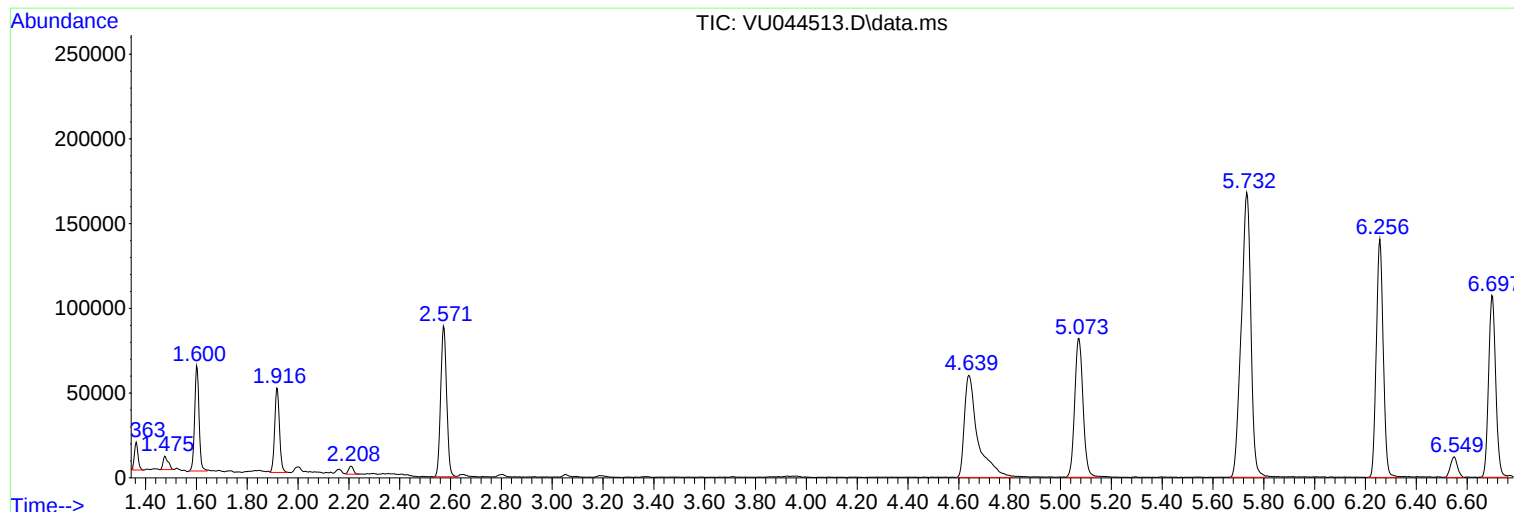

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044513.D
Acq On : 23 Aug 2021 20:20
Operator : SY/MD
Sample : M3517-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
Data File : VU044513.D
Acq On : 23 Aug 2021 20:20
Operator : SY/MD
Sample : M3517-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
