
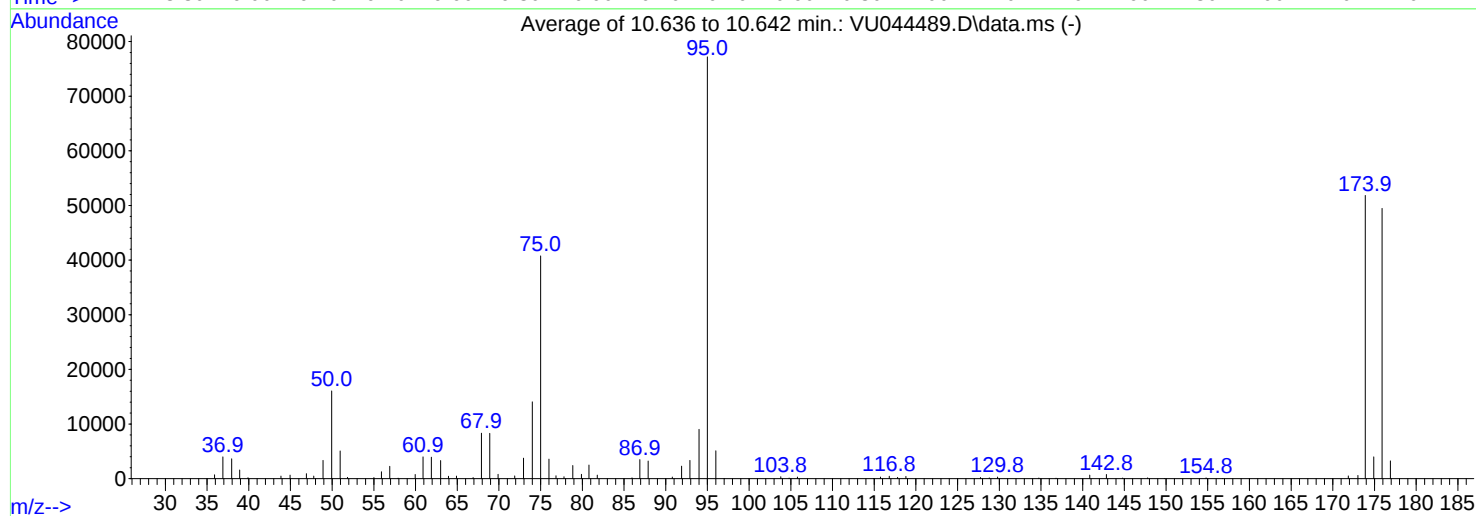


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082321\
 Data File : VU044489.D
 Acq On : 23 Aug 2021 08:55
 Operator : SY/MD
 Sample : BFB009
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB009

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Aug 24 06:16:49 2021

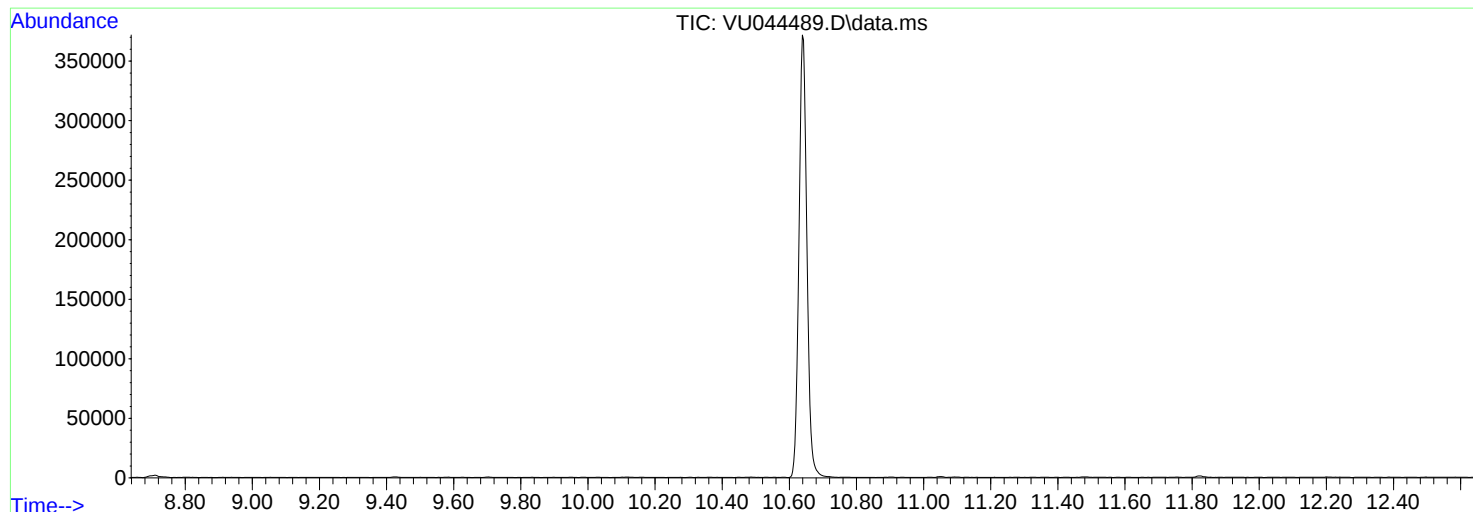

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	16055	PASS
75	95	30	80	52.8	40768	PASS
95	95	100	100	100.0	77200	PASS
96	95	5	9	6.6	5111	PASS
173	174	0.00	2	1.2	603	PASS
174	95	50	120	67.1	51829	PASS
175	174	5	9	7.7	3978	PASS
176	174	95	101	95.4	49459	PASS
177	176	5	9	6.6	3248	PASS

m/z	Abundance
43.80	332.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	688.0
36.90	3989.0
37.90	3556.0
38.90	1570.0
39.80	185.0
43.90	793.0
45.00	622.0
46.90	835.0
47.80	455.0
48.90	3304.0
50.00	15378.0
50.90	4890.0
51.80	242.0
55.00	220.0
55.90	1214.0
56.90	2150.0
59.90	688.0
60.90	3835.0
61.90	3748.0
63.00	3077.0
63.90	416.0
64.90	429.0
66.90	208.0
67.90	8016.0
68.90	7966.0
69.90	754.0
71.90	454.0
72.90	3572.0
74.00	13495.0
75.00	38824.0
76.00	3471.0
77.00	504.0
77.80	321.0
78.80	2258.0
79.90	744.0
80.80	2324.0
81.80	581.0
85.90	109.0
86.90	3285.0
87.90	3081.0
90.80	293.0
91.90	2163.0
92.90	3275.0
94.00	8628.0
95.00	73112.0
96.00	4821.0
97.00	105.0
103.80	322.0
104.80	105.0
105.80	309.0
115.70	303.0
116.80	407.0
117.80	203.0
118.80	360.0
127.70	178.0
128.80	166.0
129.80	308.0
134.80	102.0
136.80	131.0
140.80	597.0
142.80	769.0
144.80	131.0
147.80	128.0
149.80	102.0
154.80	120.0
171.90	516.0
173.10	608.0
173.90	47848.0
174.90	3897.0
175.90	46656.0
176.90	3148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	714.0
36.90	4087.0
38.00	3749.0
38.90	1623.0
39.90	179.0
43.90	841.0
45.00	681.0
46.90	949.0
47.80	468.0
48.90	3376.0
50.00	16592.0
50.90	5235.0
51.90	242.0
55.00	233.0
55.90	1307.0
56.90	2348.0
57.90	113.0
60.00	791.0
60.90	4146.0
61.90	4088.0
63.00	3432.0
64.00	475.0
64.90	480.0
66.90	204.0
67.90	8598.0
68.90	8507.0
69.90	820.0
71.90	528.0
73.00	3839.0
74.00	14612.0
75.00	42072.0
76.00	3690.0
76.80	548.0
77.80	348.0
78.80	2487.0
79.90	835.0
80.80	2590.0
81.80	658.0
86.00	157.0
86.90	3549.0
87.90	3319.0
90.80	297.0
91.90	2430.0
92.90	3415.0
94.00	9303.0
95.00	79944.0
96.00	5241.0
103.80	359.0
104.80	106.0
105.80	311.0
114.90	102.0
115.70	317.0
116.80	451.0
117.80	232.0
118.80	430.0
127.70	199.0
128.80	165.0
129.80	309.0
134.70	108.0
136.80	127.0
140.90	684.0
142.80	814.0
144.80	136.0
147.80	149.0
154.80	151.0
171.80	513.0
173.00	621.0
173.90	53464.0
174.90	4102.0
175.90	50600.0
176.90	3301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	681.0
36.90	3904.0
37.90	3581.0
38.90	1515.0
40.00	180.0
43.90	806.0
44.90	637.0
46.90	921.0
47.80	444.0
48.90	3314.0
49.90	16195.0
51.00	5064.0
51.90	230.0
55.00	216.0
55.90	1270.0
56.90	2304.0
57.90	117.0
60.00	821.0
60.90	4015.0
61.90	3976.0
63.00	3381.0
63.90	449.0
64.90	529.0
66.90	192.0
67.90	8355.0
68.90	8436.0
69.90	774.0
71.90	504.0
73.00	3799.0
74.00	14078.0
75.00	41408.0
76.00	3533.0
76.80	539.0
77.80	352.0
78.90	2509.0
79.90	838.0
80.80	2593.0
81.80	677.0
86.00	191.0
86.90	3609.0
87.90	3228.0
90.80	277.0
91.90	2285.0
92.90	3362.0
94.00	9128.0
95.00	78544.0
96.00	5270.0
103.80	379.0
104.80	103.0
105.80	285.0
115.80	297.0
116.80	473.0
117.80	251.0
118.80	472.0
127.80	210.0
128.80	140.0
129.80	262.0
134.70	117.0
140.90	663.0
142.90	748.0
144.80	125.0
147.80	162.0
154.80	164.0
156.80	122.0
171.80	493.0
172.90	579.0
173.90	54176.0
174.90	3934.0
175.90	51120.0
176.90	3295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009