

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU082418\
 Data File : VU026350.D
 Acq On : 24 Aug 2018 21:45
 Operator : MD/SY
 Sample : J4644-18 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOM8

Quant Time: Aug 25 05:01:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 25 04:25:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	226645	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	220978	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	105400	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	74123	53.62	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	107.24%
7) Chloroethane-d5	1.68	69	60998	54.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.22%
11) 1,1-Dichloroethene-d2	2.27	63	112270	41.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.64%
21) 2-Butanone-d5	4.18	46	136150	123.40	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	123.40%
24) Chloroform-d	4.65	84	175727	57.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	114.06%
26) 1,2-Dichloroethane-d4	5.31	65	118799	59.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	118.50%
32) Benzene-d6	5.35	84	337442	57.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	114.16%
36) 1,2-Dichloropropane-d6	6.33	67	113314	59.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	119.40%
41) Toluene-d8	7.57	98	303198	53.66	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.32%
43) trans-1,3-Dichloropropene-	7.85	79	52786	53.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	107.64%
47) 2-Hexanone-d5	8.31	63	95354	117.54	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	117.54%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	161005	57.31	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	114.62%
64) 1,2-Dichlorobenzene-d4	11.86	152	132476	59.23	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	118.46%

Target Compounds


					Qvalue
5) Vinyl chloride	1.40	62	709252	429.031 ug/L	95
17) trans-1,2-Dichloroethene	2.99	96	53498	36.385 ug/L	97
20) cis-1,2-Dichloroethene	4.23	96	3636452	2240.605 ug/L	98
34) Trichloroethene	6.19	95	4716	2.960 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082418\
Data File : VU026350.D
Acq On : 24 Aug 2018 21:45
Operator : MD/SY
Sample : J4644-18 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOM8

Quant Time: Aug 25 05:01:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 25 04:25:01 2018
Response via : Initial Calibration

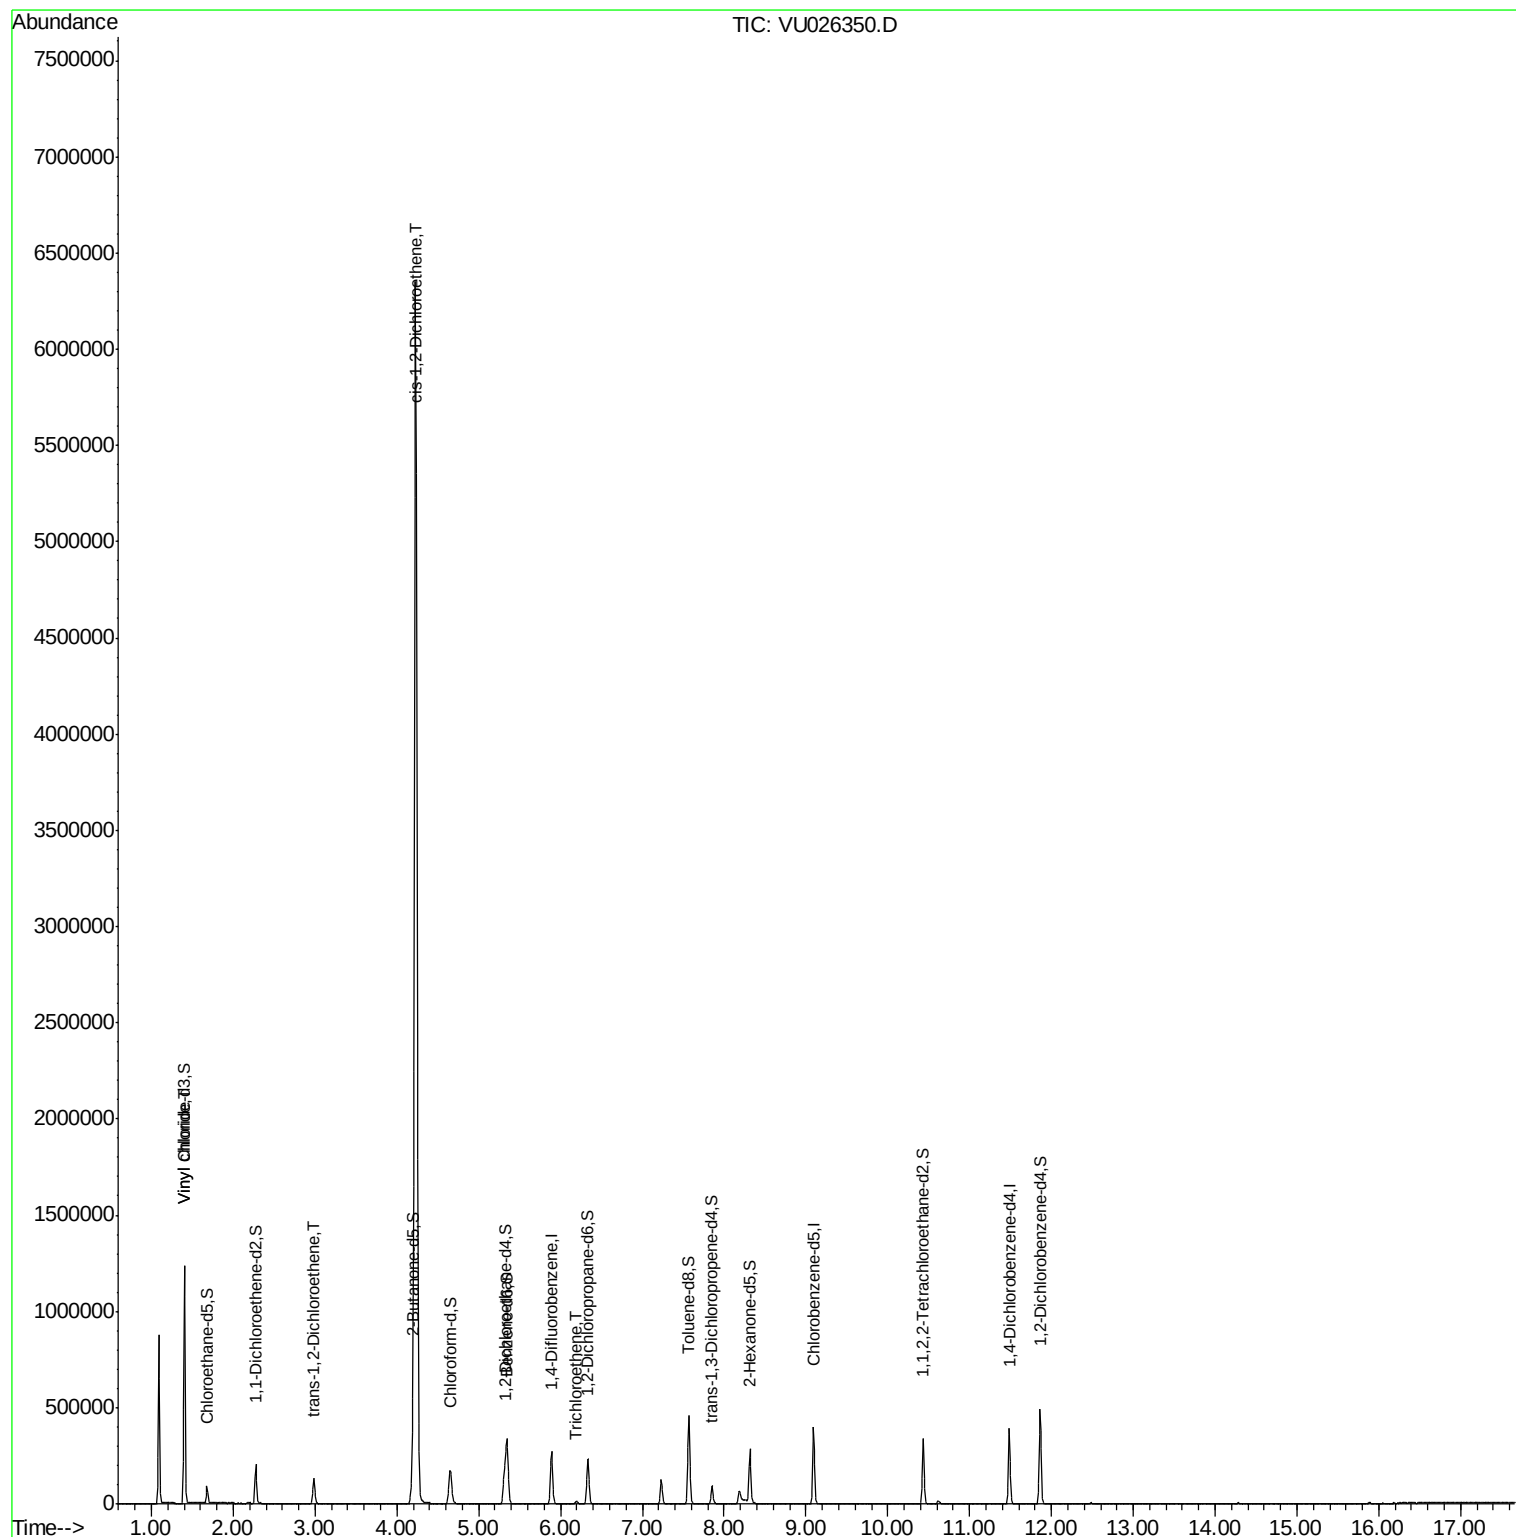

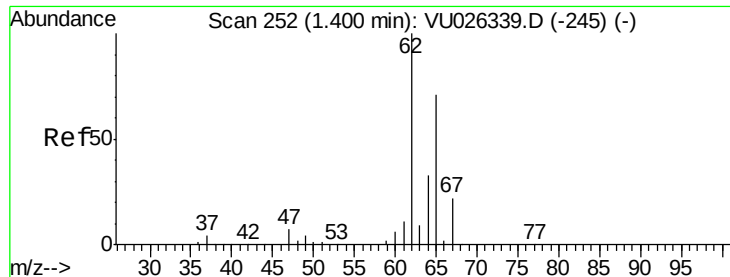

#5

Vinyl chloride

Concen: 429.031 ug/L

RT: 1.40 min Scan# 253

Delta R.T. 0.00 min

Lab File: VU026350.D

Acq: 24 Aug 2018 21:45

Instrument :

MSVOA_U

ClientSampleId :


ETOM8

Tgt Ion: 62 Resp: 709252

Ion Ratio Lower Upper




62 100

64 31.7 24.2 45.0

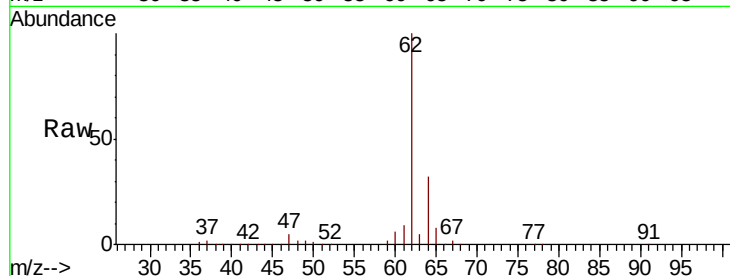

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.00 (63.70 to 64.70): VU0

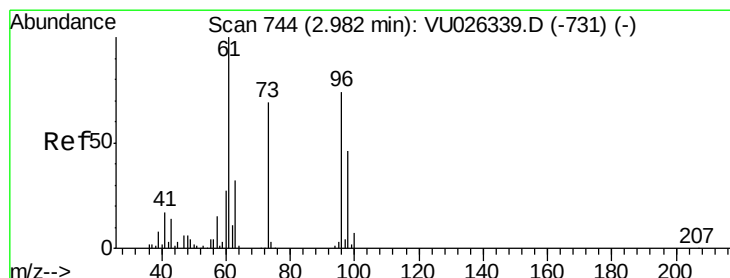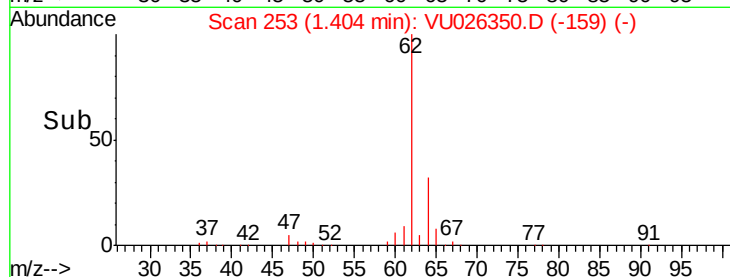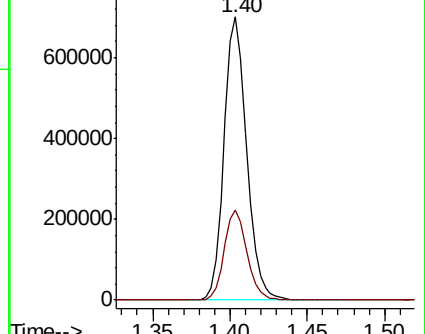

#17

trans-1,2-Dichloroethene

Concen: 36.385 ug/L

RT: 2.99 min Scan# 745

Delta R.T. 0.00 min

Lab File: VU026350.D

Acq: 24 Aug 2018 21:45


Tgt Ion: 96 Resp: 53498

Ion Ratio Lower Upper

96 100

61 136.4 97.9 181.9



98 66.0 45.1 83.7

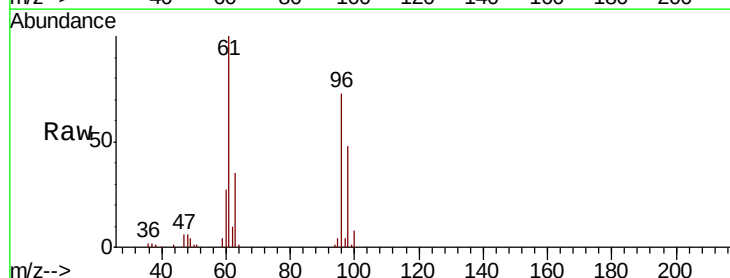


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

Ion 98.00 (97.70 to 98.70): VU0

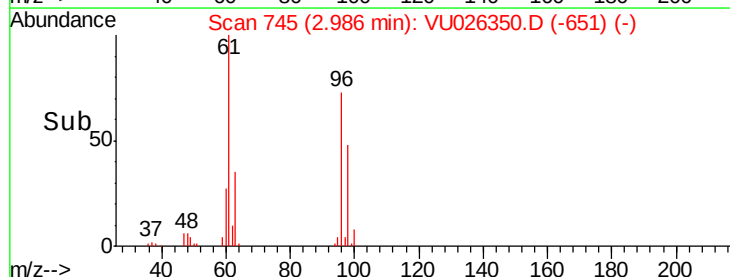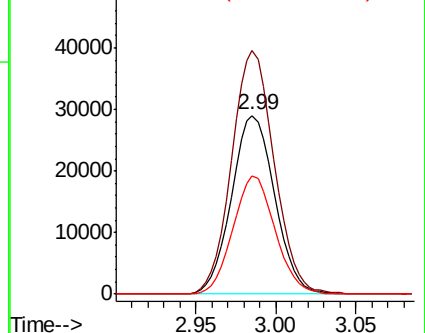

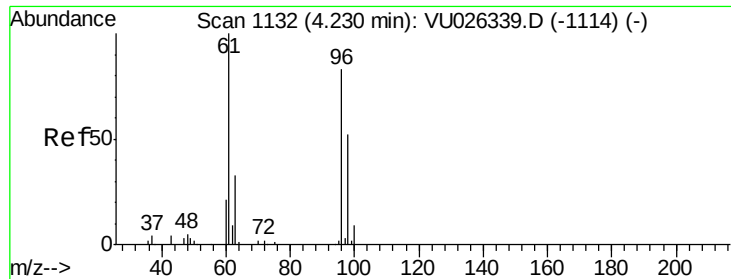

#20

cis-1,2-Dichloroethene

Concen: 2240.605 ug/L

RT: 4.23 min Scan# 1132

Delta R.T. 0.00 min

Lab File: VU026350.D

Acq: 24 Aug 2018 21:45

Instrument :

MSVOA_U

ClientSampleId :

ETOM8


Tgt Ion: 96 Resp: 3636452

Ion Ratio Lower Upper

96 100

61 126.2 90.3 167.7




68 0.0 0.0 0.0

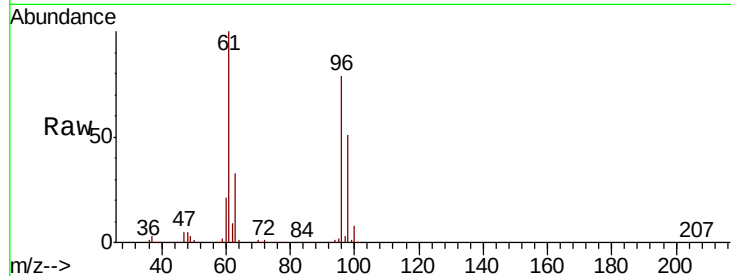

Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

Ion 68.00 (67.70 to 68.70): VU0

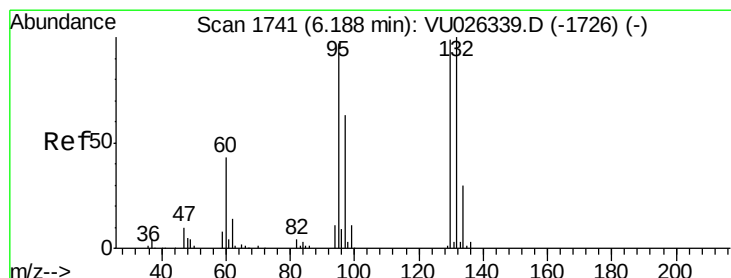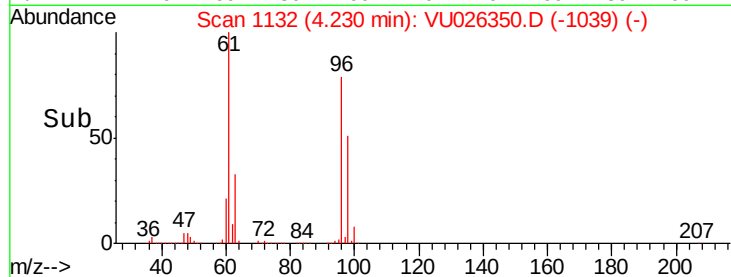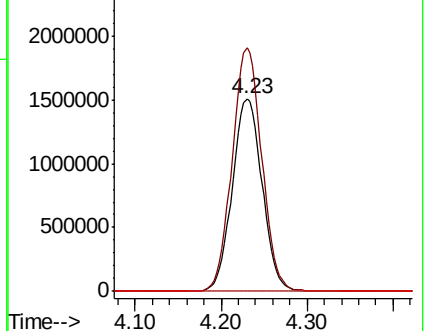

#34

Trichloroethene

Concen: 2.960 ug/L

RT: 6.19 min Scan# 1741

Delta R.T. 0.00 min

Lab File: VU026350.D

Acq: 24 Aug 2018 21:45

Tgt Ion: 95 Resp: 4716


Ion Ratio Lower Upper

95 100

97 69.4 47.2 87.6

132 92.8 70.2 130.4

130 112.9 73.4 136.4

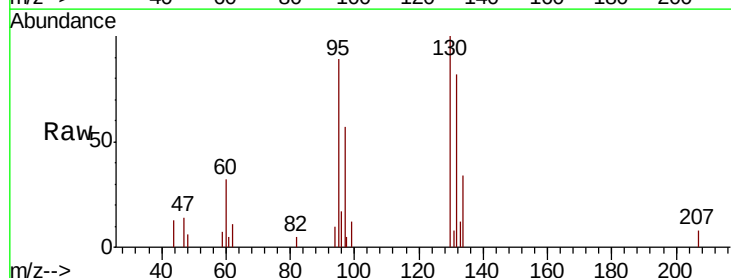

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

