


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082418\
Data File : VU026326.D
Acq On : 24 Aug 2018 11:31
Operator : MD/SY
Sample : BFB42
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Title : VOC Analysis
Last Update : Mon Aug 27 02:08:45 2018

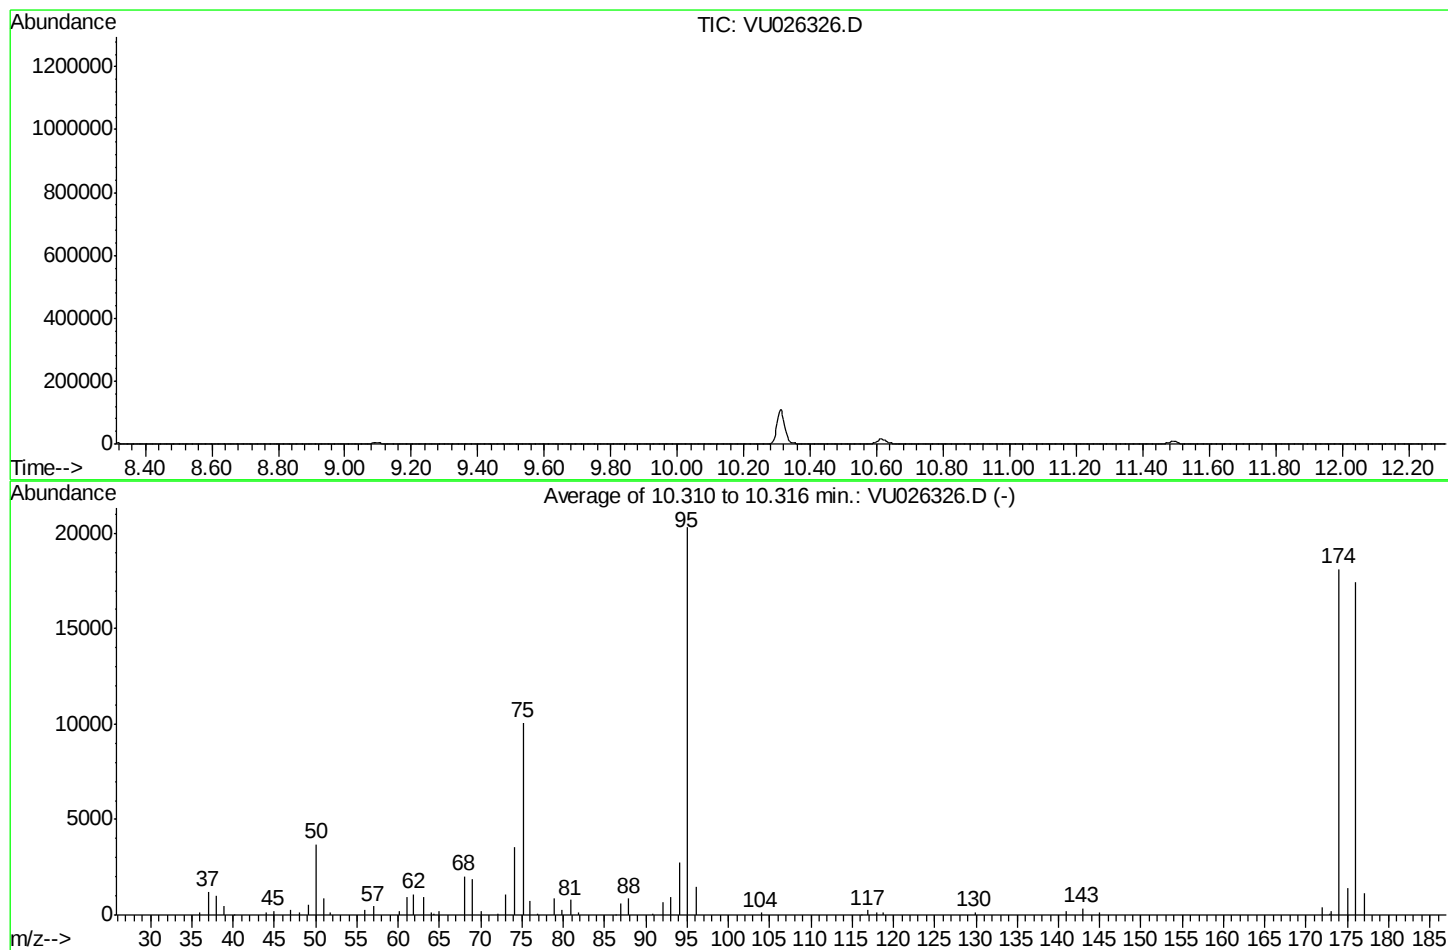

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	3716	PASS
75	95	30	80	49.5	10064	PASS
95	95	100	100	100.0	20312	PASS
96	95	5	9	7.4	1510	PASS
173	174	0.00	2	1.0	185	PASS
174	95	50	120	89.3	18141	PASS
175	174	5	9	7.7	1395	PASS
176	174	95	101	96.0	17418	PASS
177	176	5	9	6.4	1117	PASS

Scan 3011 (10.271 min): VU026326.D
BFB42

m/z	Abundance
40.10	158.0
44.00	532.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	151.0
37.00	1314.0
38.00	1046.0
39.00	522.0
40.10	186.0
44.10	694.0
44.80	209.0
47.00	325.0
48.10	145.0
49.10	583.0
50.10	4014.0
51.00	952.0
51.80	116.0
56.00	291.0
57.00	510.0
60.00	268.0
61.00	912.0
61.90	1279.0
63.00	1087.0
64.10	177.0
65.00	272.0
68.00	2223.0
69.00	1906.0
70.00	205.0
73.00	1190.0
74.00	3641.0
75.10	10562.0
75.90	744.0
76.90	153.0
78.90	858.0
79.80	279.0
80.90	852.0
81.90	159.0
87.00	724.0
87.90	879.0
90.90	121.0
92.00	709.0
93.00	988.0
94.00	2979.0
95.00	20944.0
96.10	1462.0
104.00	134.0
116.10	105.0
116.90	258.0
117.90	219.0
118.80	158.0
129.80	160.0
141.00	277.0
142.90	294.0
144.90	148.0
171.90	385.0
172.90	249.0
174.00	18688.0
175.00	1503.0
176.00	18120.0
177.00	1200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	151.0
37.00	1264.0
38.00	1029.0
39.00	482.0
40.10	179.0
44.10	706.0
44.90	181.0
47.00	277.0
48.10	130.0
49.10	550.0
50.10	3845.0
50.90	918.0
51.80	137.0
55.90	234.0
57.00	484.0
60.10	181.0
61.00	982.0
61.90	1148.0
63.00	997.0
63.90	126.0
64.20	133.0
65.00	231.0
68.00	2104.0
69.00	1870.0
70.00	186.0
73.00	1060.0
74.00	3691.0
75.10	10389.0
75.90	720.0
78.90	861.0
79.80	241.0
80.90	820.0
81.90	156.0
86.30	102.0
86.90	618.0
87.90	884.0
90.90	122.0
92.00	680.0
93.00	1006.0
94.10	2809.0
95.00	21040.0
96.10	1596.0
104.00	140.0
116.90	259.0
117.90	175.0
118.80	164.0
129.80	151.0
140.90	243.0
142.90	355.0
145.00	150.0
171.90	407.0
173.10	292.0
174.00	18672.0
175.00	1450.0
176.00	17776.0
177.00	1142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.00	135.0
37.00	1053.0
38.00	979.0
38.90	415.0
40.10	176.0
44.00	579.0
44.90	219.0
47.00	221.0
48.00	119.0
49.10	477.0
50.10	3289.0
51.00	836.0
51.80	112.0
55.80	200.0
56.90	388.0
60.10	116.0
61.00	882.0
61.90	894.0
63.00	787.0
64.30	112.0
64.90	199.0
68.00	1809.0
69.00	1904.0
70.00	126.0
72.00	127.0
73.00	876.0
74.10	3377.0
75.10	9243.0
75.90	657.0
78.90	821.0
79.90	218.0
80.90	699.0
81.90	168.0
86.90	540.0
88.00	793.0
92.00	600.0
93.10	842.0
94.00	2370.0
95.00	18952.0
96.10	1474.0
104.00	119.0
116.90	197.0
118.80	153.0
129.90	121.0
140.80	186.0
143.00	419.0
145.00	157.0
171.90	398.0
173.10	263.0
174.00	17064.0
175.00	1234.0
176.00	16358.0
177.00	1010.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42