


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082421\
Data File : VU044515.D
Acq On : 24 Aug 2021 10:14
Operator : SY/MD
Sample : BFB010
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB010

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Aug 25 03:50:31 2021

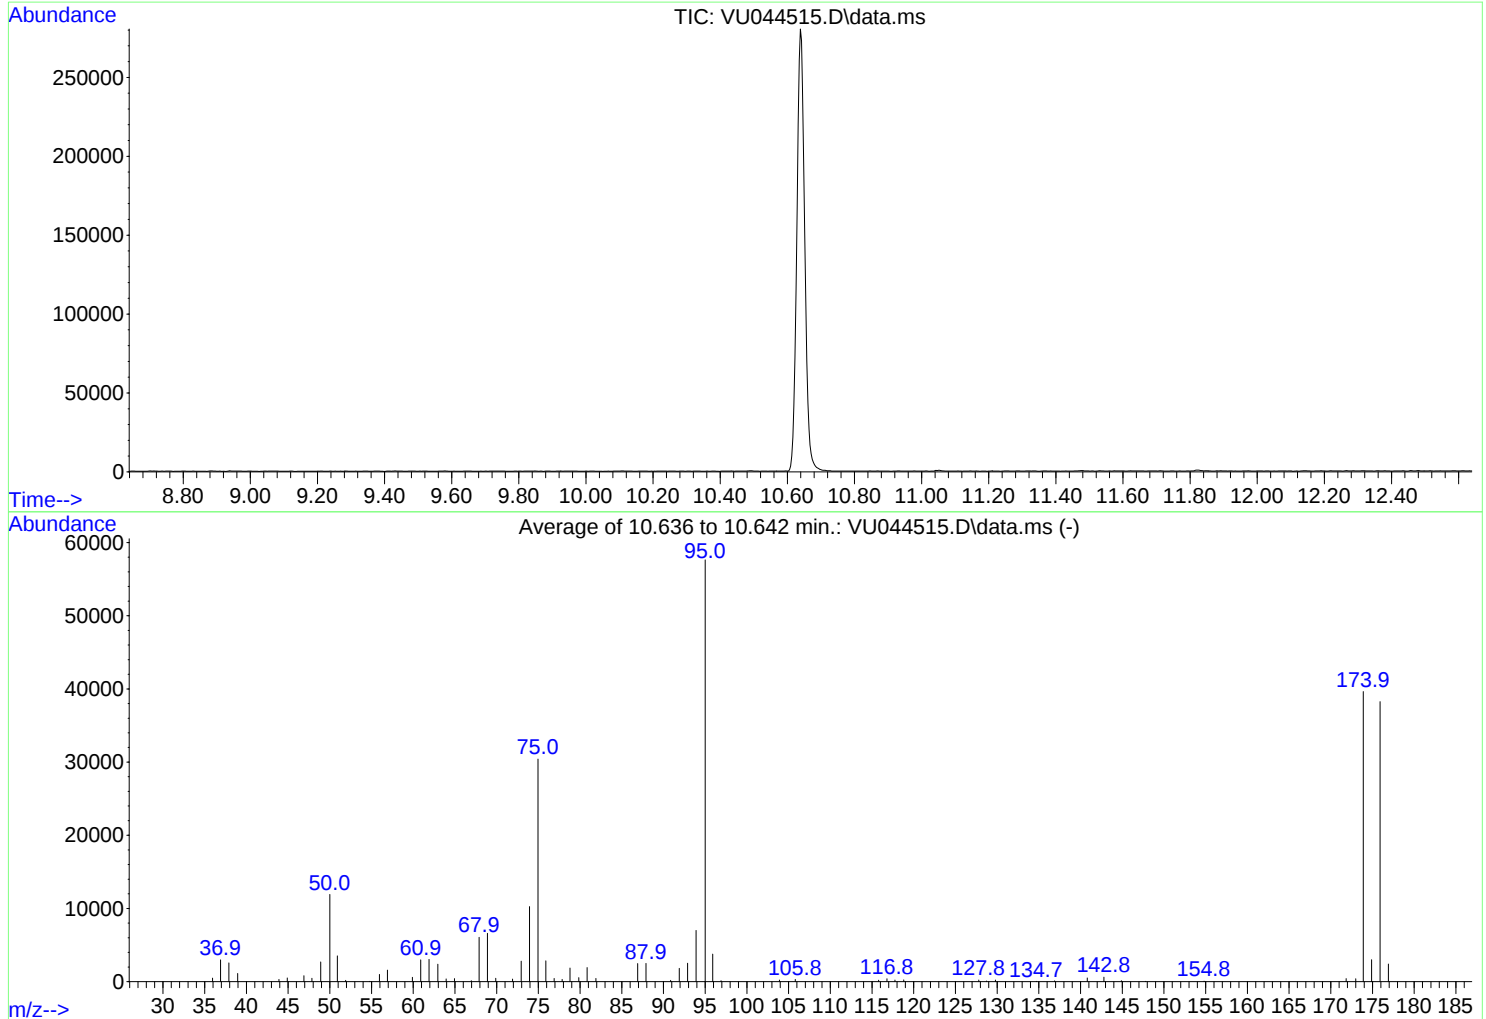

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	11916	PASS
75	95	30	80	52.8	30419	PASS
95	95	100	100	100.0	57640	PASS
96	95	5	9	6.5	3763	PASS
173	174	0.00	2	1.0	384	PASS
174	95	50	120	68.8	39640	PASS
175	174	5	9	7.5	2990	PASS
176	174	95	101	96.6	38275	PASS
177	176	5	9	6.3	2408	PASS

Scan 2878 (10.594 min): VU044515.D\data.ms
BFB010

m/z	Abundance
39.80	196.0
43.90	403.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
36.00	505.0
36.90	2957.0
37.90	2474.0
39.00	1147.0
39.80	197.0
43.90	715.0
44.90	519.0
46.90	775.0
47.90	474.0
48.90	2662.0
50.00	11639.0
50.90	3358.0
51.90	159.0
54.80	135.0
55.90	1031.0
56.90	1563.0
59.90	637.0
60.90	2970.0
61.90	2962.0
63.00	2394.0
64.00	356.0
64.90	392.0
67.00	142.0
67.90	5850.0
68.90	6347.0
69.90	464.0
71.90	355.0
73.00	2747.0
73.90	9861.0
75.00	29664.0
75.90	2836.0
76.90	404.0
77.90	307.0
78.80	1817.0
79.80	521.0
80.80	1911.0
81.90	414.0
86.90	2411.0
87.90	2320.0
90.80	166.0
91.90	1701.0
92.90	2522.0
93.90	6679.0
95.00	55384.0
95.90	3625.0
96.90	125.0
103.90	215.0
105.80	284.0
115.80	201.0
116.80	373.0
117.80	223.0
118.80	261.0
127.80	209.0
129.80	210.0
134.70	114.0
136.90	109.0
140.80	477.0
142.80	562.0
144.90	133.0
154.80	115.0
171.90	377.0
173.00	389.0
173.90	37256.0
174.90	2983.0
175.90	35736.0
176.90	2236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	473.0
36.90	3043.0
37.90	2599.0
39.00	1141.0
39.90	196.0
43.90	700.0
44.90	529.0
46.90	841.0
47.80	488.0
48.90	2825.0
50.00	12360.0
50.90	3600.0
51.90	187.0
56.00	1020.0
56.90	1630.0
59.90	622.0
60.90	3108.0
61.90	3123.0
63.00	2469.0
64.00	391.0
65.00	421.0
67.00	134.0
67.90	6279.0
68.90	6842.0
69.90	473.0
71.90	365.0
73.00	2900.0
74.00	10641.0
74.90	31360.0
75.90	2951.0
76.90	448.0
77.80	320.0
78.80	1923.0
79.90	574.0
80.90	1957.0
81.90	464.0
86.90	2555.0
87.90	2582.0
90.90	178.0
91.90	1928.0
92.90	2609.0
93.90	7242.0
95.00	59496.0
95.90	3890.0
96.90	129.0
103.90	239.0
105.80	316.0
115.80	210.0
116.80	419.0
117.70	226.0
118.80	249.0
127.80	223.0
128.70	120.0
129.80	222.0
136.90	107.0
140.80	520.0
142.80	639.0
144.90	133.0
154.80	107.0
171.90	430.0
173.00	407.0
173.90	40912.0
174.90	3068.0
175.90	39576.0
176.90	2499.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	449.0
36.90	2937.0
37.90	2605.0
38.90	1056.0
39.90	187.0
43.90	699.0
44.90	484.0
46.90	793.0
47.90	416.0
48.90	2584.0
50.00	11750.0
50.90	3581.0
51.90	179.0
56.00	915.0
56.90	1557.0
59.90	541.0
60.90	2877.0
61.90	3068.0
62.90	2318.0
63.90	383.0
65.00	415.0
66.80	121.0
67.90	6044.0
68.90	6645.0
69.90	457.0
71.90	304.0
72.90	2773.0
74.00	10285.0
75.00	30232.0
75.90	2746.0
76.90	472.0
77.80	291.0
78.80	1851.0
79.90	577.0
80.90	1885.0
81.90	438.0
86.90	2482.0
87.90	2552.0
90.90	202.0
91.90	1815.0
92.90	2397.0
93.90	7079.0
95.00	58040.0
95.90	3774.0
96.90	126.0
103.90	207.0
105.80	291.0
115.80	192.0
116.80	382.0
117.70	203.0
118.80	236.0
127.80	208.0
128.80	120.0
129.80	200.0
136.90	104.0
140.80	497.0
142.80	621.0
144.90	117.0
147.80	117.0
171.80	433.0
173.00	355.0
173.90	40752.0
174.90	2919.0
175.90	39512.0
176.90	2489.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010