

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050433.D
 Acq On : 24 Aug 2022 18:23
 Operator : SY/MD
 Sample : N4322-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY182

Quant Time: Aug 25 05:33:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 25 05:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	323824	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	317041	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	115590	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	167644	43.783	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.560%
7) Chloroethane-d5	1.900	69	133282	47.042	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.080%
11) 1,1-Dichloroethene-d2	2.562	63	189240	34.972	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.940%
21) 2-Butanone-d5	4.623	46	251207	100.233	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.230%
24) Chloroform-d	5.060	84	275598	44.838	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.680%
26) 1,2-Dichloroethane-d4	5.700	65	178688	46.776	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.560%
32) Benzene-d6	5.726	84	554053	47.296	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.600%
36) 1,2-Dichloropropane-d6	6.690	67	187472	48.308	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.620%
41) Toluene-d8	7.899	98	446635	43.572	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.140%
43) trans-1,3-Dichloroprop...	8.179	79	70285	43.418	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.840%
47) 2-Hexanone-d5	8.633	63	139277	96.708	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.710%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	278081	46.458	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.920%
66) 1,2-Dichlorobenzene-d4	12.195	152	144181	52.217	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.440%
Target Compounds						
13) Acetone	2.630	43	14992	9.098	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050433.D
Acq On : 24 Aug 2022 18:23
Operator : SY/MD
Sample : N4322-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY182

Quant Time: Aug 25 05:33:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 25 05:03:52 2022
Response via : Initial Calibration

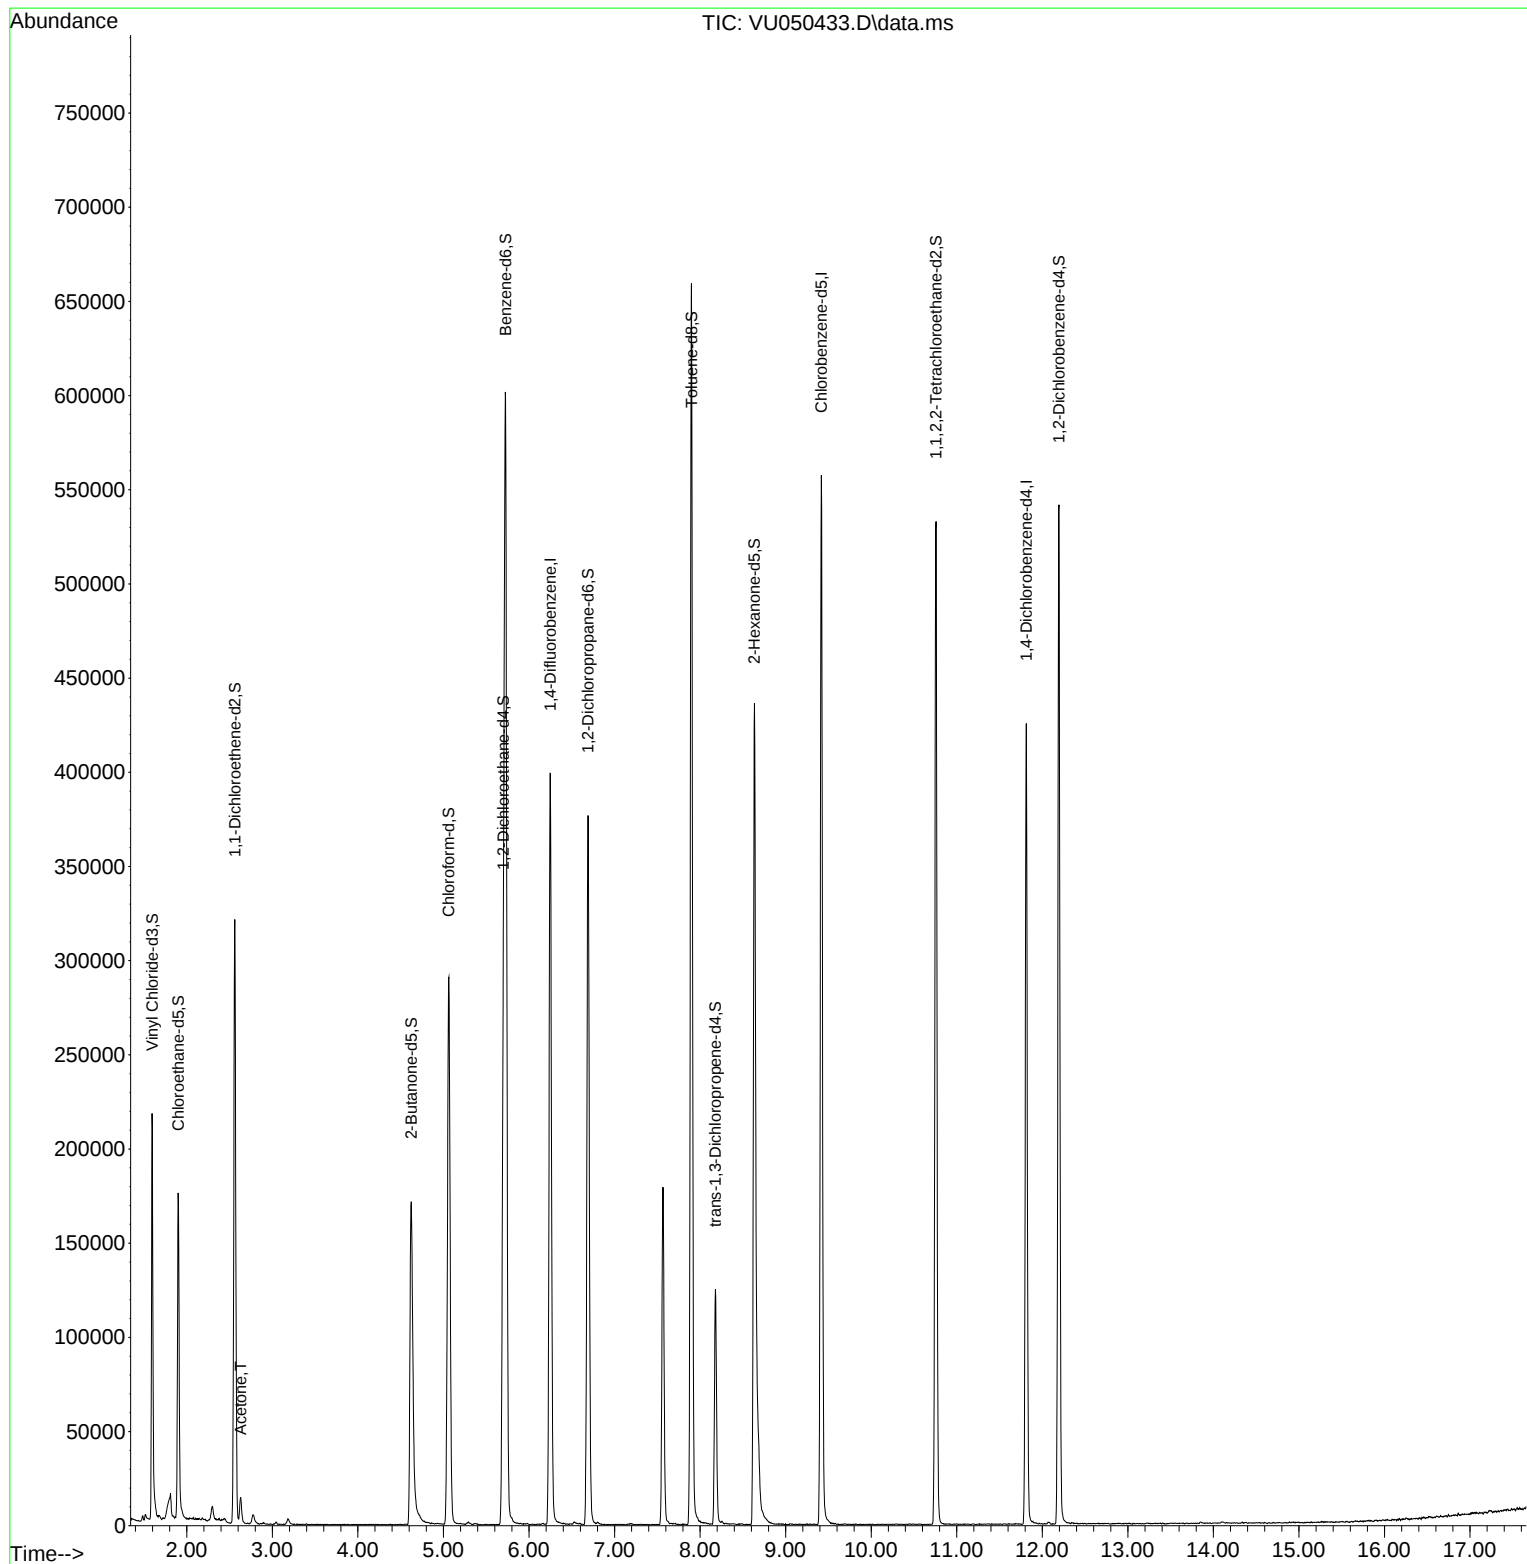

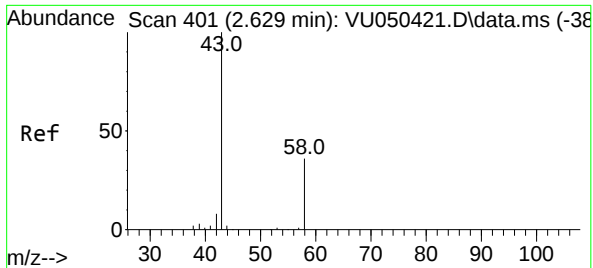

#13
 Acetone
 Concen: 9.098 ug/L
 RT: 2.630 min Scan# 401
 Delta R.T. 0.000 min
 Lab File: VU050433.D
 Acq: 24 Aug 2022 18:23

Instrument :
 MSVOA_U
 ClientSampleId :
 EY182

Tgt Ion: 43 Resp: 14992
 Ion Ratio Lower Upper
 43 100
 58 34.1 0.0 72.2

