

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050425.D
 Acq On : 24 Aug 2022 15:00
 Operator : SY/MD
 Sample : VU0824WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	50	rBV3	3317	4378	0.25%	0.036%
2	1.517	51	55	66	rVB2	3639	5240	0.30%	0.043%
3	1.597	72	80	102	rBV	233306	282027	16.19%	2.326%
4	1.903	166	175	203	rVB	189712	258732	14.85%	2.134%
5	2.562	367	380	397	rBV	356657	572165	32.84%	4.719%
6	2.787	438	450	451	rBV3	1518	2064	0.12%	0.017%
7	2.954	499	502	504	rBV	367	261	0.01%	0.002%
8	3.041	521	529	541	rVB4	2429	4560	0.26%	0.038%
9	3.186	559	574	592	rBV	17016	39559	2.27%	0.326%
10	3.337	616	621	622	rBV2	239	234	0.01%	0.002%
11	3.379	630	634	640	rBV3	311	272	0.02%	0.002%
12	3.427	647	649	657	rVB2	330	252	0.01%	0.002%
13	3.629	708	712	717	rBV	256	266	0.02%	0.002%
14	3.954	810	813	817	rVB2	224	160	0.01%	0.001%
15	4.060	843	846	849	rBV	207	169	0.01%	0.001%
16	4.314	921	925	933	rVB2	289	357	0.02%	0.003%
17	4.353	933	937	939	rBV2	174	156	0.01%	0.001%
18	4.462	968	971	977	rVB2	198	199	0.01%	0.002%
19	4.626	1008	1022	1050	rBV	180942	466905	26.80%	3.851%
20	4.925	1113	1115	1118	rBV	285	161	0.01%	0.001%
21	4.941	1118	1120	1123	rVV3	438	290	0.02%	0.002%
22	4.960	1124	1126	1129	rVB3	463	225	0.01%	0.002%
23	5.063	1141	1158	1177	rBV	311470	679153	38.98%	5.601%
24	5.205	1198	1202	1203	rBV2	348	222	0.01%	0.002%
25	5.292	1219	1229	1238	rVB5	1431	2758	0.16%	0.023%
26	5.337	1239	1243	1245	rBV2	296	204	0.01%	0.002%
27	5.362	1245	1251	1252	rVV2	597	598	0.03%	0.005%
28	5.375	1252	1255	1268	rVV5	1006	1548	0.09%	0.013%
29	5.510	1295	1297	1300	rBV2	285	205	0.01%	0.002%
30	5.613	1322	1329	1333	rBV2	230	220	0.01%	0.002%
31	5.722	1339	1363	1397	rBV2	653655	1742362	100.00%	14.369%
32	5.983	1440	1444	1449	rBV3	709	679	0.04%	0.006%
33	6.070	1469	1471	1475	rBV3	221	168	0.01%	0.001%
34	6.112	1480	1484	1491	rVB4	337	392	0.02%	0.003%
35	6.150	1493	1496	1499	rBV	269	168	0.01%	0.001%
36	6.250	1508	1527	1557	rBV	415199	791311	45.42%	6.526%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050425.D
 Acq On : 24 Aug 2022 15:00
 Operator : SY/MD
 Sample : VU0824WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.401	1572	1574	1577	rVB2	315	181	0.01%	0.001%
38	6.491	1597	1602	1604	rVB4	337	292	0.02%	0.002%
39	6.533	1608	1615	1622	rVB6	2034	3364	0.19%	0.028%
40	6.584	1627	1631	1634	rBV3	216	213	0.01%	0.002%
41	6.690	1649	1664	1687	rBV	406308	791589	45.43%	6.528%
42	6.809	1696	1701	1704	rBV5	652	629	0.04%	0.005%
43	7.063	1777	1780	1784	rVB	249	183	0.01%	0.002%
44	7.111	1792	1795	1797	rBV	299	177	0.01%	0.001%
45	7.173	1806	1814	1816	rBV3	567	639	0.04%	0.005%
46	7.269	1837	1844	1847	rVB2	161	214	0.01%	0.002%
47	7.308	1853	1856	1859	rBV	250	164	0.01%	0.001%
48	7.439	1892	1897	1899	rBV	223	215	0.01%	0.002%
49	7.565	1923	1936	1958	rBV	201726	354512	20.35%	2.924%
50	7.732	1986	1988	1991	rBV2	311	165	0.01%	0.001%
51	7.899	2026	2040	2062	rBV	731438	1267816	72.76%	10.456%
52	8.111	2103	2106	2108	rBV3	372	227	0.01%	0.002%
53	8.179	2113	2127	2146	rBV	137611	234244	13.44%	1.932%
54	8.385	2188	2191	2195	rVB	508	396	0.02%	0.003%
55	8.446	2207	2210	2213	rBV	294	189	0.01%	0.002%
56	8.504	2225	2228	2232	rVB2	400	289	0.02%	0.002%
57	8.552	2240	2243	2248	rVB3	607	498	0.03%	0.004%
58	8.584	2248	2253	2257	rBV3	396	359	0.02%	0.003%
59	8.636	2257	2269	2316	rBV2	433209	934321	53.62%	7.705%
60	8.925	2356	2359	2362	rVV3	510	252	0.01%	0.002%
61	8.983	2375	2377	2381	rVB2	299	207	0.01%	0.002%
62	9.031	2386	2392	2395	rBV2	328	345	0.02%	0.003%
63	9.108	2413	2416	2420	rBV2	298	240	0.01%	0.002%
64	9.127	2420	2422	2428	rBV2	311	172	0.01%	0.001%
65	9.163	2429	2433	2437	rBV3	243	262	0.02%	0.002%
66	9.259	2459	2463	2466	rBV2	291	253	0.01%	0.002%
67	9.417	2498	2512	2540	rBV	587668	982821	56.41%	8.105%
68	9.642	2578	2582	2586	rBV2	296	228	0.01%	0.002%
69	9.700	2593	2600	2606	rBV4	941	1234	0.07%	0.010%
70	9.941	2671	2675	2678	rBV	374	249	0.01%	0.002%
71	10.115	2723	2729	2730	rBV2	736	721	0.04%	0.006%
72	10.205	2755	2757	2762	rVB2	269	160	0.01%	0.001%
73	10.298	2783	2786	2788	rBV	245	183	0.01%	0.002%
74	10.333	2792	2797	2800	rBV2	349	362	0.02%	0.003%
75	10.484	2839	2844	2851	rVB4	803	1079	0.06%	0.009%
76	10.754	2915	2928	2955	rBV	561793	916291	52.59%	7.557%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050425.D
 Acq On : 24 Aug 2022 15:00
 Operator : SY/MD
 Sample : VU0824WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.931	2980	2983	2986	rVB2	355	216	0.01%	0.002%
78	11.092	3027	3033	3041	rVV4	901	1223	0.07%	0.010%
79	11.388	3121	3125	3130	rBV2	237	200	0.01%	0.002%
80	11.414	3130	3133	3134	rBV	295	185	0.01%	0.002%
81	11.423	3134	3136	3139	rVB2	315	173	0.01%	0.001%
82	11.468	3145	3150	3153	rBV3	858	919	0.05%	0.008%
83	11.748	3229	3237	3244	rBV4	2009	2674	0.15%	0.022%
84	11.812	3244	3257	3283	rBV	447003	735005	42.18%	6.062%
85	11.983	3307	3310	3314	rVB2	522	375	0.02%	0.003%
86	12.008	3314	3318	3321	rBV3	414	392	0.02%	0.003%
87	12.192	3362	3375	3395	rBV	598135	977562	56.11%	8.062%
88	12.442	3451	3453	3458	rVB4	375	313	0.02%	0.003%
89	12.684	3526	3528	3532	rBV2	252	161	0.01%	0.001%
90	12.787	3556	3560	3563	rBV3	545	411	0.02%	0.003%
91	12.989	3621	3623	3626	rBV3	290	195	0.01%	0.002%
92	13.005	3626	3628	3630	rBV2	495	194	0.01%	0.002%
93	13.221	3690	3695	3705	rBV3	3111	4476	0.26%	0.037%
94	13.343	3725	3733	3738	rBV3	514	834	0.05%	0.007%
95	13.783	3867	3870	3876	rBV2	407	500	0.03%	0.004%
96	13.848	3880	3890	3900	rVB3	6429	10166	0.58%	0.084%
97	14.047	3949	3952	3955	rVB2	647	484	0.03%	0.004%
98	14.092	3955	3966	3981	rBV	12906	23004	1.32%	0.190%
99	14.333	4033	4041	4051	rVB3	7590	11273	0.65%	0.093%
100	15.159	4296	4298	4302	rBV3	508	292	0.02%	0.002%




Sum of corrected areas: 12125782

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050425.D
Acq On : 24 Aug 2022 15:00
Operator : SY/MD
Sample : VU0824WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

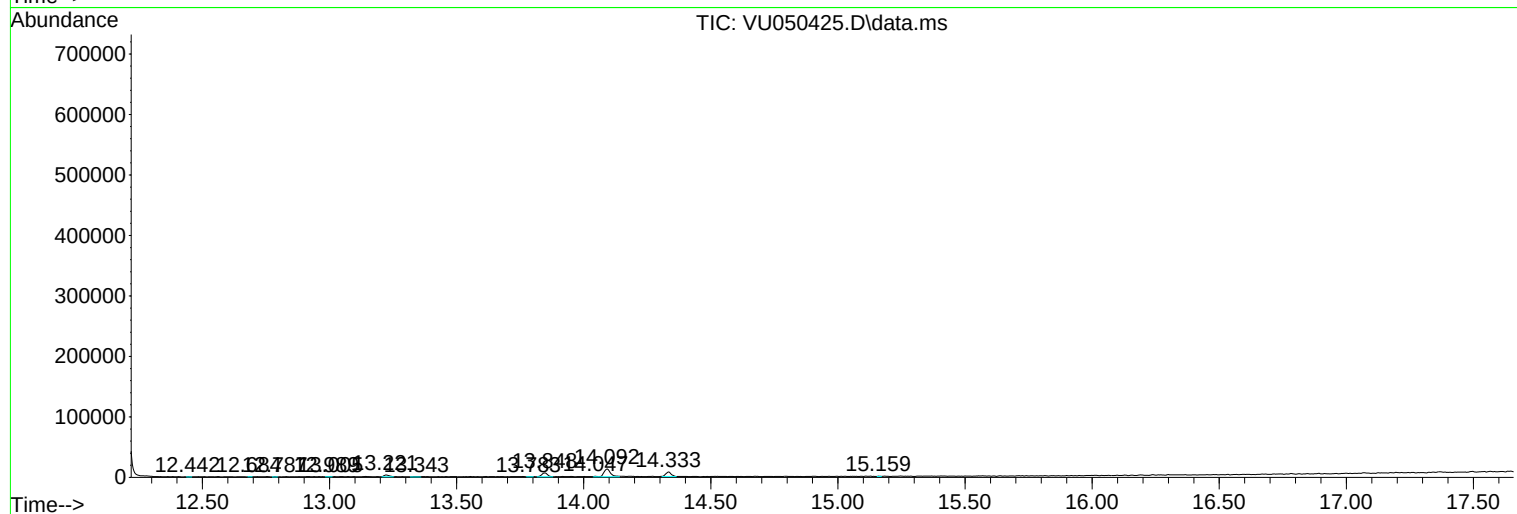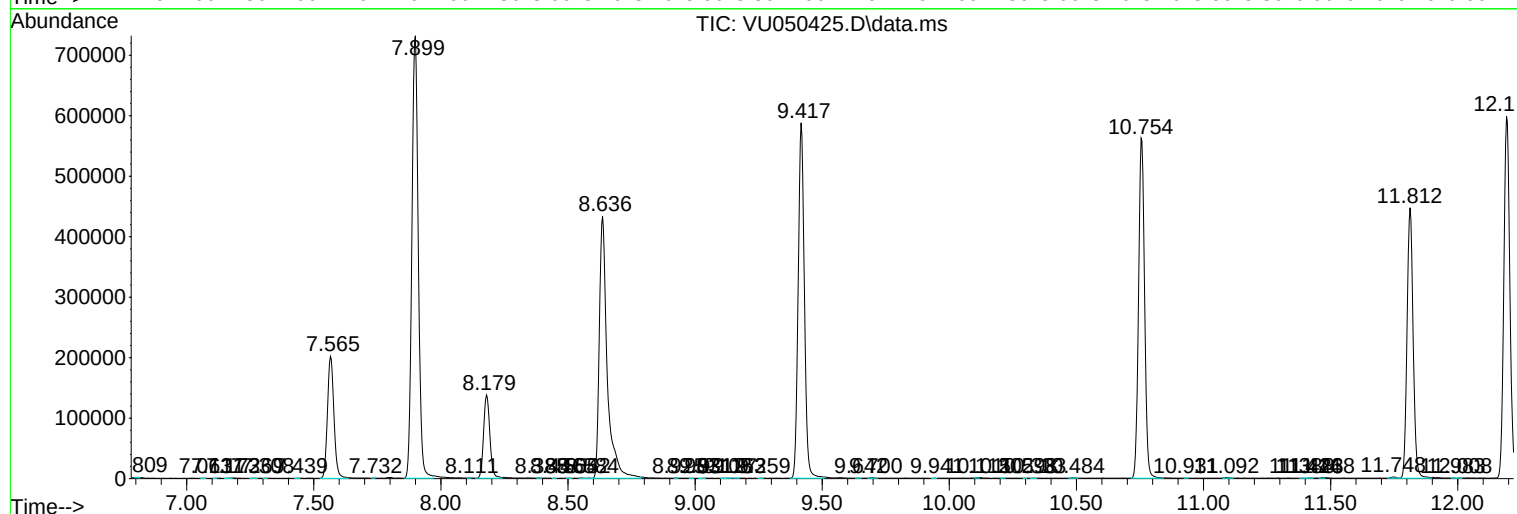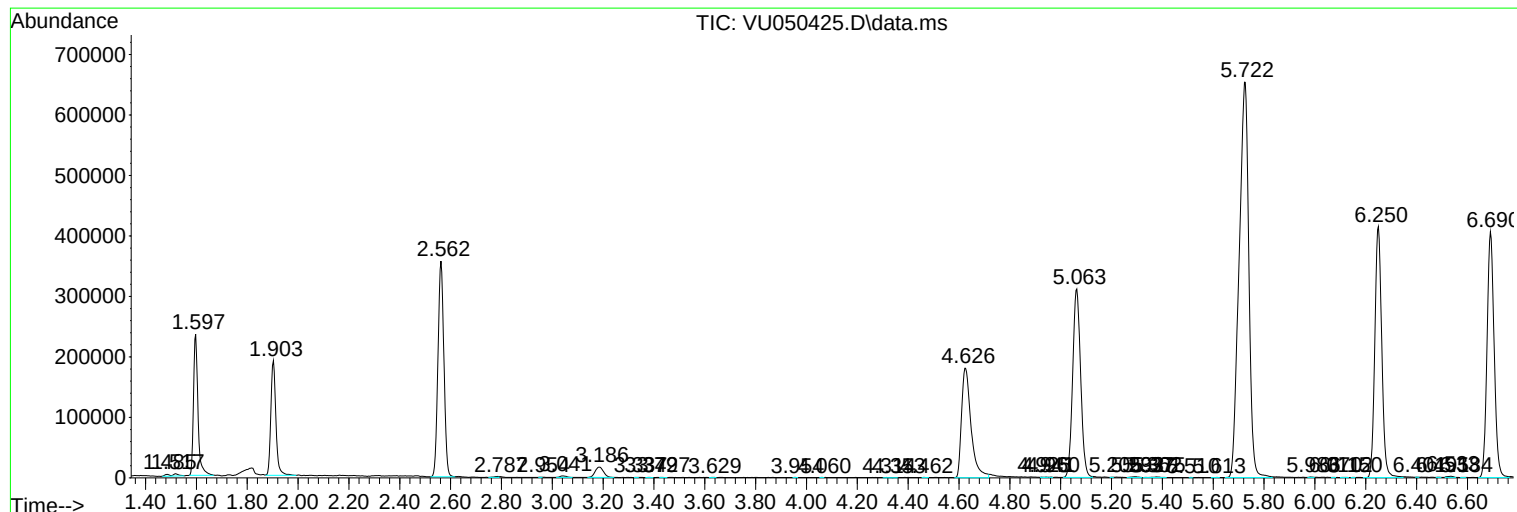

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050425.D
Acq On : 24 Aug 2022 15:00
Operator : SY/MD
Sample : VU0824WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050425.D
Acq On : 24 Aug 2022 15:00
Operator : SY/MD
Sample : VU0824WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------