

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050426.D
 Acq On : 24 Aug 2022 15:24
 Operator : SY/MD
 Sample : N4319-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COZH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	50	rBV2	3391	3510	0.21%	0.029%
2	1.517	50	55	67	rBV2	4775	7236	0.43%	0.060%
3	1.597	72	80	98	rBV	231386	277262	16.31%	2.306%
4	1.906	167	176	198	rVB	188368	253297	14.90%	2.106%
5	2.562	367	380	394	rBV	345752	559752	32.93%	4.655%
6	2.629	395	401	418	rVB	6135	11065	0.65%	0.092%
7	2.755	436	440	441	rBV2	676	462	0.03%	0.004%
8	2.774	443	446	447	rVV2	1695	1172	0.07%	0.010%
9	2.787	447	450	462	rVB4	2520	3569	0.21%	0.030%
10	3.044	523	530	537	rVB4	1244	1693	0.10%	0.014%
11	3.128	553	556	560	rBV2	236	193	0.01%	0.002%
12	3.186	560	574	588	rVB	4750	10809	0.64%	0.090%
13	3.314	604	614	616	rBV	269	333	0.02%	0.003%
14	3.346	622	624	634	rVB3	290	372	0.02%	0.003%
15	3.391	634	638	643	rVB2	313	286	0.02%	0.002%
16	3.433	648	651	657	rVB2	216	200	0.01%	0.002%
17	3.475	657	664	666	rBV	255	285	0.02%	0.002%
18	3.523	676	679	686	rVB	319	315	0.02%	0.003%
19	3.578	692	696	700	rVV3	505	496	0.03%	0.004%
20	4.105	856	860	865	rBV2	335	325	0.02%	0.003%
21	4.292	911	918	920	rBV	386	371	0.02%	0.003%
22	4.356	933	938	941	rBV2	215	198	0.01%	0.002%
23	4.436	960	963	966	rVV2	388	372	0.02%	0.003%
24	4.523	983	990	992	rBV	313	319	0.02%	0.003%
25	4.623	1004	1021	1042	rBV	176381	439258	25.84%	3.653%
26	5.063	1141	1158	1182	rBV	316239	690832	40.64%	5.745%
27	5.288	1220	1228	1241	rVB7	1833	3748	0.22%	0.031%
28	5.378	1249	1256	1270	rVB3	1198	2280	0.13%	0.019%
29	5.491	1288	1291	1296	rVB2	273	237	0.01%	0.002%
30	5.526	1296	1302	1304	rBV3	372	400	0.02%	0.003%
31	5.600	1322	1325	1331	rVB2	249	234	0.01%	0.002%
32	5.726	1341	1364	1385	rBV2	634459	1699831	100.00%	14.135%
33	5.944	1429	1432	1435	rVB3	279	201	0.01%	0.002%
34	5.977	1440	1442	1448	rVB3	294	279	0.02%	0.002%
35	6.038	1456	1461	1464	rBV3	510	548	0.03%	0.005%
36	6.083	1471	1475	1477	rBV2	376	310	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050426.D
 Acq On : 24 Aug 2022 15:24
 Operator : SY/MD
 Sample : N4319-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COZH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.198	1507	1511	1512	rBV	296	194	0.01%	0.002%
38	6.250	1512	1527	1555	rBV	418861	795540	46.80%	6.616%
39	6.485	1596	1600	1603	rVB2	594	435	0.03%	0.004%
40	6.533	1607	1615	1625	rVB7	1459	3008	0.18%	0.025%
41	6.591	1625	1633	1635	rBV3	508	600	0.04%	0.005%
42	6.690	1649	1664	1693	rBV	397850	777255	45.73%	6.463%
43	6.796	1693	1697	1699	rBV4	591	541	0.03%	0.004%
44	6.886	1722	1725	1736	rVB5	911	997	0.06%	0.008%
45	6.957	1741	1747	1749	rBV3	251	236	0.01%	0.002%
46	7.057	1769	1778	1780	rBV3	365	382	0.02%	0.003%
47	7.182	1810	1817	1818	rBV2	481	471	0.03%	0.004%
48	7.565	1923	1936	1955	rBV	197568	349161	20.54%	2.904%
49	7.716	1979	1983	1985	rBV	254	202	0.01%	0.002%
50	7.796	1998	2008	2020	rVB4	3368	5921	0.35%	0.049%
51	7.899	2022	2040	2070	rBV	715632	1243672	73.16%	10.342%
52	8.179	2115	2127	2150	rBV2	136689	232827	13.70%	1.936%
53	8.401	2194	2196	2202	rVB3	526	488	0.03%	0.004%
54	8.433	2202	2206	2210	rBV4	475	586	0.03%	0.005%
55	8.507	2226	2229	2237	rVB3	518	515	0.03%	0.004%
56	8.549	2237	2242	2243	rBV3	414	307	0.02%	0.003%
57	8.636	2256	2269	2299	rBV2	430050	939264	55.26%	7.811%
58	8.787	2310	2316	2327	rVB2	12642	19890	1.17%	0.165%
59	8.976	2371	2375	2377	rBV2	335	256	0.02%	0.002%
60	9.034	2389	2393	2395	rBV2	344	271	0.02%	0.002%
61	9.214	2444	2449	2452	rBV2	280	242	0.01%	0.002%
62	9.417	2499	2512	2547	rBV	582186	983381	57.85%	8.178%
63	9.571	2554	2560	2563	rBV4	748	778	0.05%	0.006%
64	9.603	2566	2570	2577	rVB3	567	724	0.04%	0.006%
65	9.697	2593	2599	2606	rVB3	873	1247	0.07%	0.010%
66	9.732	2606	2610	2616	rBV2	274	329	0.02%	0.003%
67	10.021	2691	2700	2703	rBV	270	366	0.02%	0.003%
68	10.041	2703	2706	2712	rVV	221	216	0.01%	0.002%
69	10.082	2712	2719	2736	rVB5	2836	6179	0.36%	0.051%
70	10.150	2736	2740	2745	rBV2	261	318	0.02%	0.003%
71	10.243	2756	2769	2776	rBV5	994	2008	0.12%	0.017%
72	10.282	2779	2781	2787	rVB2	470	458	0.03%	0.004%
73	10.314	2787	2791	2794	rBV	390	327	0.02%	0.003%
74	10.353	2798	2803	2807	rVV2	926	921	0.05%	0.008%
75	10.565	2866	2869	2875	rVB3	257	241	0.01%	0.002%
76	10.600	2875	2880	2884	rBV2	268	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050426.D
 Acq On : 24 Aug 2022 15:24
 Operator : SY/MD
 Sample : N4319-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.658	2895	2898	2902	rBV2	297	254	0.01%	0.002%
78	10.697	2906	2910	2913	rBV2	294	258	0.02%	0.002%
79	10.758	2915	2929	2950	rBV	567722	913826	53.76%	7.599%
80	10.886	2966	2969	2972	rVV2	450	356	0.02%	0.003%
81	10.941	2984	2986	2989	rBV	246	195	0.01%	0.002%
82	11.481	3145	3154	3156	rBV3	1249	1633	0.10%	0.014%
83	11.745	3232	3236	3244	rBV3	1091	1219	0.07%	0.010%
84	11.812	3244	3257	3276	rBV	467269	750469	44.15%	6.241%
85	12.070	3330	3337	3352	rVB5	3828	6831	0.40%	0.057%
86	12.195	3363	3376	3402	rBV	593805	975112	57.37%	8.109%
87	12.385	3432	3435	3439	rVB2	548	419	0.02%	0.003%
88	12.462	3456	3459	3460	rBV	427	255	0.02%	0.002%
89	12.516	3473	3476	3477	rBV2	544	324	0.02%	0.003%
90	12.899	3589	3595	3599	rBV4	854	816	0.05%	0.007%
91	13.028	3632	3635	3639	rBV2	622	434	0.03%	0.004%
92	13.166	3675	3678	3682	rVB3	544	383	0.02%	0.003%
93	13.221	3687	3695	3702	rBV7	1901	2839	0.17%	0.024%
94	13.272	3709	3711	3717	rBV2	502	606	0.04%	0.005%
95	13.423	3754	3758	3763	rBV3	529	575	0.03%	0.005%
96	13.848	3884	3890	3899	rVB4	3690	5679	0.33%	0.047%
97	14.092	3958	3966	3979	rBV	7801	12204	0.72%	0.101%
98	14.333	4034	4041	4052	rBV4	4607	6959	0.41%	0.058%
99	14.667	4143	4145	4147	rBV2	385	211	0.01%	0.002%
100	15.343	4353	4355	4358	rBV3	561	394	0.02%	0.003%




Sum of corrected areas: 12025337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050426.D
Acq On : 24 Aug 2022 15:24
Operator : SY/MD
Sample : N4319-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

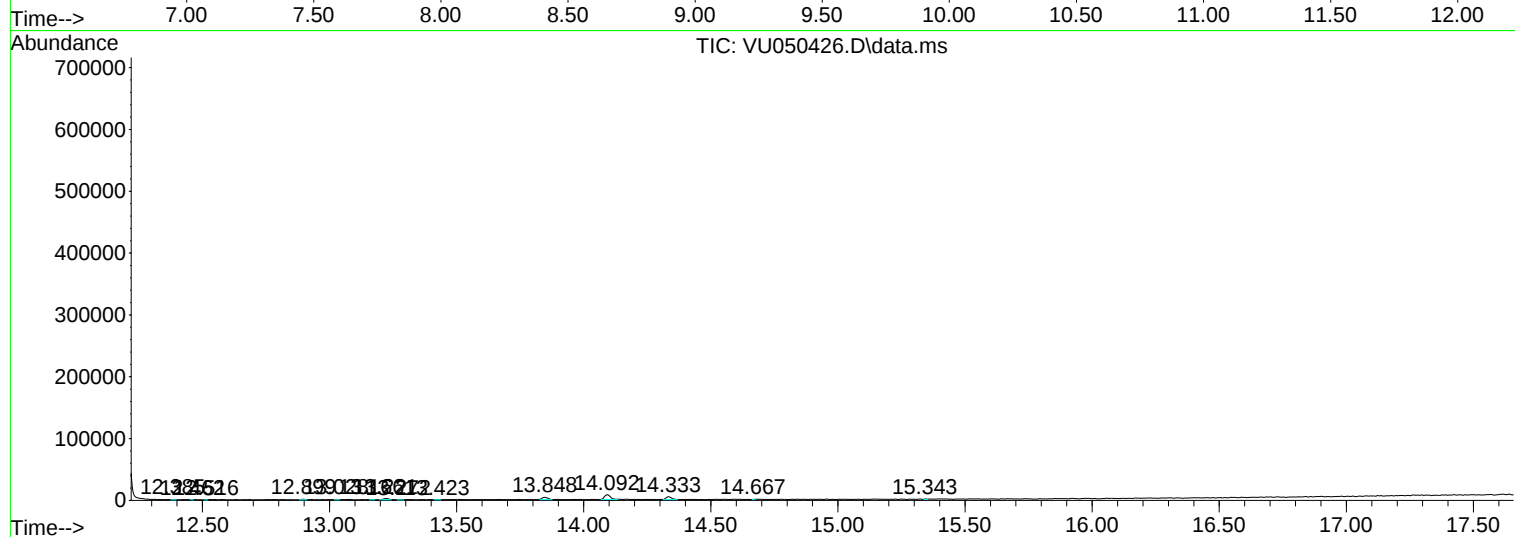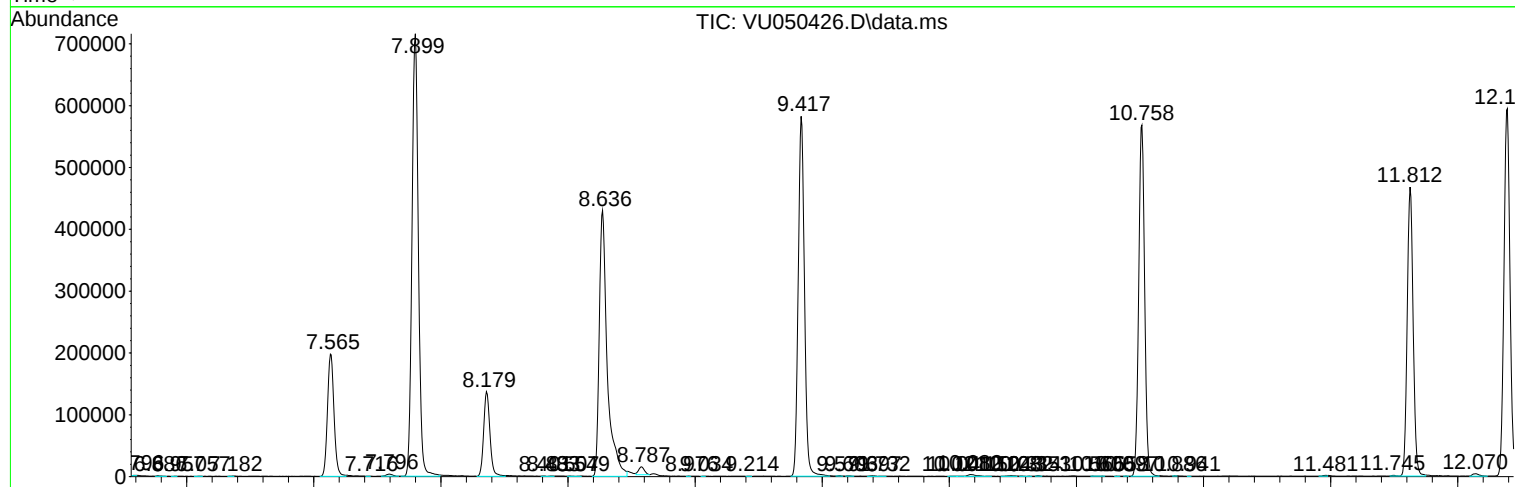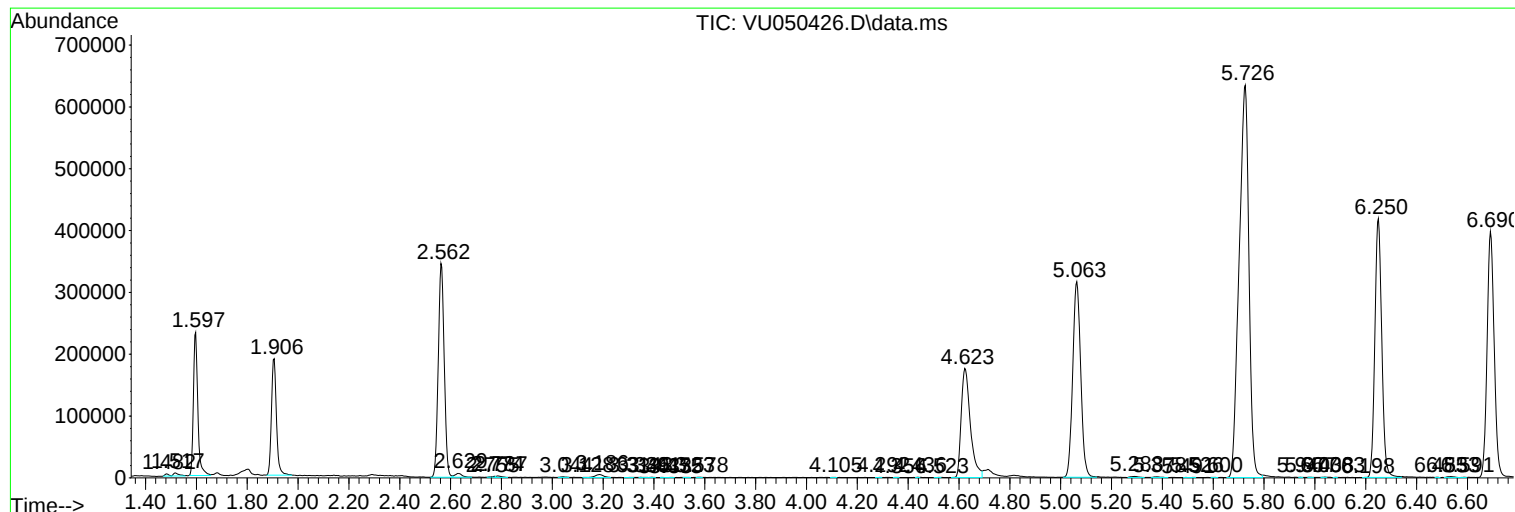

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050426.D
Acq On : 24 Aug 2022 15:24
Operator : SY/MD
Sample : N4319-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050426.D
Acq On : 24 Aug 2022 15:24
Operator : SY/MD
Sample : N4319-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc