

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050427.D
 Acq On : 24 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4319-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COZH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rVB3	3548	3676	0.22%	0.031%
2	1.517	50	55	68	rBV	4949	7959	0.47%	0.067%
3	1.597	72	80	101	rBV	227506	279950	16.55%	2.359%
4	1.900	165	174	185	rBV	177028	238287	14.08%	2.008%
5	2.562	367	380	395	rBV	344653	554870	32.80%	4.677%
6	2.726	429	431	439	rBV2	308	297	0.02%	0.003%
7	2.774	441	446	448	rBV3	674	737	0.04%	0.006%
8	2.874	474	477	480	rBV2	238	206	0.01%	0.002%
9	2.954	497	502	506	rBV2	376	480	0.03%	0.004%
10	2.986	510	512	515	rVB2	439	237	0.01%	0.002%
11	3.038	523	528	540	rVB4	1205	1910	0.11%	0.016%
12	3.131	550	557	561	rBV3	276	372	0.02%	0.003%
13	3.186	562	574	585	rVV2	2556	5432	0.32%	0.046%
14	3.369	628	631	635	rVB2	328	294	0.02%	0.002%
15	3.633	711	713	718	rVB	355	221	0.01%	0.002%
16	3.874	782	788	791	rBV3	382	439	0.03%	0.004%
17	3.912	797	800	803	rBV	290	186	0.01%	0.002%
18	4.012	828	831	835	rVB2	342	250	0.01%	0.002%
19	4.035	835	838	841	rBV2	287	266	0.02%	0.002%
20	4.234	894	900	905	rBV2	270	415	0.02%	0.003%
21	4.289	914	917	923	rBV2	170	184	0.01%	0.002%
22	4.337	928	932	936	rVB2	245	202	0.01%	0.002%
23	4.375	941	944	947	rBV2	228	168	0.01%	0.001%
24	4.430	957	961	963	rBV2	309	177	0.01%	0.001%
25	4.443	963	965	968	rBV	313	186	0.01%	0.002%
26	4.623	1008	1021	1042	rBV	179528	440794	26.05%	3.715%
27	4.996	1134	1137	1141	rBV2	269	210	0.01%	0.002%
28	5.060	1141	1157	1180	rBV	312309	686107	40.55%	5.783%
29	5.288	1222	1228	1230	rBV2	932	906	0.05%	0.008%
30	5.301	1230	1232	1243	rVB4	1608	1573	0.09%	0.013%
31	5.372	1243	1254	1255	rBV2	872	1066	0.06%	0.009%
32	5.542	1301	1307	1315	rVB2	283	353	0.02%	0.003%
33	5.578	1315	1318	1323	rBV2	214	216	0.01%	0.002%
34	5.610	1323	1328	1332	rVB	292	269	0.02%	0.002%
35	5.726	1341	1364	1394	rBV2	622942	1691902	100.00%	14.260%
36	5.967	1436	1439	1441	rBV	394	250	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050427.D
 Acq On : 24 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4319-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.041	1459	1462	1463	rBV2	469	315	0.02%	0.003%
38	6.141	1492	1493	1498	rVB	437	233	0.01%	0.002%
39	6.166	1498	1501	1502	rBV	340	201	0.01%	0.002%
40	6.250	1512	1527	1550	rBV	402680	771785	45.62%	6.505%
41	6.440	1583	1586	1587	rBV	279	170	0.01%	0.001%
42	6.488	1598	1601	1602	rBV	432	243	0.01%	0.002%
43	6.533	1610	1615	1622	rVB5	1256	1761	0.10%	0.015%
44	6.562	1622	1624	1626	rBV	273	166	0.01%	0.001%
45	6.626	1639	1644	1649	rBV	329	288	0.02%	0.002%
46	6.690	1649	1664	1690	rBV	401524	773963	45.75%	6.523%
47	6.784	1690	1693	1695	rBV3	694	414	0.02%	0.003%
48	6.880	1720	1723	1724	rBV	397	178	0.01%	0.002%
49	7.022	1764	1767	1772	rVB	317	244	0.01%	0.002%
50	7.250	1834	1838	1840	rVV2	256	205	0.01%	0.002%
51	7.349	1864	1869	1872	rBV	204	209	0.01%	0.002%
52	7.427	1889	1893	1901	rBV	278	367	0.02%	0.003%
53	7.513	1915	1920	1922	rBV	388	350	0.02%	0.003%
54	7.565	1924	1936	1958	rVV	196623	346523	20.48%	2.921%
55	7.700	1975	1978	1982	rVV2	343	253	0.01%	0.002%
56	7.716	1982	1983	1988	rVB4	507	336	0.02%	0.003%
57	7.742	1988	1991	1993	rBV3	295	200	0.01%	0.002%
58	7.793	2000	2007	2008	rBV4	2837	2652	0.16%	0.022%
59	7.899	2024	2040	2063	rBV	716729	1233024	72.88%	10.392%
60	8.179	2115	2127	2144	rBV	136154	225875	13.35%	1.904%
61	8.433	2203	2206	2209	rBV2	403	251	0.01%	0.002%
62	8.636	2256	2269	2307	rBV2	450492	952613	56.30%	8.029%
63	8.790	2311	2317	2327	rVB2	11039	16938	1.00%	0.143%
64	8.906	2351	2353	2358	rVB3	480	279	0.02%	0.002%
65	9.005	2378	2384	2388	rBV2	653	774	0.05%	0.007%
66	9.417	2498	2512	2532	rBV	570832	957230	56.58%	8.068%
67	9.571	2557	2560	2568	rVB4	736	780	0.05%	0.007%
68	9.623	2573	2576	2580	rBV3	238	206	0.01%	0.002%
69	9.697	2594	2599	2603	rBV3	742	824	0.05%	0.007%
70	9.803	2628	2632	2634	rVB2	404	322	0.02%	0.003%
71	9.931	2668	2672	2674	rBV	269	204	0.01%	0.002%
72	9.957	2677	2680	2685	rVV	229	210	0.01%	0.002%
73	10.086	2712	2720	2727	rBV4	2779	4448	0.26%	0.037%
74	10.243	2762	2769	2777	rVB5	1054	1630	0.10%	0.014%
75	10.346	2795	2801	2807	rBV4	1207	1206	0.07%	0.010%
76	10.398	2812	2817	2818	rBV	261	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050427.D
 Acq On : 24 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4319-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.697	2908	2910	2916	rVB2	302	188	0.01%	0.002%
78	10.758	2916	2929	2949	rBV	562547	921112	54.44%	7.763%
79	11.147	3048	3050	3056	rBV2	353	313	0.02%	0.003%
80	11.301	3095	3098	3100	rBV	336	186	0.01%	0.002%
81	11.410	3129	3132	3134	rBV	353	219	0.01%	0.002%
82	11.468	3145	3150	3151	rBV3	813	742	0.04%	0.006%
83	11.562	3173	3179	3181	rBV2	287	319	0.02%	0.003%
84	11.748	3229	3237	3242	rBV4	803	1188	0.07%	0.010%
85	11.812	3245	3257	3285	rBV	449395	725601	42.89%	6.116%
86	12.070	3327	3337	3347	rBV6	4233	7966	0.47%	0.067%
87	12.195	3362	3376	3393	rBV	592032	967535	57.19%	8.155%
88	12.471	3459	3462	3465	rBV2	280	193	0.01%	0.002%
89	12.491	3466	3468	3472	rVB2	550	352	0.02%	0.003%
90	12.536	3479	3482	3484	rBV2	378	226	0.01%	0.002%
91	12.816	3566	3569	3572	rBV	442	305	0.02%	0.003%
92	12.841	3575	3577	3581	rVB2	487	294	0.02%	0.002%
93	12.899	3589	3595	3597	rBV2	813	693	0.04%	0.006%
94	12.951	3608	3611	3615	rVB3	507	403	0.02%	0.003%
95	13.224	3693	3696	3712	rVB5	1379	1900	0.11%	0.016%
96	13.442	3761	3764	3770	rBV3	359	410	0.02%	0.003%
97	13.738	3854	3856	3859	rBV2	459	294	0.02%	0.002%
98	13.848	3883	3890	3901	rBV5	2664	3810	0.23%	0.032%
99	14.092	3960	3966	3979	rVB2	4675	6992	0.41%	0.059%
100	14.336	4035	4042	4051	rVB6	2842	4556	0.27%	0.038%




Sum of corrected areas: 11864940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050427.D
Acq On : 24 Aug 2022 15:48
Operator : SY/MD
Sample : N4319-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

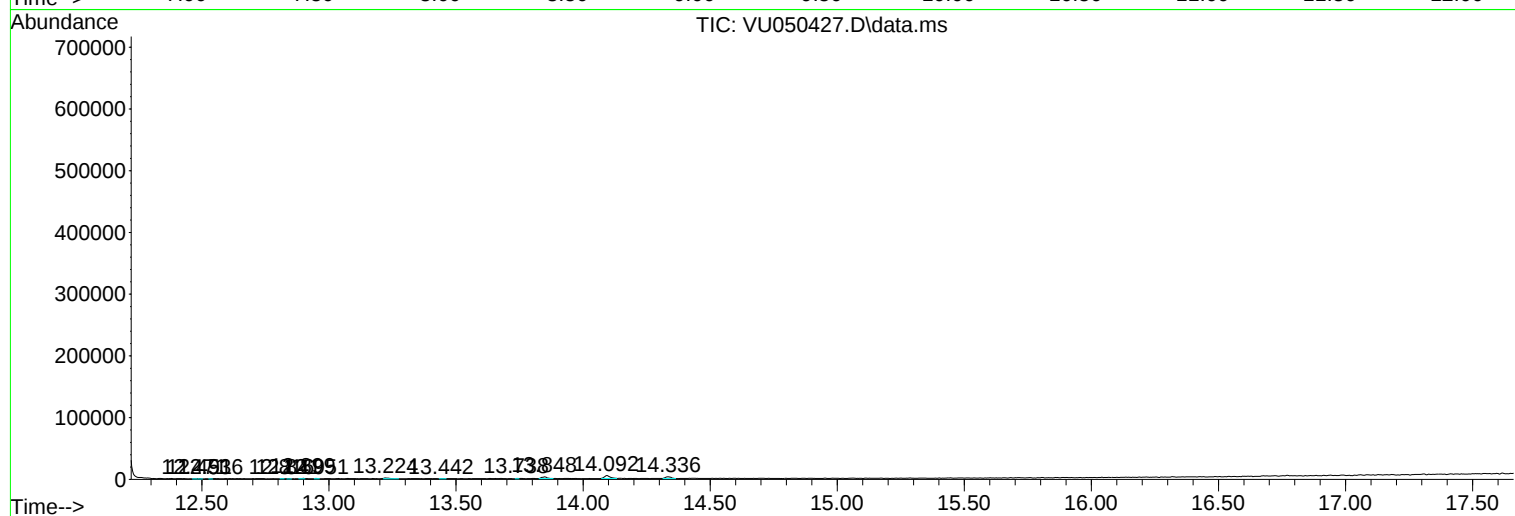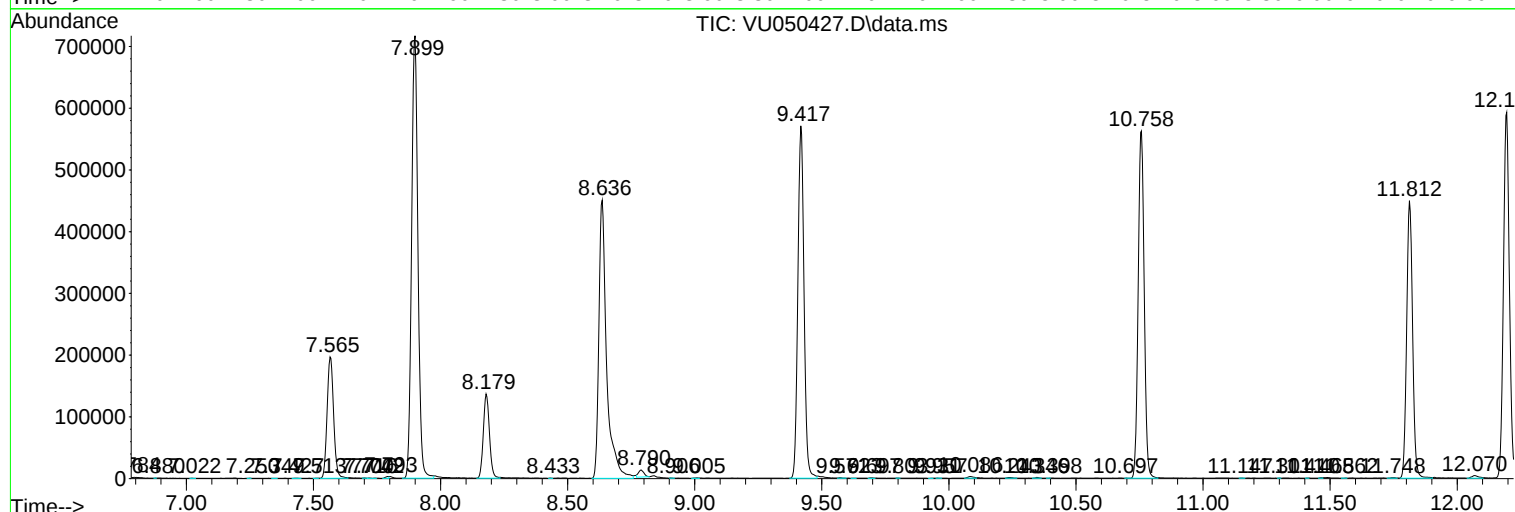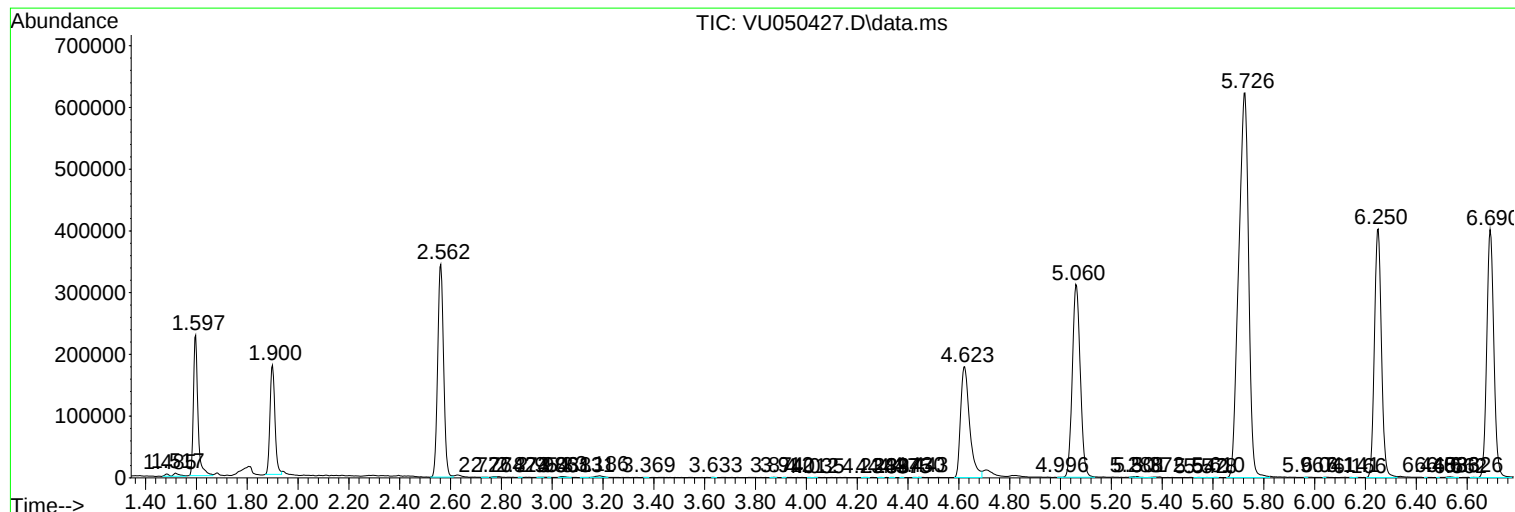

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050427.D
Acq On : 24 Aug 2022 15:48
Operator : SY/MD
Sample : N4319-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050427.D
Acq On : 24 Aug 2022 15:48
Operator : SY/MD
Sample : N4319-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc