

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050429.D
 Acq On : 24 Aug 2022 16:48
 Operator : SY/MD
 Sample : N4322-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV3	3438	3989	0.24%	0.034%
2	1.517	51	55	64	rVV3	2879	4631	0.28%	0.040%
3	1.594	72	79	103	rBV	223504	269297	16.12%	2.326%
4	1.903	167	175	195	rVB	182359	243164	14.56%	2.101%
5	2.292	288	296	313	rVB	20077	38030	2.28%	0.329%
6	2.562	367	380	398	rBV	333430	535287	32.05%	4.624%
7	2.771	430	445	460	rBV2	11811	26271	1.57%	0.227%
8	2.919	488	491	496	rVB	335	277	0.02%	0.002%
9	3.038	524	528	530	rBV3	853	724	0.04%	0.006%
10	3.092	542	545	552	rVB2	215	198	0.01%	0.002%
11	3.125	552	555	557	rBV2	273	179	0.01%	0.002%
12	3.182	563	573	589	rVB	5976	12171	0.73%	0.105%
13	3.440	648	653	657	rBV2	334	303	0.02%	0.003%
14	3.520	672	678	682	rBV2	251	232	0.01%	0.002%
15	3.642	714	716	720	rVV3	215	184	0.01%	0.002%
16	3.726	739	742	745	rVB2	367	240	0.01%	0.002%
17	3.755	745	751	753	rBV2	194	208	0.01%	0.002%
18	4.002	822	828	831	rBV	216	225	0.01%	0.002%
19	4.263	903	909	911	rBV2	183	187	0.01%	0.002%
20	4.346	931	935	939	rBV2	182	183	0.01%	0.002%
21	4.424	954	959	964	rVB2	276	258	0.02%	0.002%
22	4.623	1008	1021	1052	rBV	176945	443799	26.57%	3.834%
23	5.063	1140	1158	1184	rBV	301538	659355	39.48%	5.696%
24	5.292	1220	1229	1239	rVB2	1488	2398	0.14%	0.021%
25	5.375	1248	1255	1263	rVB3	1324	2067	0.12%	0.018%
26	5.427	1268	1271	1275	rBV2	249	181	0.01%	0.002%
27	5.726	1342	1364	1396	rBV2	622132	1670099	100.00%	14.427%
28	5.989	1442	1446	1452	rBV3	488	530	0.03%	0.005%
29	6.022	1452	1456	1460	rVB3	369	253	0.02%	0.002%
30	6.044	1460	1463	1466	rBV2	554	392	0.02%	0.003%
31	6.112	1481	1484	1491	rVB3	383	440	0.03%	0.004%
32	6.250	1513	1527	1554	rBV	401989	764509	45.78%	6.604%
33	6.385	1566	1569	1570	rBV3	385	226	0.01%	0.002%
34	6.404	1573	1575	1579	rVV3	464	228	0.01%	0.002%
35	6.491	1596	1602	1608	rVB3	411	511	0.03%	0.004%
36	6.539	1608	1617	1627	rBV8	6008	12687	0.76%	0.110%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050429.D
 Acq On : 24 Aug 2022 16:48
 Operator : SY/MD
 Sample : N4322-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1689	rBV2	396132	763493	45.72%	6.596%
38	6.800	1696	1698	1702	rBV2	655	520	0.03%	0.004%
39	6.989	1755	1757	1762	rVB2	326	206	0.01%	0.002%
40	7.169	1810	1813	1817	rVB2	440	349	0.02%	0.003%
41	7.195	1817	1821	1831	rBV3	447	725	0.04%	0.006%
42	7.243	1831	1836	1839	rBV	235	172	0.01%	0.001%
43	7.288	1846	1850	1852	rBV	370	242	0.01%	0.002%
44	7.378	1871	1878	1881	rBV	210	237	0.01%	0.002%
45	7.420	1888	1891	1895	rVB2	348	228	0.01%	0.002%
46	7.452	1895	1901	1904	rBV2	170	189	0.01%	0.002%
47	7.565	1924	1936	1960	rBV	190677	335760	20.10%	2.901%
48	7.755	1993	1995	1999	rVB	305	216	0.01%	0.002%
49	7.793	1999	2007	2008	rBV3	512	358	0.02%	0.003%
50	7.899	2024	2040	2061	rBV	680738	1184318	70.91%	10.231%
51	8.179	2115	2127	2148	rBV	132876	224494	13.44%	1.939%
52	8.475	2216	2219	2221	rVV2	343	228	0.01%	0.002%
53	8.549	2238	2242	2244	rBV3	352	291	0.02%	0.003%
54	8.636	2252	2269	2311	rBV2	438247	942807	56.45%	8.145%
55	8.870	2339	2342	2345	rBV2	412	296	0.02%	0.003%
56	8.902	2348	2352	2356	rBV3	474	348	0.02%	0.003%
57	8.925	2356	2359	2363	rVB2	341	235	0.01%	0.002%
58	9.005	2381	2384	2388	rVB2	326	186	0.01%	0.002%
59	9.070	2399	2404	2407	rBV3	217	217	0.01%	0.002%
60	9.269	2461	2466	2469	rBV2	289	303	0.02%	0.003%
61	9.417	2498	2512	2533	rBV	561691	939310	56.24%	8.114%
62	9.690	2593	2597	2598	rBV2	387	286	0.02%	0.002%
63	9.832	2637	2641	2645	rBV2	231	193	0.01%	0.002%
64	9.864	2645	2651	2655	rVB2	303	315	0.02%	0.003%
65	10.124	2730	2732	2737	rVB2	491	342	0.02%	0.003%
66	10.484	2840	2844	2849	rBV2	365	411	0.02%	0.004%
67	10.513	2850	2853	2860	rVV2	176	194	0.01%	0.002%
68	10.584	2873	2875	2879	rVB2	354	220	0.01%	0.002%
69	10.626	2885	2888	2893	rVB	259	182	0.01%	0.002%
70	10.677	2899	2904	2908	rVB2	193	212	0.01%	0.002%
71	10.758	2916	2929	2950	rBV	546963	898170	53.78%	7.759%
72	10.896	2969	2972	2978	rVB3	366	366	0.02%	0.003%
73	10.925	2978	2981	2986	rVB	522	284	0.02%	0.002%
74	11.169	3054	3057	3064	rBV2	314	244	0.01%	0.002%
75	11.205	3064	3068	3069	rBV2	381	236	0.01%	0.002%
76	11.336	3105	3109	3111	rBV	241	210	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050429.D
 Acq On : 24 Aug 2022 16:48
 Operator : SY/MD
 Sample : N4322-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.410	3129	3132	3137	rVB3	447	278	0.02%	0.002%
78	11.568	3173	3181	3184	rBV2	341	497	0.03%	0.004%
79	11.745	3233	3236	3238	rBV2	460	336	0.02%	0.003%
80	11.812	3245	3257	3278	rBV	418937	675293	40.43%	5.834%
81	11.963	3301	3304	3310	rVB4	460	374	0.02%	0.003%
82	12.076	3332	3339	3348	rVB4	943	1376	0.08%	0.012%
83	12.192	3362	3375	3397	rBV	535160	897136	53.72%	7.750%
84	12.500	3469	3471	3473	rBV	293	180	0.01%	0.002%
85	12.555	3485	3488	3492	rBV	565	432	0.03%	0.004%
86	12.713	3535	3537	3541	rVB2	385	193	0.01%	0.002%
87	12.774	3552	3556	3559	rBV2	445	305	0.02%	0.003%
88	12.819	3567	3570	3573	rBV	354	245	0.01%	0.002%
89	12.848	3575	3579	3581	rBV2	388	295	0.02%	0.003%
90	12.896	3591	3594	3596	rBV2	338	198	0.01%	0.002%
91	13.034	3635	3637	3639	rBV2	355	202	0.01%	0.002%
92	13.160	3672	3676	3679	rBV3	388	348	0.02%	0.003%
93	13.513	3782	3786	3790	rBV2	404	428	0.03%	0.004%
94	13.648	3824	3828	3833	rVB3	548	488	0.03%	0.004%
95	13.848	3885	3890	3896	rBV2	1528	1747	0.10%	0.015%
96	14.095	3958	3967	3968	rBV3	1698	1929	0.12%	0.017%
97	14.195	3994	3998	4005	rBV3	478	718	0.04%	0.006%
98	14.883	4209	4212	4216	rBV	546	406	0.02%	0.004%
99	15.240	4320	4323	4327	rBV3	1030	744	0.04%	0.006%
100	15.282	4334	4336	4340	rBV3	534	268	0.02%	0.002%




Sum of corrected areas: 11575922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050429.D
Acq On : 24 Aug 2022 16:48
Operator : SY/MD
Sample : N4322-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY172

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

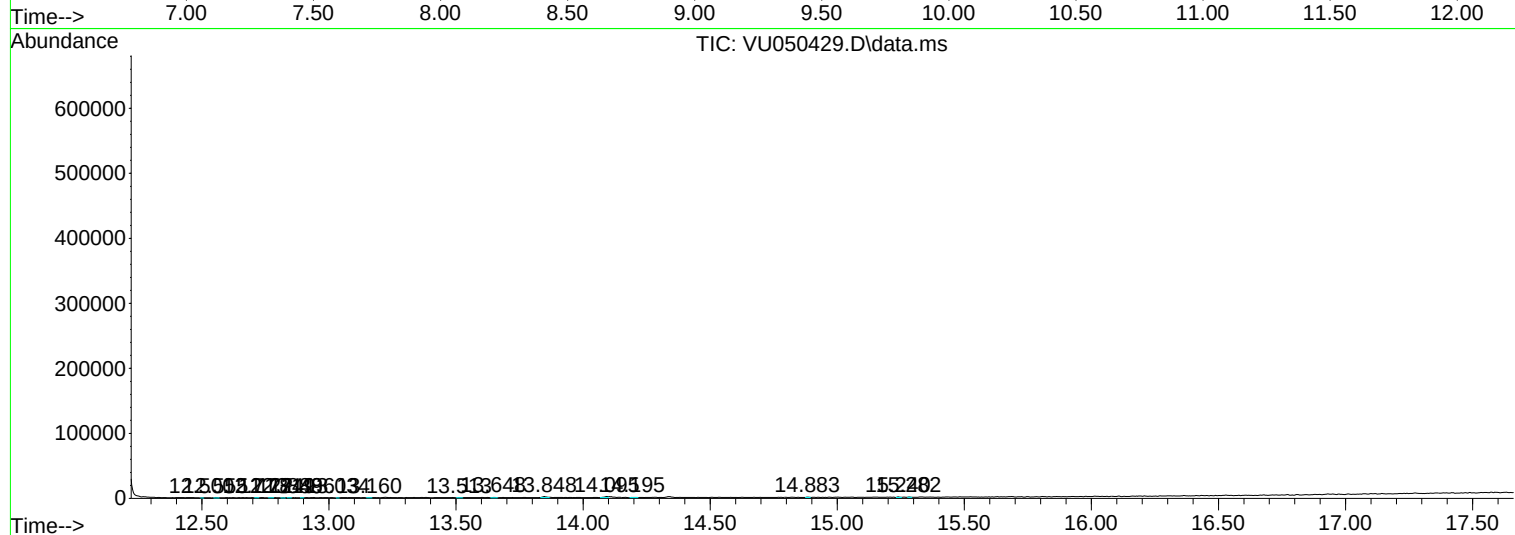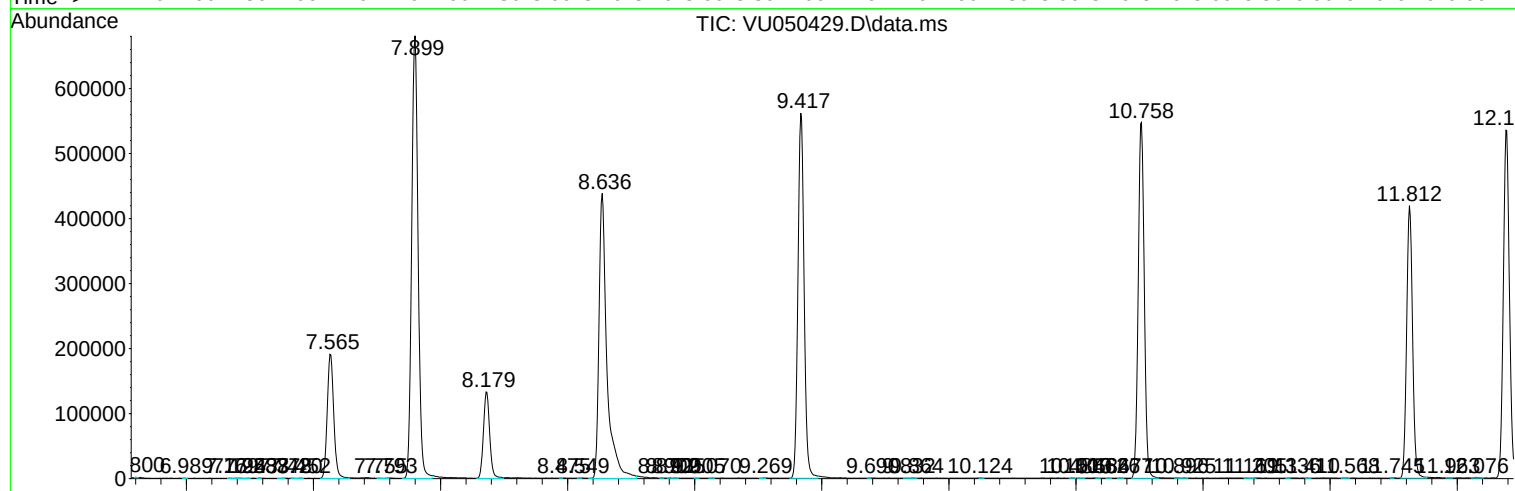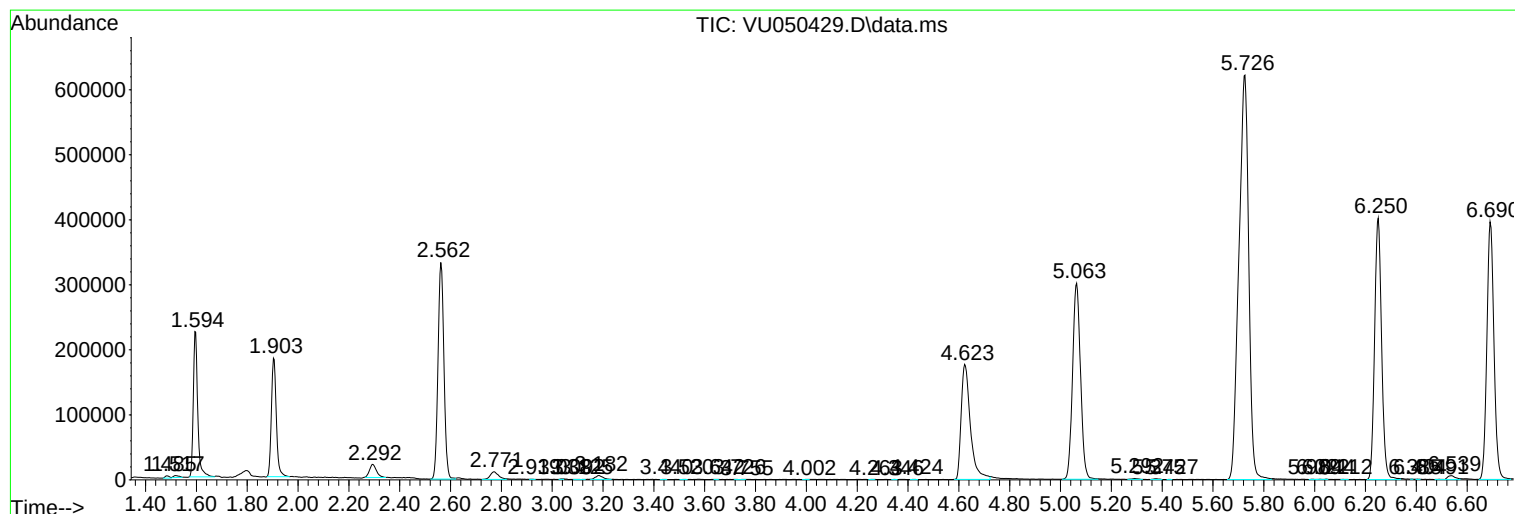

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050429.D
Acq On : 24 Aug 2022 16:48
Operator : SY/MD
Sample : N4322-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY172

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050429.D
Acq On : 24 Aug 2022 16:48
Operator : SY/MD
Sample : N4322-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY172

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc