

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050430.D
 Acq On : 24 Aug 2022 17:12
 Operator : SY/MD
 Sample : N4322-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	3218	3372	0.20%	0.029%
2	1.517	50	55	66	rVV	3862	5345	0.32%	0.046%
3	1.594	72	79	102	rBV	220979	269162	16.08%	2.313%
4	1.900	165	174	189	rBV	182473	240526	14.37%	2.067%
5	2.562	367	380	394	rBV	333903	536326	32.05%	4.608%
6	2.739	432	435	437	rBV	242	191	0.01%	0.002%
7	2.777	437	447	458	rBV3	3649	8269	0.49%	0.071%
8	2.919	483	491	496	rBV3	350	538	0.03%	0.005%
9	3.035	523	527	528	rBV2	747	465	0.03%	0.004%
10	3.112	548	551	557	rVB2	307	341	0.02%	0.003%
11	3.183	562	573	587	rVV2	2998	6541	0.39%	0.056%
12	3.343	617	623	625	rBV	338	297	0.02%	0.003%
13	3.388	631	637	640	rBV	242	205	0.01%	0.002%
14	3.414	640	645	649	rVV2	311	235	0.01%	0.002%
15	3.539	678	684	686	rBV	304	319	0.02%	0.003%
16	3.681	723	728	733	rBV2	225	310	0.02%	0.003%
17	3.707	733	736	739	rVV2	275	240	0.01%	0.002%
18	3.729	739	743	746	rVV2	336	308	0.02%	0.003%
19	3.893	787	794	798	rBV2	195	239	0.01%	0.002%
20	3.922	798	803	811	rVB2	242	423	0.03%	0.004%
21	3.957	811	814	818	rBV2	370	240	0.01%	0.002%
22	4.022	829	834	840	rVB2	234	287	0.02%	0.002%
23	4.086	849	854	859	rBV	230	217	0.01%	0.002%
24	4.166	872	879	883	rBV2	303	285	0.02%	0.002%
25	4.366	936	941	946	rBV2	202	229	0.01%	0.002%
26	4.623	1008	1021	1046	rBV	179061	449140	26.84%	3.859%
27	4.967	1125	1128	1134	rBV	471	390	0.02%	0.003%
28	5.063	1140	1158	1181	rBV	304425	664318	39.70%	5.708%
29	5.292	1219	1229	1238	rVB5	1570	3149	0.19%	0.027%
30	5.356	1246	1249	1250	rBV2	353	189	0.01%	0.002%
31	5.369	1250	1253	1258	rVV2	569	359	0.02%	0.003%
32	5.723	1339	1363	1396	rBV2	626965	1673505	100.00%	14.379%
33	5.964	1435	1438	1440	rBV	322	212	0.01%	0.002%
34	6.115	1479	1485	1488	rBV3	459	453	0.03%	0.004%
35	6.166	1499	1501	1506	rVB	317	243	0.01%	0.002%
36	6.250	1511	1527	1556	rBV	404260	775719	46.35%	6.665%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050430.D
 Acq On : 24 Aug 2022 17:12
 Operator : SY/MD
 Sample : N4322-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.362	1560	1562	1565	rVB3	452	305	0.02%	0.003%
38	6.526	1609	1613	1614	rBV2	1141	805	0.05%	0.007%
39	6.690	1648	1664	1689	rBV	393197	766415	45.80%	6.585%
40	6.870	1714	1720	1721	rBV2	354	256	0.02%	0.002%
41	7.009	1756	1763	1765	rBV2	346	293	0.02%	0.003%
42	7.041	1772	1773	1778	rVB2	360	204	0.01%	0.002%
43	7.160	1804	1810	1812	rBV3	358	356	0.02%	0.003%
44	7.192	1814	1820	1827	rVV4	670	1071	0.06%	0.009%
45	7.356	1864	1871	1874	rBV2	171	204	0.01%	0.002%
46	7.469	1901	1906	1909	rBV2	231	237	0.01%	0.002%
47	7.491	1909	1913	1916	rVV2	378	234	0.01%	0.002%
48	7.565	1923	1936	1961	rBV	193672	338651	20.24%	2.910%
49	7.716	1974	1983	1988	rBV6	1642	2517	0.15%	0.022%
50	7.800	2003	2009	2014	rVB2	295	326	0.02%	0.003%
51	7.899	2025	2040	2068	rBV	689755	1199847	71.70%	10.309%
52	8.121	2103	2109	2112	rBV2	311	322	0.02%	0.003%
53	8.179	2115	2127	2142	rBV	131490	219961	13.14%	1.890%
54	8.375	2185	2188	2193	rVB2	391	297	0.02%	0.003%
55	8.398	2193	2195	2200	rVB2	241	195	0.01%	0.002%
56	8.636	2257	2269	2312	rBV2	463645	973657	58.18%	8.366%
57	8.838	2329	2332	2336	rBV3	312	245	0.01%	0.002%
58	8.861	2336	2339	2344	rVB3	697	600	0.04%	0.005%
59	8.890	2344	2348	2351	rBV2	275	272	0.02%	0.002%
60	8.948	2363	2366	2373	rVB2	377	310	0.02%	0.003%
61	9.067	2400	2403	2410	rVB2	214	255	0.02%	0.002%
62	9.144	2424	2427	2430	rVV	434	319	0.02%	0.003%
63	9.169	2433	2435	2440	rVB3	386	299	0.02%	0.003%
64	9.198	2440	2444	2447	rVB2	456	309	0.02%	0.003%
65	9.234	2447	2455	2461	rBV2	385	642	0.04%	0.006%
66	9.417	2499	2512	2549	rBV	565731	945644	56.51%	8.125%
67	9.755	2610	2617	2627	rBV3	912	2044	0.12%	0.018%
68	9.906	2659	2664	2667	rBV2	215	207	0.01%	0.002%
69	9.954	2675	2679	2683	rVB3	256	234	0.01%	0.002%
70	10.105	2723	2726	2730	rBV2	290	226	0.01%	0.002%
71	10.189	2747	2752	2757	rBV2	215	307	0.02%	0.003%
72	10.321	2789	2793	2797	rBV2	269	248	0.01%	0.002%
73	10.758	2915	2929	2950	rBV	553746	911449	54.46%	7.831%
74	10.874	2962	2965	2967	rBV2	315	199	0.01%	0.002%
75	11.275	3085	3090	3093	rVB	216	195	0.01%	0.002%
76	11.298	3093	3097	3104	rVB2	487	581	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050430.D
 Acq On : 24 Aug 2022 17:12
 Operator : SY/MD
 Sample : N4322-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.343	3104	3111	3116	rBV2	432	604	0.04%	0.005%
78	11.449	3141	3144	3148	rBV2	219	213	0.01%	0.002%
79	11.475	3148	3152	3154	rBV	310	232	0.01%	0.002%
80	11.639	3198	3203	3207	rBV	283	333	0.02%	0.003%
81	11.751	3232	3238	3244	rBV	392	325	0.02%	0.003%
82	11.812	3244	3257	3278	rBV	430898	690019	41.23%	5.929%
83	11.967	3302	3305	3310	rBV2	314	276	0.02%	0.002%
84	12.079	3333	3340	3343	rBV3	1557	1664	0.10%	0.014%
85	12.195	3362	3376	3394	rBV	564626	922557	55.13%	7.927%
86	12.346	3420	3423	3426	rBV4	536	433	0.03%	0.004%
87	12.738	3541	3545	3552	rVB3	406	436	0.03%	0.004%
88	12.941	3605	3608	3614	rVB	671	555	0.03%	0.005%
89	12.996	3622	3625	3629	rBV3	269	192	0.01%	0.002%
90	13.018	3629	3632	3635	rBV2	391	316	0.02%	0.003%
91	13.230	3694	3698	3701	rVV3	509	483	0.03%	0.004%
92	13.291	3714	3717	3718	rBV2	270	197	0.01%	0.002%
93	13.343	3728	3733	3736	rBV2	380	397	0.02%	0.003%
94	13.504	3780	3783	3786	rVB	507	295	0.02%	0.003%
95	13.529	3786	3791	3793	rBV2	378	336	0.02%	0.003%
96	13.854	3885	3892	3898	rBV5	1021	1352	0.08%	0.012%
97	14.098	3961	3968	3977	rBV3	1509	2497	0.15%	0.021%
98	14.324	4035	4038	4040	rBV	630	397	0.02%	0.003%
99	15.568	4423	4425	4431	rBV3	944	864	0.05%	0.007%
100	15.696	4462	4465	4468	rBV3	838	515	0.03%	0.004%




Sum of corrected areas: 11638813

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050430.D
Acq On : 24 Aug 2022 17:12
Operator : SY/MD
Sample : N4322-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

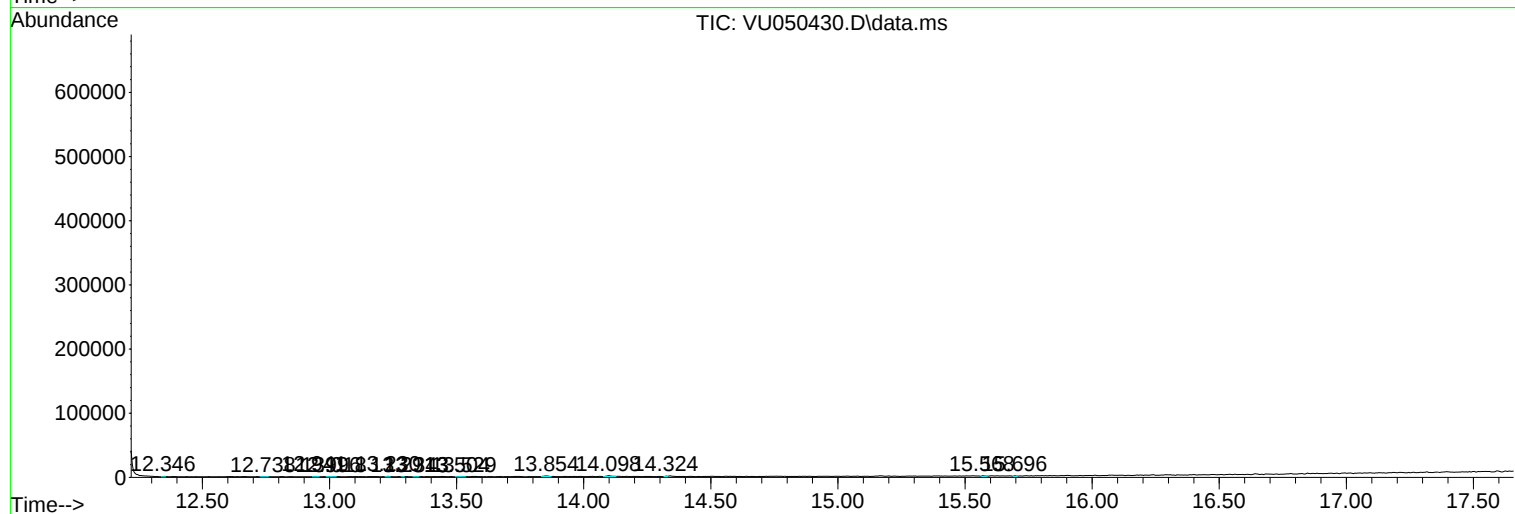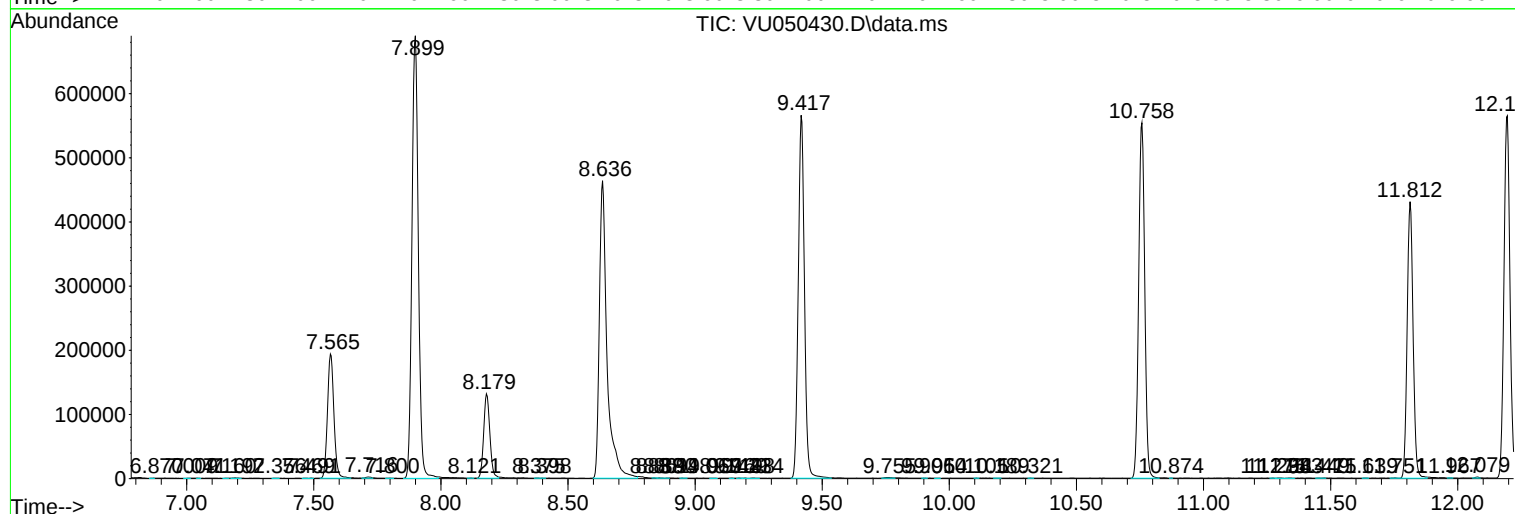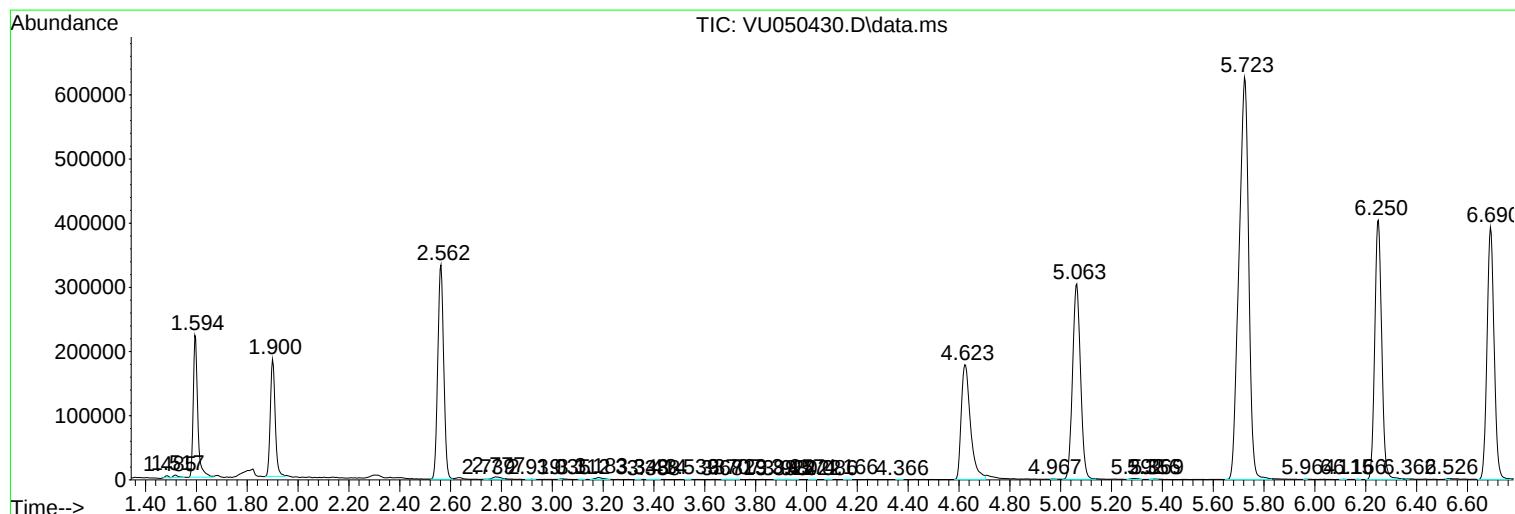

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050430.D
Acq On : 24 Aug 2022 17:12
Operator : SY/MD
Sample : N4322-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050430.D
Acq On : 24 Aug 2022 17:12
Operator : SY/MD
Sample : N4322-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc