

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050431.D
 Acq On : 24 Aug 2022 17:36
 Operator : SY/MD
 Sample : N4322-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY174

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV2	2975	3241	0.20%	0.029%
2	1.597	72	80	103	rBV	203116	246987	15.30%	2.205%
3	1.903	166	175	198	rVB	170874	229861	14.24%	2.052%
4	2.562	367	380	396	rBV	306561	491468	30.45%	4.387%
5	2.787	439	450	459	rBV2	3101	7171	0.44%	0.064%
6	2.932	493	495	501	rVB3	268	233	0.01%	0.002%
7	2.960	501	504	506	rBV2	402	224	0.01%	0.002%
8	3.041	526	529	536	rVB3	851	997	0.06%	0.009%
9	3.089	536	544	547	rBV2	326	337	0.02%	0.003%
10	3.176	563	571	572	rBV4	1710	1831	0.11%	0.016%
11	3.340	620	622	627	rVB	379	234	0.01%	0.002%
12	3.507	669	674	677	rBV2	296	271	0.02%	0.002%
13	3.864	775	785	800	rVB4	1573	3516	0.22%	0.031%
14	3.928	800	805	807	rBV2	285	253	0.02%	0.002%
15	3.976	814	820	822	rBV	262	263	0.02%	0.002%
16	4.057	839	845	848	rBV2	242	245	0.02%	0.002%
17	4.414	950	956	959	rBV2	181	216	0.01%	0.002%
18	4.485	974	978	982	rBV2	295	288	0.02%	0.003%
19	4.562	997	1002	1008	rVB2	191	240	0.01%	0.002%
20	4.626	1008	1022	1056	rBV	173846	439306	27.22%	3.922%
21	4.896	1104	1106	1111	rBV3	323	293	0.02%	0.003%
22	5.063	1141	1158	1183	rBV	297710	696659	43.16%	6.219%
23	5.250	1213	1216	1220	rVB4	430	342	0.02%	0.003%
24	5.292	1220	1229	1232	rBV3	1570	2352	0.15%	0.021%
25	5.369	1249	1253	1254	rBV	515	354	0.02%	0.003%
26	5.462	1278	1282	1286	rBV2	311	302	0.02%	0.003%
27	5.520	1295	1300	1303	rBV	315	263	0.02%	0.002%
28	5.613	1323	1329	1331	rBV	288	245	0.02%	0.002%
29	5.726	1342	1364	1393	rBV2	595151	1614030	100.00%	14.408%
30	6.047	1459	1464	1470	rVB4	574	627	0.04%	0.006%
31	6.118	1480	1486	1489	rBV2	254	266	0.02%	0.002%
32	6.176	1496	1504	1509	rVB2	361	510	0.03%	0.005%
33	6.250	1509	1527	1554	rBV	388031	737487	45.69%	6.583%
34	6.401	1572	1574	1579	rVB2	335	244	0.02%	0.002%
35	6.436	1582	1585	1590	rVB2	503	457	0.03%	0.004%
36	6.484	1598	1600	1604	rVB	382	223	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050431.D
 Acq On : 24 Aug 2022 17:36
 Operator : SY/MD
 Sample : N4322-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY174

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.513	1607	1609	1610	rBV	377	212	0.01%	0.002%
38	6.539	1610	1617	1623	rVB5	1242	1839	0.11%	0.016%
39	6.594	1630	1634	1641	rBV3	554	648	0.04%	0.006%
40	6.690	1649	1664	1688	rBV	381447	743508	46.07%	6.637%
41	6.806	1695	1700	1707	rVB6	998	1080	0.07%	0.010%
42	6.864	1715	1718	1723	rVB2	325	229	0.01%	0.002%
43	6.893	1723	1727	1731	rBV2	341	277	0.02%	0.002%
44	7.005	1756	1762	1765	rVV2	281	265	0.02%	0.002%
45	7.050	1773	1776	1783	rVV2	209	205	0.01%	0.002%
46	7.111	1793	1795	1799	rVV2	314	220	0.01%	0.002%
47	7.192	1816	1820	1828	rVB2	786	760	0.05%	0.007%
48	7.295	1847	1852	1860	rVB2	221	329	0.02%	0.003%
49	7.343	1860	1867	1873	rBV2	257	312	0.02%	0.003%
50	7.565	1922	1936	1954	rBV	185672	325392	20.16%	2.905%
51	7.700	1974	1978	1979	rBV3	696	419	0.03%	0.004%
52	7.716	1979	1983	1987	rVB4	1367	1286	0.08%	0.011%
53	7.738	1987	1990	1993	rVB	351	228	0.01%	0.002%
54	7.767	1996	1999	2002	rVB2	423	268	0.02%	0.002%
55	7.799	2007	2009	2017	rVB2	405	359	0.02%	0.003%
56	7.899	2025	2040	2068	rBV	657886	1142852	70.81%	10.202%
57	8.179	2115	2127	2150	rBV	125167	216603	13.42%	1.934%
58	8.311	2165	2168	2171	rBV2	310	242	0.01%	0.002%
59	8.475	2215	2219	2225	rVB3	734	870	0.05%	0.008%
60	8.513	2225	2231	2234	rBV3	370	460	0.03%	0.004%
61	8.584	2248	2253	2257	rBV2	286	261	0.02%	0.002%
62	8.635	2257	2269	2314	rBV2	434969	931530	57.71%	8.316%
63	8.861	2337	2339	2341	rVV3	422	247	0.02%	0.002%
64	8.880	2343	2345	2349	rVV2	345	245	0.02%	0.002%
65	8.912	2351	2355	2359	rVV3	304	354	0.02%	0.003%
66	8.973	2369	2374	2379	rVB2	395	370	0.02%	0.003%
67	9.002	2379	2383	2386	rBV2	276	242	0.01%	0.002%
68	9.070	2400	2404	2410	rBV3	274	232	0.01%	0.002%
69	9.166	2431	2434	2441	rVB2	468	463	0.03%	0.004%
70	9.417	2499	2512	2532	rBV	538170	906578	56.17%	8.093%
71	10.185	2747	2751	2755	rBV3	234	209	0.01%	0.002%
72	10.356	2801	2804	2810	rBV2	264	264	0.02%	0.002%
73	10.420	2821	2824	2830	rBV2	220	227	0.01%	0.002%
74	10.658	2895	2898	2904	rVB2	330	292	0.02%	0.003%
75	10.690	2904	2908	2912	rBV2	278	296	0.02%	0.003%
76	10.758	2915	2929	2954	rBV	545431	887082	54.96%	7.919%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050431.D
 Acq On : 24 Aug 2022 17:36
 Operator : SY/MD
 Sample : N4322-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY174

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.896	2969	2972	2977	rVB2	551	365	0.02%	0.003%
78	10.918	2977	2979	2983	rBV2	318	301	0.02%	0.003%
79	11.086	3028	3031	3035	rBV3	413	377	0.02%	0.003%
80	11.195	3062	3065	3073	rBV	225	219	0.01%	0.002%
81	11.233	3073	3077	3082	rVV3	323	289	0.02%	0.003%
82	11.426	3131	3137	3138	rBV2	363	292	0.02%	0.003%
83	11.468	3146	3150	3156	rBV2	409	482	0.03%	0.004%
84	11.716	3224	3227	3229	rBV	351	205	0.01%	0.002%
85	11.812	3245	3257	3278	rBV	409923	657873	40.76%	5.873%
86	12.012	3313	3319	3322	rBV3	337	455	0.03%	0.004%
87	12.069	3330	3337	3348	rBV4	2367	3761	0.23%	0.034%
88	12.195	3362	3376	3394	rBV	542897	882157	54.66%	7.875%
89	12.365	3426	3429	3436	rBV4	520	604	0.04%	0.005%
90	12.503	3470	3472	3475	rVB	491	251	0.02%	0.002%
91	12.526	3475	3479	3483	rVB3	537	444	0.03%	0.004%
92	12.552	3483	3487	3491	rBV2	356	389	0.02%	0.003%
93	12.635	3509	3513	3520	rVB4	483	635	0.04%	0.006%
94	12.680	3523	3527	3529	rBV2	309	229	0.01%	0.002%
95	12.761	3548	3552	3555	rVB3	399	291	0.02%	0.003%
96	12.790	3555	3561	3568	rBV2	516	752	0.05%	0.007%
97	13.127	3662	3666	3668	rVB2	391	257	0.02%	0.002%
98	13.233	3697	3699	3705	rBV3	603	483	0.03%	0.004%
99	13.648	3823	3828	3832	rBV3	518	571	0.04%	0.005%
100	14.330	4037	4040	4044	rBV5	754	829	0.05%	0.007%




Sum of corrected areas: 11202102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050431.D
Acq On : 24 Aug 2022 17:36
Operator : SY/MD
Sample : N4322-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY174

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

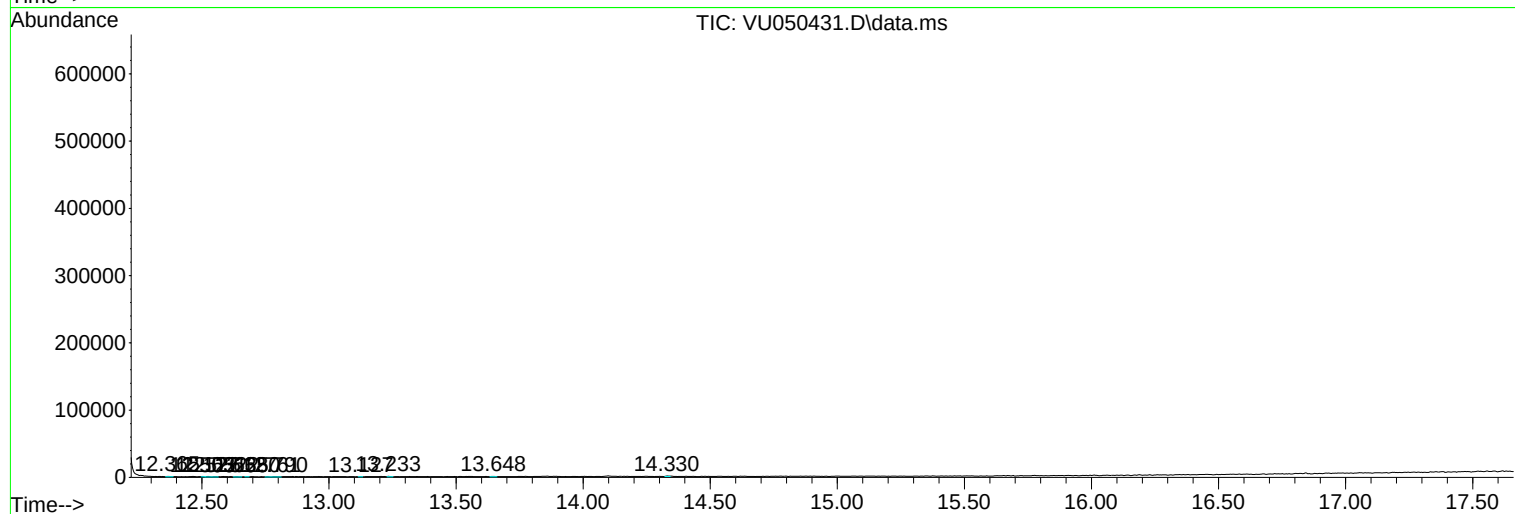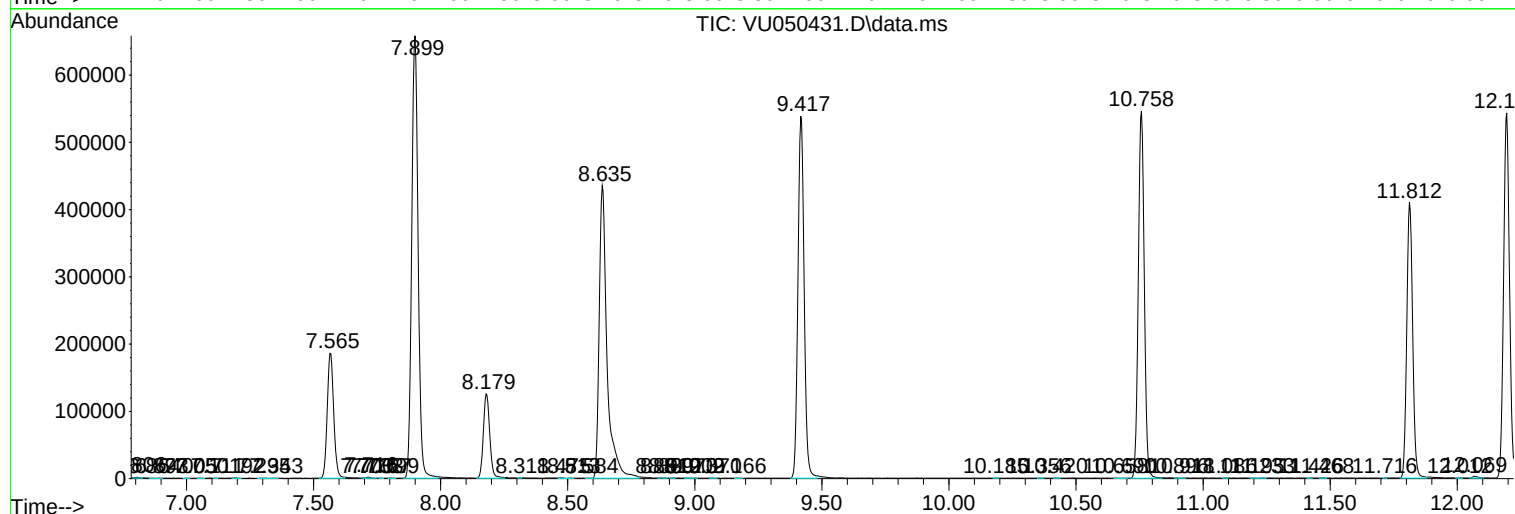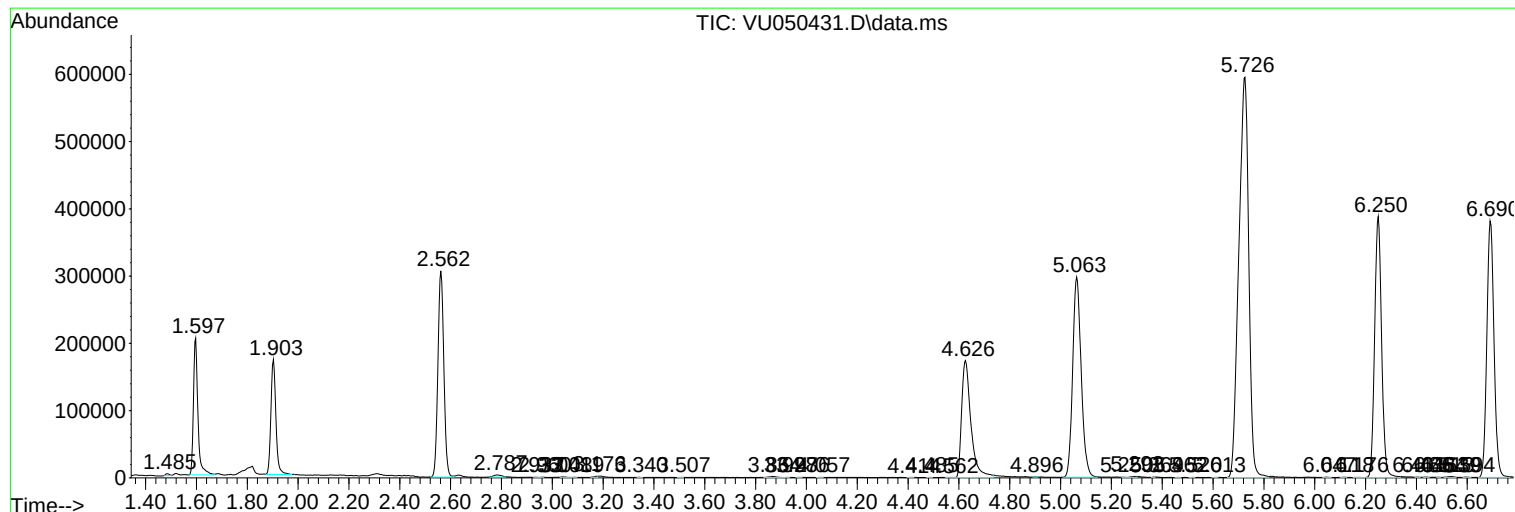

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050431.D
Acq On : 24 Aug 2022 17:36
Operator : SY/MD
Sample : N4322-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY174

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050431.D
Acq On : 24 Aug 2022 17:36
Operator : SY/MD
Sample : N4322-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY174

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc