

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050432.D
 Acq On : 24 Aug 2022 18:00
 Operator : SY/MD
 Sample : N4322-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY175

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	41	46	52	rBV2	4075	4217	0.27%	0.039%
2	1.597	72	80	102	rBV	193347	231417	14.91%	2.161%
3	1.900	166	174	196	rBV	156388	217344	14.00%	2.029%
4	2.289	285	295	304	rBV	5274	10457	0.67%	0.098%
5	2.562	368	380	394	rBV	275788	442698	28.52%	4.133%
6	2.729	428	432	433	rBV4	407	264	0.02%	0.002%
7	2.768	436	444	462	rVB3	4047	8795	0.57%	0.082%
8	2.858	468	472	475	rBV2	361	284	0.02%	0.003%
9	2.900	481	485	487	rBV3	358	244	0.02%	0.002%
10	3.041	524	529	536	rVV4	895	1084	0.07%	0.010%
11	3.157	560	565	566	rBV	768	605	0.04%	0.006%
12	3.186	566	574	590	rVB2	3200	6790	0.44%	0.063%
13	3.321	614	616	620	rVB2	317	196	0.01%	0.002%
14	3.356	624	627	631	rVB2	242	191	0.01%	0.002%
15	3.382	631	635	641	rBV2	212	184	0.01%	0.002%
16	3.488	665	668	673	rBV2	343	261	0.02%	0.002%
17	3.681	725	728	731	rVB2	246	175	0.01%	0.002%
18	4.202	883	890	895	rVB2	211	278	0.02%	0.003%
19	4.234	895	900	904	rVB2	211	208	0.01%	0.002%
20	4.327	920	929	932	rBV2	175	229	0.01%	0.002%
21	4.379	939	945	949	rBV2	189	207	0.01%	0.002%
22	4.623	1008	1021	1060	rBV	174743	434918	28.02%	4.061%
23	4.893	1102	1105	1109	rBV2	364	261	0.02%	0.002%
24	4.935	1115	1118	1127	rVB4	386	350	0.02%	0.003%
25	5.063	1138	1158	1187	rBV	279721	617882	39.81%	5.769%
26	5.260	1213	1219	1221	rBV3	442	396	0.03%	0.004%
27	5.295	1221	1230	1242	rVB5	1486	2657	0.17%	0.025%
28	5.379	1248	1256	1263	rVB5	1180	1947	0.13%	0.018%
29	5.491	1285	1291	1294	rBV2	193	194	0.01%	0.002%
30	5.620	1325	1331	1338	rVB2	204	241	0.02%	0.002%
31	5.726	1338	1364	1388	rBV2	572748	1552190	100.00%	14.493%
32	5.977	1439	1442	1447	rVB4	396	323	0.02%	0.003%
33	6.153	1494	1497	1502	rBV3	624	608	0.04%	0.006%
34	6.250	1513	1527	1556	rBV	372152	713439	45.96%	6.661%
35	6.526	1608	1613	1616	rBV2	834	856	0.06%	0.008%
36	6.623	1641	1643	1647	rVB2	383	195	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050432.D
 Acq On : 24 Aug 2022 18:00
 Operator : SY/MD
 Sample : N4322-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY175

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.690	1647	1664	1692	rBV	367682	724058	46.65%	6.760%
38	6.880	1719	1723	1724	rBV2	327	238	0.02%	0.002%
39	7.160	1804	1810	1811	rBV	463	346	0.02%	0.003%
40	7.176	1811	1815	1818	rBV4	245	228	0.01%	0.002%
41	7.440	1894	1897	1903	rVB2	387	392	0.03%	0.004%
42	7.488	1909	1912	1919	rVB	205	193	0.01%	0.002%
43	7.565	1923	1936	1955	rBV	177382	313509	20.20%	2.927%
44	7.710	1975	1981	1983	rBV3	1463	1553	0.10%	0.015%
45	7.796	2003	2008	2019	rVB2	646	875	0.06%	0.008%
46	7.842	2019	2022	2026	rBV2	243	257	0.02%	0.002%
47	7.899	2026	2040	2072	rBV	619262	1081724	69.69%	10.100%
48	8.179	2116	2127	2146	rBV	122778	206554	13.31%	1.929%
49	8.279	2154	2158	2162	rVB4	694	559	0.04%	0.005%
50	8.465	2207	2216	2219	rBV5	572	709	0.05%	0.007%
51	8.497	2223	2226	2230	rVB2	249	174	0.01%	0.002%
52	8.636	2253	2269	2310	rBV2	426526	907245	58.45%	8.471%
53	8.989	2374	2379	2380	rBV	380	246	0.02%	0.002%
54	9.047	2392	2397	2403	rVB2	216	306	0.02%	0.003%
55	9.417	2498	2512	2550	rBV	533461	895847	57.72%	8.364%
56	9.571	2557	2560	2567	rVB3	603	591	0.04%	0.006%
57	9.694	2593	2598	2606	rVV3	600	833	0.05%	0.008%
58	9.857	2646	2649	2651	rVV	313	206	0.01%	0.002%
59	9.874	2651	2654	2659	rVB2	279	176	0.01%	0.002%
60	9.973	2682	2685	2688	rVB	366	248	0.02%	0.002%
61	9.993	2688	2691	2695	rVB	230	179	0.01%	0.002%
62	10.021	2695	2700	2701	rBV	350	234	0.02%	0.002%
63	10.263	2772	2775	2778	rBV	209	177	0.01%	0.002%
64	10.333	2794	2797	2806	rBV2	228	270	0.02%	0.003%
65	10.369	2806	2808	2813	rVB2	295	211	0.01%	0.002%
66	10.472	2836	2840	2843	rBV	291	220	0.01%	0.002%
67	10.607	2880	2882	2888	rVB2	274	197	0.01%	0.002%
68	10.674	2900	2903	2908	rVB2	181	180	0.01%	0.002%
69	10.758	2914	2929	2948	rBV	530730	870782	56.10%	8.130%
70	10.874	2962	2965	2971	rBV2	334	271	0.02%	0.003%
71	10.983	2996	2999	3004	rVB2	366	308	0.02%	0.003%
72	11.009	3004	3007	3013	rVB	249	212	0.01%	0.002%
73	11.054	3013	3021	3024	rBV2	317	426	0.03%	0.004%
74	11.237	3072	3078	3080	rBV2	216	241	0.02%	0.002%
75	11.372	3117	3120	3126	rVB2	290	312	0.02%	0.003%
76	11.401	3126	3129	3131	rBV2	290	209	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050432.D
 Acq On : 24 Aug 2022 18:00
 Operator : SY/MD
 Sample : N4322-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY175

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.468	3147	3150	3153	rBV2	497	434	0.03%	0.004%
78	11.552	3173	3176	3178	rBV2	322	209	0.01%	0.002%
79	11.812	3245	3257	3276	rBV	381579	620320	39.96%	5.792%
80	12.063	3332	3335	3337	rBV3	912	706	0.05%	0.007%
81	12.192	3363	3375	3401	rBV	494535	817868	52.69%	7.636%
82	12.356	3423	3426	3428	rBV2	298	193	0.01%	0.002%
83	12.526	3475	3479	3481	rBV3	325	240	0.02%	0.002%
84	12.587	3495	3498	3500	rBV2	282	179	0.01%	0.002%
85	12.655	3515	3519	3522	rBV2	377	375	0.02%	0.004%
86	12.816	3565	3569	3572	rBV3	317	280	0.02%	0.003%
87	12.867	3582	3585	3588	rVB3	396	238	0.02%	0.002%
88	12.886	3588	3591	3594	rBV3	465	272	0.02%	0.003%
89	12.912	3597	3599	3604	rVB2	612	429	0.03%	0.004%
90	12.938	3605	3607	3610	rBV2	265	193	0.01%	0.002%
91	13.259	3705	3707	3710	rBV2	376	266	0.02%	0.002%
92	13.481	3774	3776	3778	rBV	413	262	0.02%	0.002%
93	13.520	3785	3788	3791	rVB3	439	280	0.02%	0.003%
94	13.639	3822	3825	3828	rBV2	361	345	0.02%	0.003%
95	13.777	3865	3868	3869	rBV	376	203	0.01%	0.002%
96	13.851	3888	3891	3900	rVB2	1020	1220	0.08%	0.011%
97	13.983	3930	3932	3935	rVB3	398	225	0.01%	0.002%
98	14.063	3954	3957	3961	rVB3	518	315	0.02%	0.003%
99	14.343	4039	4044	4045	rBV2	684	591	0.04%	0.006%
100	15.452	4385	4389	4390	rBV2	753	535	0.03%	0.005%




Sum of corrected areas: 10710259

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050432.D
Acq On : 24 Aug 2022 18:00
Operator : SY/MD
Sample : N4322-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY175

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

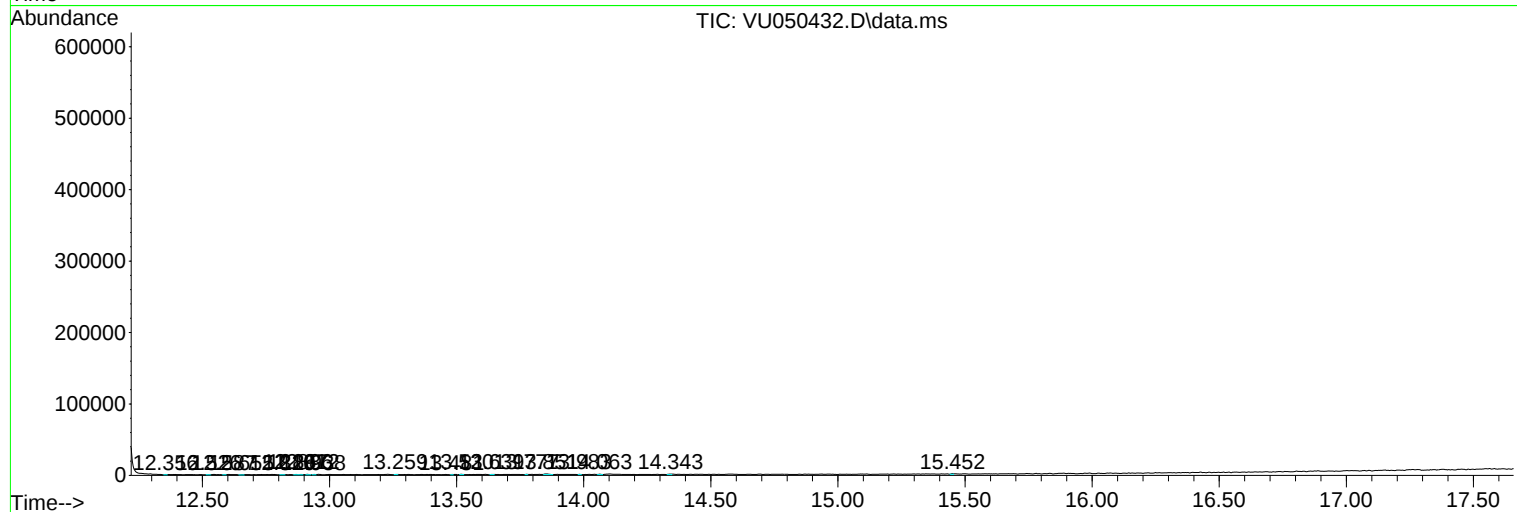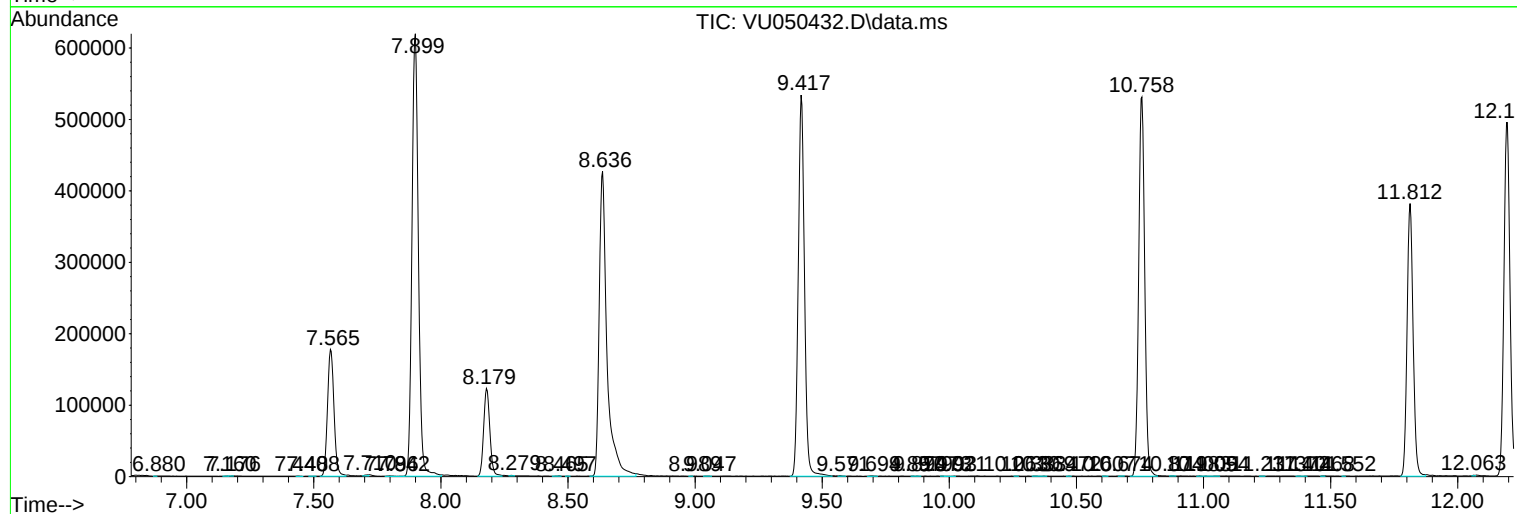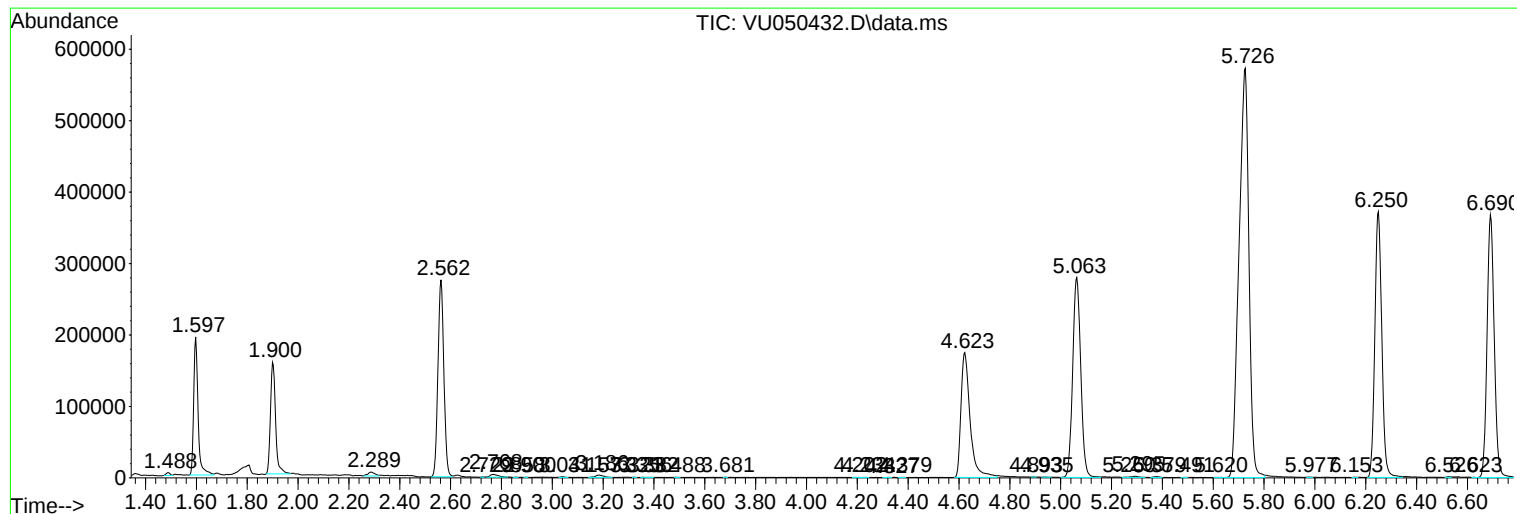

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050432.D
Acq On : 24 Aug 2022 18:00
Operator : SY/MD
Sample : N4322-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY175

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050432.D
Acq On : 24 Aug 2022 18:00
Operator : SY/MD
Sample : N4322-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY175

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------