

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050433.D
 Acq On : 24 Aug 2022 18:23
 Operator : SY/MD
 Sample : N4322-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rVB4	2292	1973	0.12%	0.018%
2	1.517	50	55	62	rBV3	2938	4056	0.25%	0.036%
3	1.594	72	79	97	rBV	214977	257087	16.06%	2.290%
4	1.900	165	174	202	rVB	172750	236999	14.81%	2.111%
5	2.562	367	380	393	rBV	320301	515477	32.21%	4.592%
6	2.630	394	401	416	rVB	13821	23012	1.44%	0.205%
7	2.774	432	446	463	rBV2	4768	11337	0.71%	0.101%
8	2.839	463	466	468	rVB2	477	281	0.02%	0.003%
9	2.864	470	474	476	rBV3	395	376	0.02%	0.003%
10	2.887	478	481	482	rVV2	493	294	0.02%	0.003%
11	2.900	482	485	495	rVV3	870	822	0.05%	0.007%
12	3.044	527	530	536	rVB3	1274	1216	0.08%	0.011%
13	3.076	536	540	543	rVB2	286	196	0.01%	0.002%
14	3.105	543	549	556	rBV2	165	255	0.02%	0.002%
15	3.183	563	573	587	rBV2	2822	5621	0.35%	0.050%
16	3.401	635	641	647	rVB2	416	414	0.03%	0.004%
17	3.639	711	715	721	rVB2	235	272	0.02%	0.002%
18	4.244	900	903	908	rVB2	245	188	0.01%	0.002%
19	4.305	917	922	928	rBV	153	214	0.01%	0.002%
20	4.372	936	943	945	rBV2	223	238	0.01%	0.002%
21	4.437	957	963	967	rBV2	184	188	0.01%	0.002%
22	4.491	976	980	985	rVV2	241	260	0.02%	0.002%
23	4.552	994	999	1001	rBV	352	278	0.02%	0.002%
24	4.623	1008	1021	1067	rBV	171372	438349	27.39%	3.905%
25	4.858	1092	1094	1096	rBV	471	273	0.02%	0.002%
26	5.064	1141	1158	1186	rBV	290472	634623	39.65%	5.654%
27	5.276	1220	1224	1225	rBV2	789	498	0.03%	0.004%
28	5.353	1245	1248	1250	rBV2	401	277	0.02%	0.002%
29	5.369	1250	1253	1261	rVV2	619	954	0.06%	0.008%
30	5.401	1261	1263	1266	rVB2	388	201	0.01%	0.002%
31	5.504	1284	1295	1297	rBV2	278	445	0.03%	0.004%
32	5.543	1304	1307	1310	rBV2	204	179	0.01%	0.002%
33	5.723	1341	1363	1397	rBV2	601312	1600410	100.00%	14.257%
34	5.951	1432	1434	1437	rVV	330	228	0.01%	0.002%
35	5.977	1437	1442	1453	rVB4	658	1001	0.06%	0.009%
36	6.092	1475	1478	1481	rBV2	321	263	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050433.D
 Acq On : 24 Aug 2022 18:23
 Operator : SY/MD
 Sample : N4322-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.157	1492	1498	1499	rBV2	568	490	0.03%	0.004%
38	6.247	1512	1526	1551	rBV	398648	761006	47.55%	6.779%
39	6.527	1608	1613	1614	rBV	1095	811	0.05%	0.007%
40	6.690	1648	1664	1686	rBV	376459	731509	45.71%	6.517%
41	6.800	1692	1698	1708	rVB4	1129	1945	0.12%	0.017%
42	7.250	1832	1838	1843	rVB	167	193	0.01%	0.002%
43	7.404	1884	1886	1893	rVB2	211	189	0.01%	0.002%
44	7.436	1893	1896	1901	rBV2	272	307	0.02%	0.003%
45	7.565	1923	1936	1961	rBV	179164	315223	19.70%	2.808%
46	7.713	1980	1982	1984	rVB2	588	273	0.02%	0.002%
47	7.800	2005	2009	2012	rBV3	471	314	0.02%	0.003%
48	7.899	2025	2040	2069	rBV	658942	1144587	71.52%	10.197%
49	8.099	2099	2102	2107	rVB3	571	418	0.03%	0.004%
50	8.179	2116	2127	2146	rBV	124628	209144	13.07%	1.863%
51	8.298	2161	2164	2165	rBV	296	182	0.01%	0.002%
52	8.456	2210	2213	2215	rVV	411	200	0.01%	0.002%
53	8.475	2215	2219	2222	rVV2	390	328	0.02%	0.003%
54	8.494	2223	2225	2231	rVB4	471	338	0.02%	0.003%
55	8.539	2235	2239	2242	rBV2	365	295	0.02%	0.003%
56	8.636	2256	2269	2314	rBV3	435952	921819	57.60%	8.212%
57	8.970	2369	2373	2379	rVB2	427	336	0.02%	0.003%
58	8.999	2379	2382	2386	rVB2	453	239	0.01%	0.002%
59	9.051	2394	2398	2401	rBV2	372	325	0.02%	0.003%
60	9.083	2405	2408	2411	rVB	331	208	0.01%	0.002%
61	9.115	2411	2418	2422	rBV2	309	331	0.02%	0.003%
62	9.243	2454	2458	2460	rBV	310	225	0.01%	0.002%
63	9.276	2464	2468	2471	rBV	267	221	0.01%	0.002%
64	9.417	2499	2512	2546	rVV	557021	936795	58.53%	8.345%
65	9.552	2552	2554	2557	rVB2	443	228	0.01%	0.002%
66	9.578	2560	2562	2568	rVB4	565	378	0.02%	0.003%
67	9.687	2591	2596	2599	rBV2	368	378	0.02%	0.003%
68	9.822	2635	2638	2644	rVB	446	351	0.02%	0.003%
69	9.912	2662	2666	2669	rBV	245	263	0.02%	0.002%
70	9.980	2681	2687	2689	rBV2	273	246	0.02%	0.002%
71	10.192	2748	2753	2754	rBV	203	193	0.01%	0.002%
72	10.214	2757	2760	2765	rVB2	192	204	0.01%	0.002%
73	10.288	2778	2783	2787	rBV2	274	353	0.02%	0.003%
74	10.578	2871	2873	2881	rVB2	271	274	0.02%	0.002%
75	10.677	2902	2904	2907	rBV2	314	230	0.01%	0.002%
76	10.758	2915	2929	2956	rBV	532349	874247	54.63%	7.788%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050433.D
 Acq On : 24 Aug 2022 18:23
 Operator : SY/MD
 Sample : N4322-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.893	2965	2971	2972	rBV2	264	262	0.02%	0.002%
78	10.993	2998	3002	3003	rBV	315	180	0.01%	0.002%
79	11.189	3057	3063	3072	rVB2	377	685	0.04%	0.006%
80	11.237	3072	3078	3080	rBV2	202	210	0.01%	0.002%
81	11.378	3119	3122	3127	rVB	312	226	0.01%	0.002%
82	11.597	3185	3190	3192	rBV2	236	231	0.01%	0.002%
83	11.610	3192	3194	3197	rVV	397	229	0.01%	0.002%
84	11.629	3197	3200	3205	rVV	204	187	0.01%	0.002%
85	11.671	3210	3213	3216	rVV2	284	185	0.01%	0.002%
86	11.690	3216	3219	3224	rVV	404	403	0.03%	0.004%
87	11.812	3242	3257	3278	rBV	425270	684250	42.75%	6.096%
88	11.964	3301	3304	3308	rVB2	390	234	0.01%	0.002%
89	12.066	3332	3336	3339	rBV2	969	949	0.06%	0.008%
90	12.111	3348	3350	3353	rBV	301	182	0.01%	0.002%
91	12.195	3362	3376	3407	rBV	541103	888354	55.51%	7.914%
92	12.343	3419	3422	3425	rBV2	627	545	0.03%	0.005%
93	12.494	3465	3469	3471	rBV2	356	301	0.02%	0.003%
94	12.681	3524	3527	3530	rBV2	294	222	0.01%	0.002%
95	12.732	3540	3543	3545	rBV	289	200	0.01%	0.002%
96	13.063	3643	3646	3648	rBV2	564	377	0.02%	0.003%
97	13.407	3750	3753	3757	rVB2	433	295	0.02%	0.003%
98	13.848	3886	3890	3896	rBV5	752	1112	0.07%	0.010%
99	14.414	4064	4066	4068	rBV2	375	224	0.01%	0.002%
100	14.648	4133	4139	4146	rBV2	508	841	0.05%	0.007%




Sum of corrected areas: 11225235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050433.D
Acq On : 24 Aug 2022 18:23
Operator : SY/MD
Sample : N4322-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

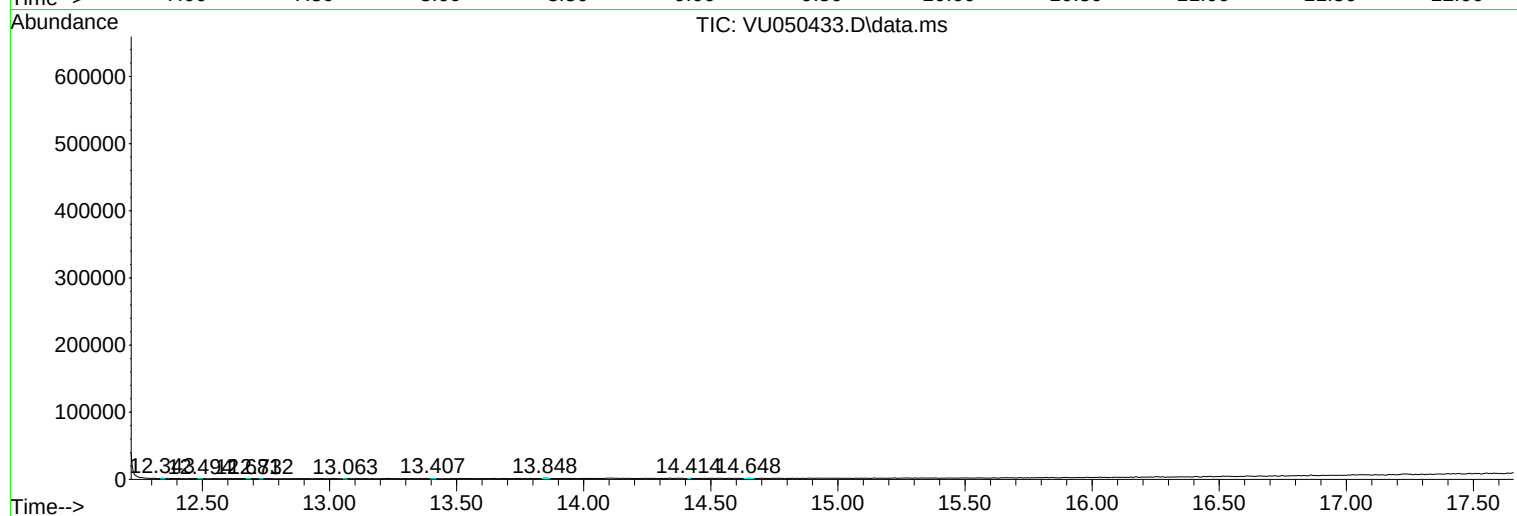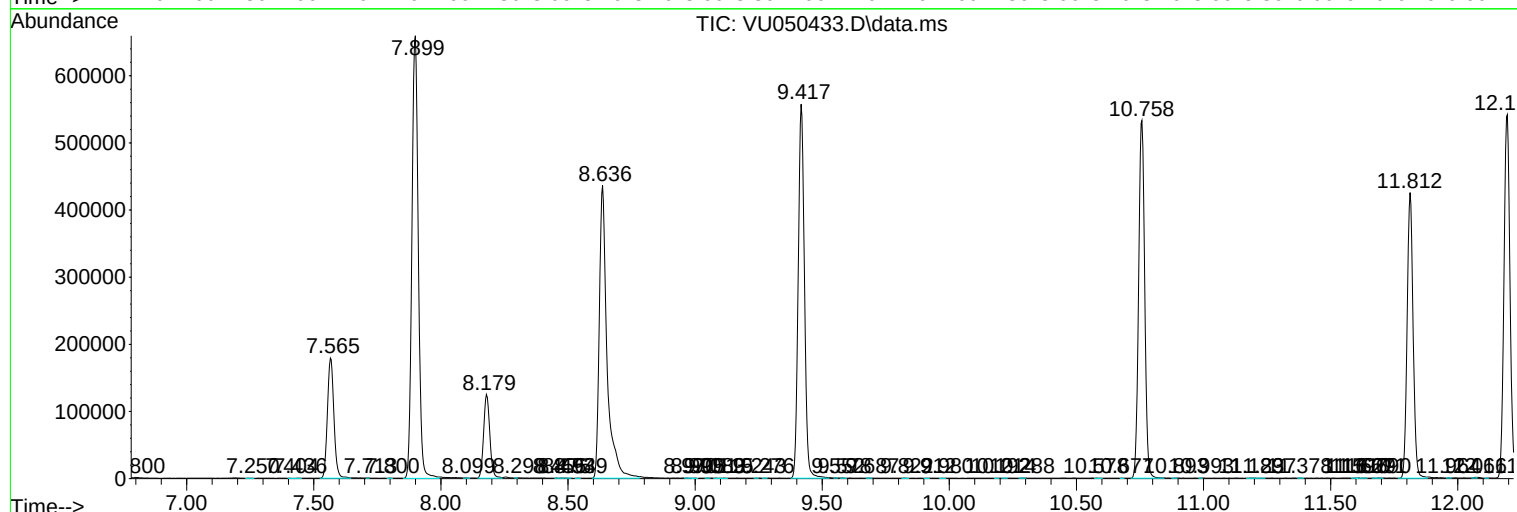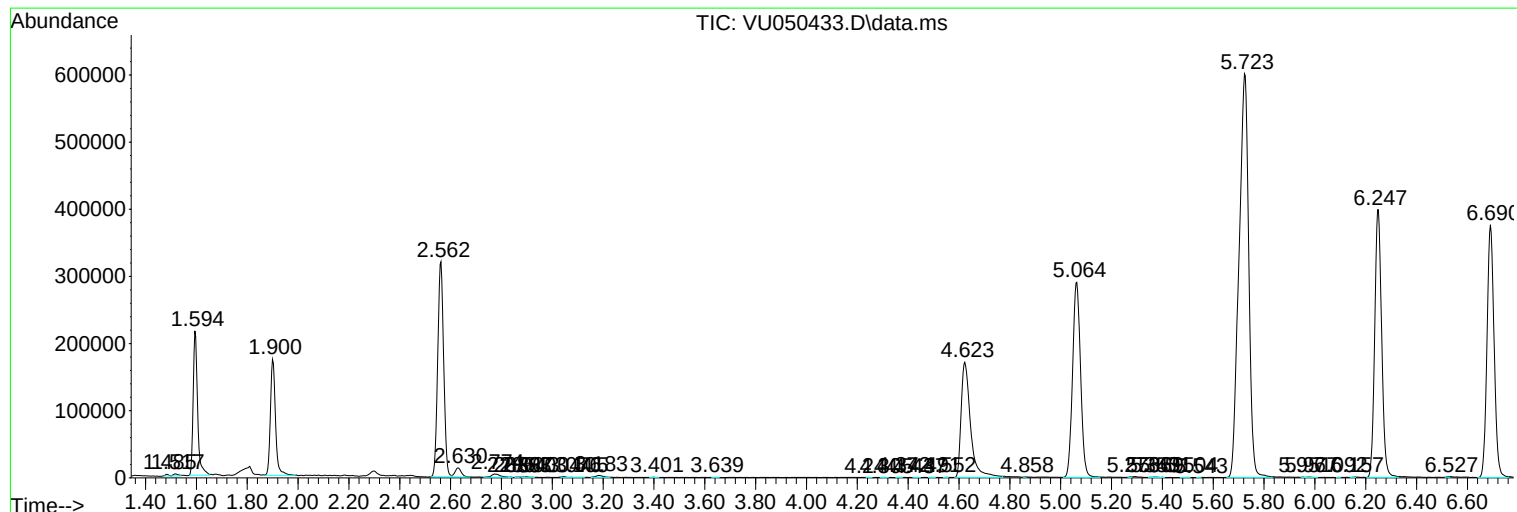

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050433.D
Acq On : 24 Aug 2022 18:23
Operator : SY/MD
Sample : N4322-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
Data File : VU050433.D
Acq On : 24 Aug 2022 18:23
Operator : SY/MD
Sample : N4322-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------