


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082422\
 Data File : VU050418.D
 Acq On : 24 Aug 2022 09:45
 Operator : SY/MD
 Sample : BFB112
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB112

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 25 05:03:52 2022

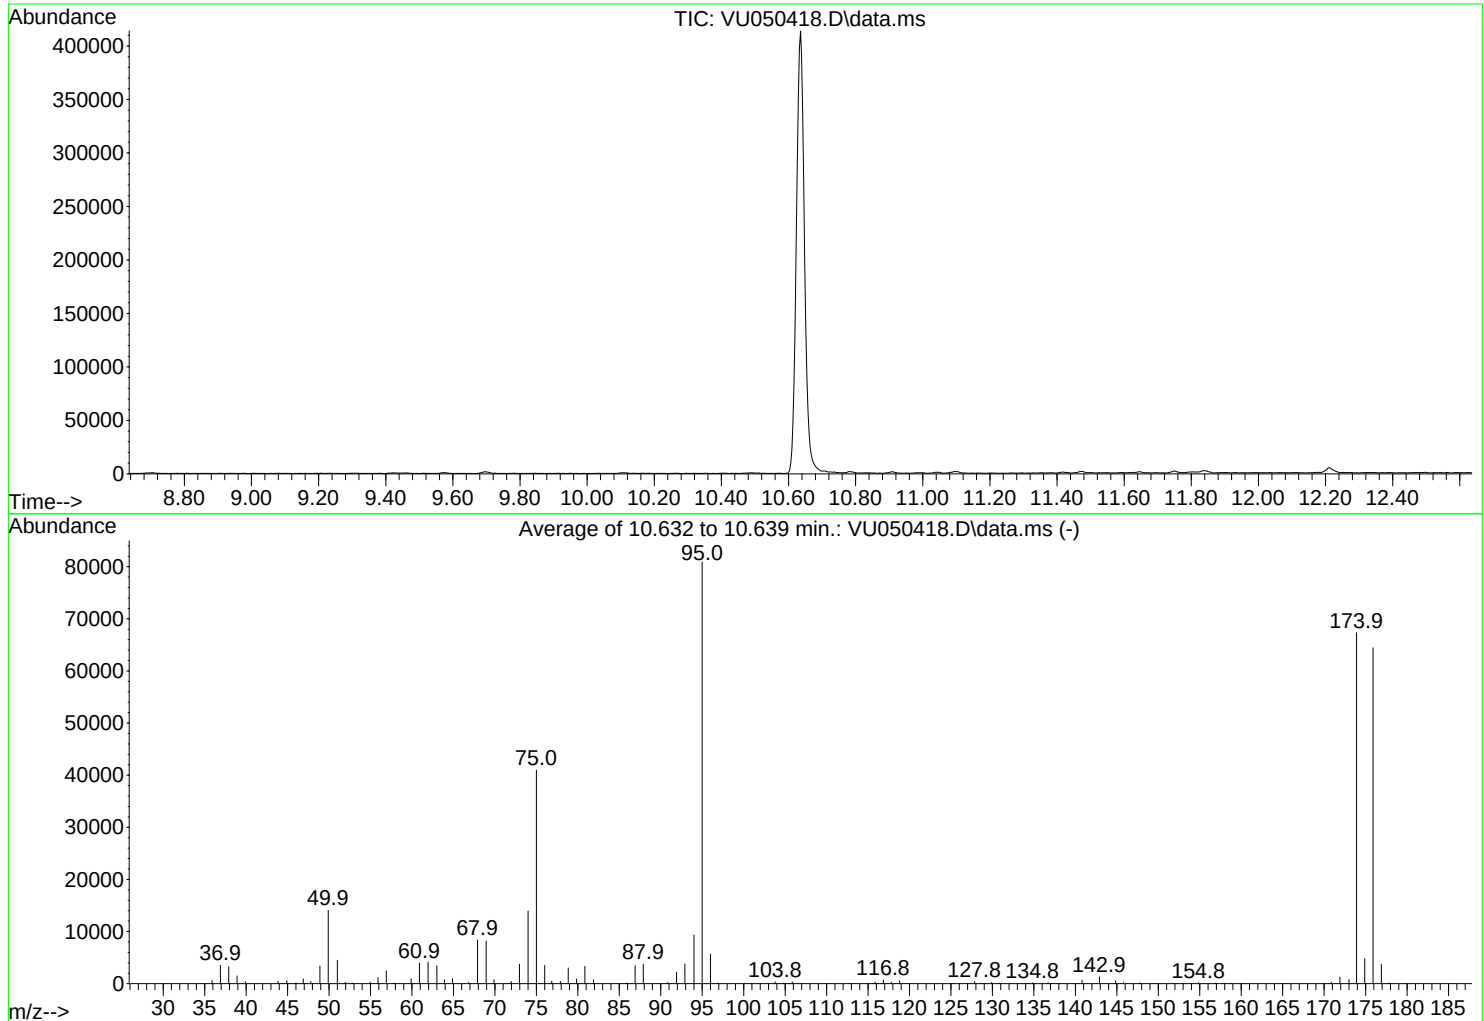

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	14065	PASS
75	95	30	80	50.6	40981	PASS
95	95	100	100	100.0	80931	PASS
96	95	5	9	7.0	5659	PASS
173	174	0.00	2	1.2	813	PASS
174	95	50	120	83.2	67349	PASS
175	174	5	9	7.1	4807	PASS
176	174	95	101	95.7	64429	PASS
177	176	5	9	5.8	3758	PASS

m/z	Abundance
39.90	134.0
43.80	409.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112

m/z	Abundance
35.90	656.0
36.90	3580.0
37.90	3233.0
38.90	1438.0
39.90	532.0
43.90	812.0
44.90	667.0
46.00	118.0
46.90	939.0
47.80	385.0
48.90	3341.0
49.90	14181.0
51.00	4614.0
52.00	192.0
52.80	118.0
54.90	283.0
55.90	1213.0
56.90	2536.0
59.90	1001.0
60.90	4033.0
62.00	4102.0
63.00	3351.0
63.90	769.0
64.90	931.0
66.80	223.0
67.90	8451.0
69.00	8306.0
69.90	753.0
71.90	418.0
72.90	3752.0
74.00	13930.0
75.00	40800.0
76.00	3606.0
76.80	446.0
77.90	421.0
78.90	2961.0
79.90	932.0
80.80	3298.0
81.90	666.0
85.90	136.0
86.90	3568.0
87.90	3613.0
90.80	213.0
91.90	2045.0
92.90	3671.0
94.00	9102.0
95.00	81336.0
96.00	5948.0
96.90	113.0
103.90	384.0
105.80	334.0
115.80	276.0
116.90	686.0
117.80	314.0
118.80	501.0
127.80	366.0
128.70	169.0
129.90	194.0
134.80	159.0
136.70	225.0
140.80	689.0
142.90	1280.0
144.80	566.0
145.80	245.0
147.80	182.0
154.90	233.0
170.90	307.0
171.90	1207.0
173.00	775.0
173.90	65688.0
174.90	4838.0
175.90	62784.0
176.90	3836.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112

m/z	Abundance
35.90	634.0
36.90	3633.0
37.90	3338.0
38.90	1514.0
39.90	537.0
43.90	947.0
44.90	596.0
46.00	158.0
46.90	930.0
47.80	400.0
48.90	3534.0
49.90	14477.0
51.00	4616.0
51.90	243.0
52.80	128.0
55.00	336.0
55.90	1172.0
56.90	2576.0
57.80	139.0
59.90	991.0
60.90	4074.0
61.90	4279.0
63.00	3562.0
63.90	824.0
64.90	958.0
66.80	202.0
67.90	8701.0
68.90	8478.0
69.90	796.0
71.90	421.0
73.00	3891.0
74.00	14399.0
75.00	42264.0
76.00	3637.0
76.80	532.0
77.90	409.0
78.80	3057.0
79.90	926.0
80.90	3413.0
81.90	784.0
85.80	147.0
86.90	3546.0
87.90	3957.0
90.90	210.0
91.90	2283.0
92.90	3934.0
94.00	9602.0
95.00	83288.0
96.00	5853.0
96.90	126.0
103.80	340.0
104.80	123.0
105.90	373.0
112.70	106.0
115.90	263.0
116.90	674.0
117.80	263.0
118.80	597.0
127.90	412.0
128.70	132.0
129.90	207.0
130.80	104.0
134.90	169.0
136.70	201.0
140.80	738.0
142.90	1366.0
144.80	563.0
145.80	202.0
147.80	214.0
154.80	233.0
156.90	116.0
158.80	100.0
170.90	299.0
171.90	1314.0
173.00	833.0
173.90	69328.0
174.90	5003.0
175.90	66288.0
176.90	3841.0
177.80	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112

m/z	Abundance
35.90	561.0
36.90	3425.0
37.90	3097.0
38.90	1457.0
39.90	512.0
43.90	982.0
44.90	478.0
46.00	174.0
46.90	836.0
47.80	416.0
48.90	3223.0
49.90	13538.0
51.00	4246.0
51.90	273.0
52.80	121.0
55.00	305.0
55.90	1106.0
56.90	2270.0
57.90	135.0
59.90	891.0
60.90	3807.0
61.90	3953.0
63.00	3401.0
63.90	716.0
64.90	942.0
66.90	203.0
67.90	8015.0
68.90	7733.0
69.90	736.0
72.00	408.0
73.00	3589.0
74.00	13481.0
75.00	39880.0
76.00	3264.0
76.90	510.0
77.90	415.0
78.80	2998.0
79.80	835.0
80.90	3227.0
81.90	784.0
85.80	131.0
86.90	3320.0
87.90	3686.0
90.90	226.0
91.90	2307.0
92.90	3717.0
94.00	9341.0
95.00	78168.0
96.00	5175.0
96.90	133.0
103.70	347.0
104.80	152.0
105.90	355.0
106.80	125.0
115.90	260.0
116.80	635.0
117.80	236.0
118.80	598.0
127.90	420.0
129.90	216.0
130.80	145.0
134.90	168.0
136.70	126.0
140.80	742.0
142.90	1370.0
144.90	512.0
145.80	177.0
147.80	189.0
154.80	218.0
156.90	154.0
170.80	229.0
171.90	1271.0
173.00	830.0
173.90	67032.0
174.90	4581.0
175.90	64216.0
176.90	3598.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112