

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082518\
 Data File : VU026361.D
 Acq On : 25 Aug 2018 11:24
 Operator : MD/SY
 Sample : J4622-08DL2 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBK0DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.706	30	36	37	rBV	338	284	0.02%	0.003%
2	0.841	75	78	80	rBV2	244	165	0.01%	0.001%
3	0.956	112	114	117	rBV2	173	55	0.00%	0.000%
4	1.024	130	135	136	rBV	369	277	0.02%	0.002%
5	1.088	147	155	175	rBV	1157017	1266720	100.00%	11.196%
6	1.397	244	251	265	rBV	169572	176365	13.92%	1.559%
7	1.680	332	339	354	rVB	127034	163190	12.88%	1.442%
8	2.272	514	523	536	rVB	280892	426572	33.68%	3.770%
9	2.391	556	560	563	rBV2	712	664	0.05%	0.006%
10	2.699	650	656	657	rBV3	1318	1032	0.08%	0.009%
11	2.837	692	699	712	rVB4	1479	2965	0.23%	0.026%
12	3.181	803	806	811	rVB2	466	485	0.04%	0.004%
13	3.210	811	815	819	rBV2	384	363	0.03%	0.003%
14	3.506	904	907	910	rBV2	342	201	0.02%	0.002%
15	3.590	928	933	934	rBV	307	205	0.02%	0.002%
16	3.638	946	948	950	rBV	195	112	0.01%	0.001%
17	3.853	1010	1015	1020	rBV2	305	387	0.03%	0.003%
18	3.956	1045	1047	1048	rBV	132	57	0.00%	0.001%
19	4.037	1070	1072	1074	rBV	341	172	0.01%	0.002%
20	4.075	1082	1084	1086	rVB	360	130	0.01%	0.001%
21	4.178	1101	1116	1149	rBV	102599	294616	23.26%	2.604%
22	4.525	1217	1224	1230	rVB2	462	570	0.04%	0.005%
23	4.590	1238	1244	1245	rBV2	389	256	0.02%	0.002%
24	4.651	1246	1263	1287	rVV	212054	511027	40.34%	4.517%
25	4.828	1315	1318	1319	rBV	307	206	0.02%	0.002%
26	4.953	1355	1357	1361	rVB3	575	307	0.02%	0.003%
27	4.995	1361	1370	1374	rBV2	642	931	0.07%	0.008%
28	5.101	1400	1403	1405	rBV2	373	216	0.02%	0.002%
29	5.124	1405	1410	1413	rBV3	340	300	0.02%	0.003%
30	5.156	1418	1420	1422	rBV	192	111	0.01%	0.001%
31	5.191	1429	1431	1433	rBV2	184	111	0.01%	0.001%
32	5.226	1440	1442	1445	rBV2	232	93	0.01%	0.001%
33	5.246	1445	1448	1450	rBV	399	195	0.02%	0.002%
34	5.342	1453	1478	1500	rBV2	431732	1265132	99.87%	11.182%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082518\
 Data File : VU026361.D
 Acq On : 25 Aug 2018 11:24
 Operator : MD/SY
 Sample : J4622-08DL2 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBK0DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

35	5.554	1540	1544	1546	rBV2	528	363	0.03%	0.003%
36	5.625	1563	1566	1567	rBV	166	82	0.01%	0.001%
37	5.712	1590	1593	1595	rBV2	192	139	0.01%	0.001%
38	5.821	1624	1627	1630	rBV2	286	207	0.02%	0.002%
39	5.889	1633	1648	1675	rBV	395016	776379	61.29%	6.862%
40	6.146	1725	1728	1729	rBV2	393	223	0.02%	0.002%
41	6.188	1729	1741	1757	rVV2	85617	163033	12.87%	1.441%
42	6.332	1772	1786	1808	rBV	287517	568589	44.89%	5.025%
43	6.455	1821	1824	1829	rBV3	653	531	0.04%	0.005%
44	6.529	1845	1847	1852	rVB	493	277	0.02%	0.002%
45	6.551	1852	1854	1855	rBV	107	33	0.00%	0.000%
46	6.564	1855	1858	1861	rBV3	321	209	0.02%	0.002%
47	6.609	1866	1872	1874	rBV2	510	485	0.04%	0.004%
48	6.744	1910	1914	1915	rBV	257	154	0.01%	0.001%
49	6.818	1935	1937	1938	rBV	175	52	0.00%	0.000%
50	6.828	1938	1940	1944	rBV2	336	163	0.01%	0.001%
51	6.853	1944	1948	1951	rBV2	570	641	0.05%	0.006%
52	6.953	1975	1979	1982	rBV3	318	231	0.02%	0.002%
53	7.075	2015	2017	2024	rVB2	469	317	0.03%	0.003%
54	7.104	2024	2026	2030	rBV2	347	259	0.02%	0.002%
55	7.230	2053	2065	2083	rBV	159590	279831	22.09%	2.473%
56	7.371	2107	2109	2111	rBV3	374	229	0.02%	0.002%
57	7.493	2145	2147	2151	rBV2	179	137	0.01%	0.001%
58	7.512	2151	2153	2155	rVB	351	173	0.01%	0.002%
59	7.567	2156	2170	2192	rBV	593391	1012892	79.96%	8.952%
60	7.850	2247	2258	2277	rBV	117440	199991	15.79%	1.768%
61	8.184	2350	2362	2372	rBV	47704	108010	8.53%	0.955%
62	8.313	2393	2402	2426	rVB	344044	577751	45.61%	5.106%
63	8.474	2448	2452	2454	rBV2	602	458	0.04%	0.004%
64	8.622	2491	2498	2510	rVB4	4907	7951	0.63%	0.070%
65	8.760	2538	2541	2542	rBV2	322	197	0.02%	0.002%
66	8.873	2573	2576	2578	rBV	319	189	0.01%	0.002%
67	9.091	2631	2644	2666	rBV	591685	964182	76.12%	8.522%
68	9.249	2690	2693	2694	rBV	393	232	0.02%	0.002%
69	9.474	2760	2763	2765	rBV	419	301	0.02%	0.003%
70	9.680	2822	2827	2830	rBV3	410	452	0.04%	0.004%
71	9.953	2908	2912	2915	rBV3	813	690	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082518\
Data File : VU026361.D
Acq On : 25 Aug 2018 11:24
Operator : MD/SY
Sample : J4622-08DL2 5000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBK0DL2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Title : VOC Analysis

72	10.432	3050	3061	3077	rBV	396854	621156	49.04%	5.490%
73	10.522	3086	3089	3091	rBV2	417	280	0.02%	0.002%
74	10.551	3095	3098	3103	rBV2	400	419	0.03%	0.004%
75	10.618	3109	3119	3131	rVB5	11074	20809	1.64%	0.184%
76	10.876	3195	3199	3207	rVB2	786	961	0.08%	0.008%
77	11.483	3376	3388	3404	rBV	585224	913719	72.13%	8.076%
78	11.863	3493	3506	3521	rBV	620247	976483	77.09%	8.630%


Sum of corrected areas: 11314332

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082518\
Data File : VU026361.D
Acq On : 25 Aug 2018 11:24
Operator : MD/SY
Sample : J4622-08DL2 5000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
ETBK0DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

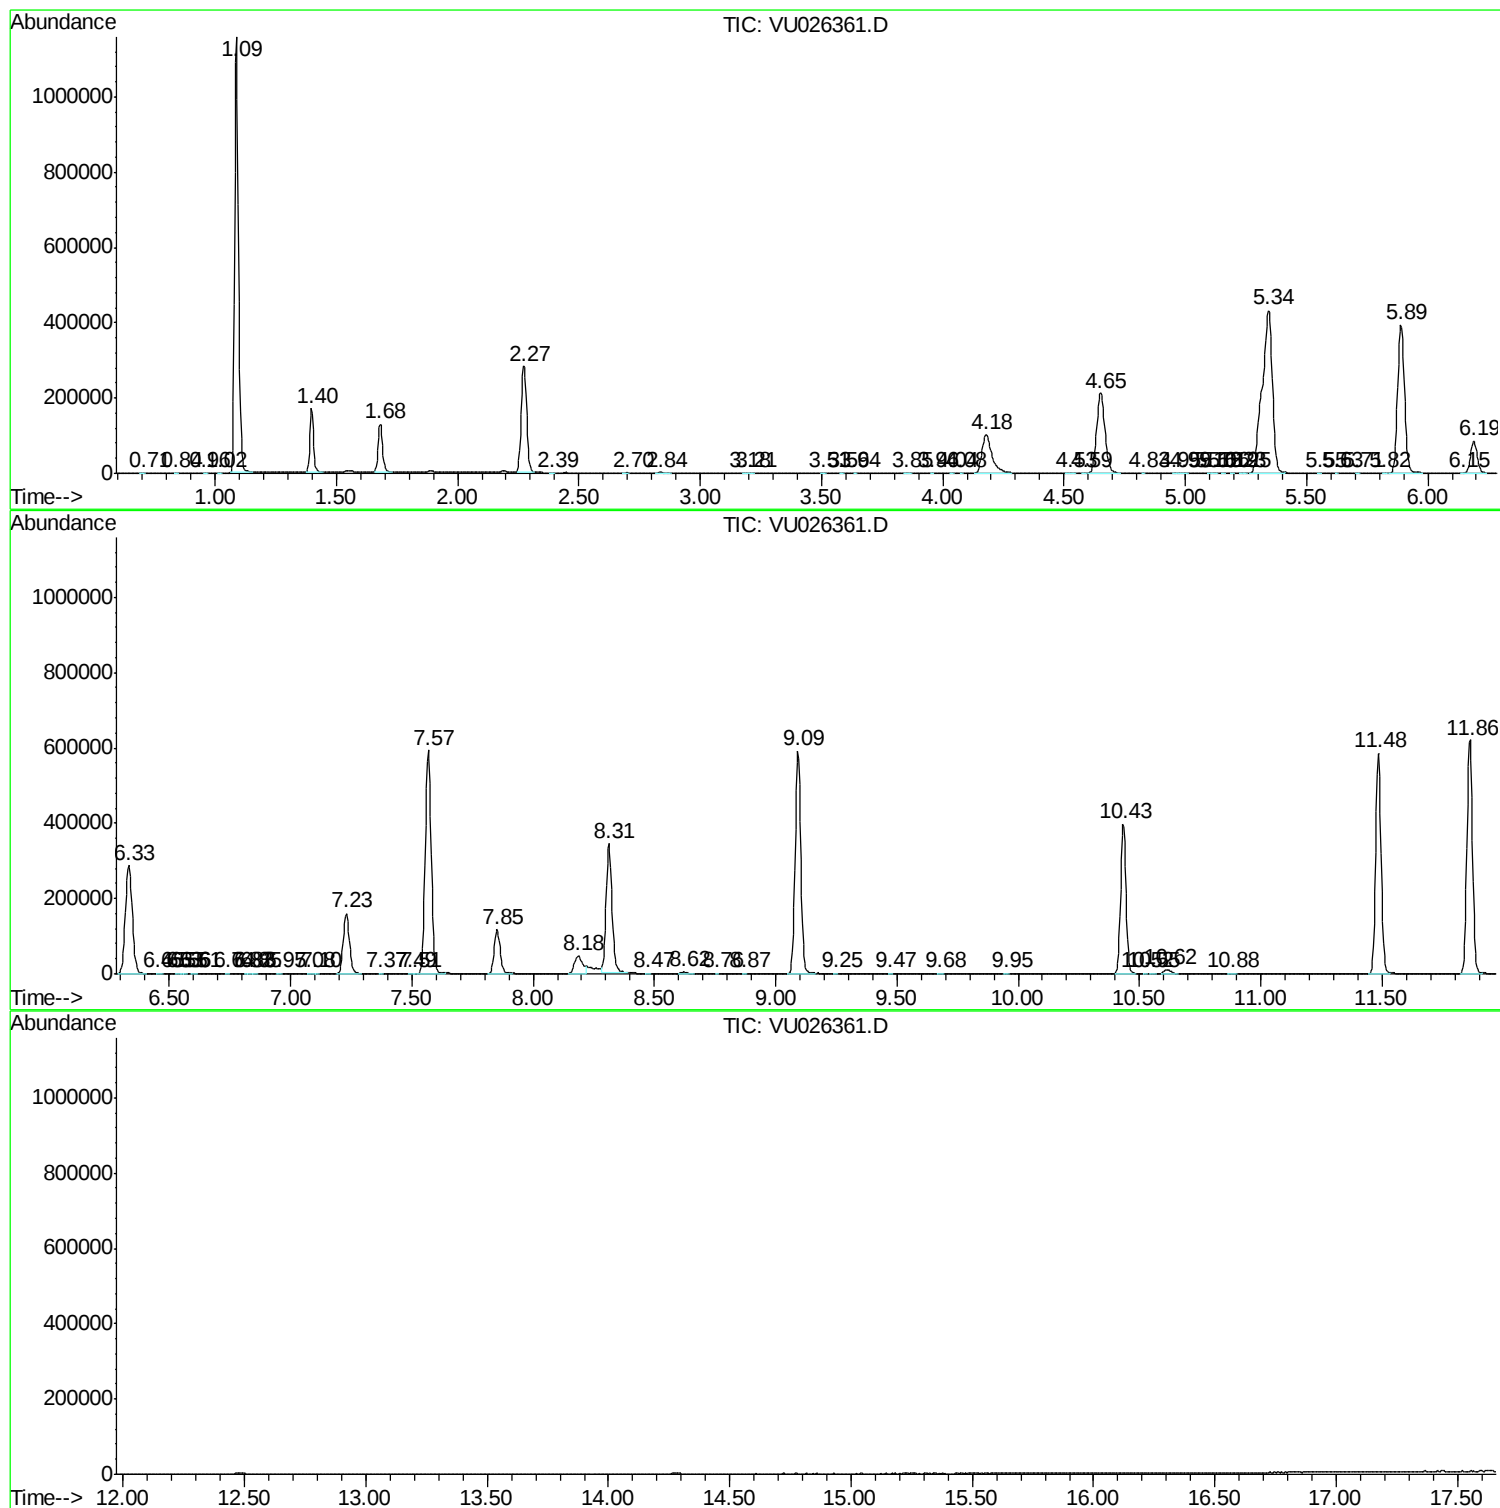

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082518\
Data File : VU026361.D
Acq On : 25 Aug 2018 11:24
Operator : MD/SY
Sample : J4622-08DL2 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBK0DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082518\
Data File : VU026361.D
Acq On : 25 Aug 2018 11:24
Operator : MD/SY
Sample : J4622-08DL2 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBK0DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc