

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082518\
 Data File : VU026377.D
 Acq On : 25 Aug 2018 17:35
 Operator : MD/SY
 Sample : J4644-14DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOM4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.641	11	16	18	rBV	235	213	0.002%	0.0002%
2	0.683	24	29	30	rBV2	291	258	0.002%	0.0002%
3	0.732	42	44	49	rBV2	259	206	0.002%	0.0002%
4	0.757	49	52	54	rBV2	326	257	0.002%	0.0002%
5	0.831	66	75	78	rBV2	369	532	0.005%	0.0005%
6	0.873	86	88	92	rVB	150	54	0.000%	0.0001%
7	0.892	92	94	97	rBV	230	127	0.001%	0.0001%
8	0.934	104	107	111	rBV2	396	284	0.002%	0.0003%
9	0.986	121	123	126	rBV2	299	197	0.002%	0.0002%
10	1.037	136	139	140	rBV	213	103	0.001%	0.0001%
11	1.088	140	155	173	rBV	1033394	1149009	99.66%	11.054%
12	1.400	244	252	264	rBV2	325435	349020	30.27%	3.358%
13	1.680	332	339	353	rVB	111807	140640	12.20%	1.353%
14	2.272	513	523	536	rVB	249959	376771	32.68%	3.625%
15	2.725	661	664	666	rBV	281	196	0.002%	0.0002%
16	3.362	860	862	864	rBV	576	386	0.003%	0.0004%
17	3.510	906	908	911	rBV	257	160	0.001%	0.0002%
18	3.529	911	914	918	rVV2	468	337	0.003%	0.0003%
19	3.555	918	922	928	rVV2	493	391	0.003%	0.0004%
20	3.625	942	944	946	rBV	142	63	0.001%	0.0001%
21	3.690	961	964	968	rBV	304	223	0.002%	0.0002%
22	3.741	975	980	983	rBV3	351	363	0.003%	0.0003%
23	3.799	996	998	1001	rBV	314	177	0.002%	0.0002%
24	3.950	1043	1045	1048	rBV2	227	123	0.001%	0.0001%
25	3.995	1056	1059	1062	rVB	125	89	0.001%	0.0001%
26	4.014	1062	1065	1068	rBV2	278	198	0.002%	0.0002%
27	4.178	1100	1116	1122	rBV	99063	217935	18.90%	2.097%
28	4.391	1179	1182	1185	rBV2	512	350	0.003%	0.0003%
29	4.471	1204	1207	1211	rBV2	296	220	0.002%	0.0002%
30	4.490	1211	1213	1218	rVB2	496	246	0.002%	0.0002%
31	4.516	1218	1221	1223	rBV	394	286	0.002%	0.0003%
32	4.574	1235	1239	1241	rBV2	585	355	0.003%	0.0003%
33	4.651	1246	1263	1291	rVB	190025	473198	41.04%	4.552%
34	4.747	1291	1293	1296	rBV2	440	304	0.003%	0.0003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082518\
 Data File : VU026377.D
 Acq On : 25 Aug 2018 17:35
 Operator : MD/SY
 Sample : J4644-14DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOM4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis

35	4.953	1355	1357	1358	rBV	227	77	0.01%	0.001%
36	4.992	1365	1369	1372	rVB3	625	556	0.05%	0.005%
37	5.005	1372	1373	1377	rVB2	176	104	0.01%	0.001%
38	5.027	1377	1380	1383	rBV	281	244	0.02%	0.002%
39	5.072	1392	1394	1397	rVB	271	144	0.01%	0.001%
40	5.095	1397	1401	1403	rBV2	547	420	0.04%	0.004%
41	5.111	1403	1406	1407	rBV	180	91	0.01%	0.001%
42	5.146	1414	1417	1420	rBV	77	69	0.01%	0.001%
43	5.178	1425	1427	1428	rBV	243	124	0.01%	0.001%
44	5.233	1441	1444	1448	rBV2	202	156	0.01%	0.002%
45	5.249	1448	1449	1453	rVB2	219	94	0.01%	0.001%
46	5.342	1453	1478	1498	rBV2	387993	1152972	100.00%	11.092%
47	5.545	1539	1541	1544	rBV2	207	83	0.01%	0.001%
48	5.561	1544	1546	1551	rVB2	584	315	0.03%	0.003%
49	5.590	1551	1555	1558	rBV2	279	190	0.02%	0.002%
50	5.609	1558	1561	1563	rBV2	436	243	0.02%	0.002%
51	5.683	1581	1584	1586	rBV2	328	177	0.02%	0.002%
52	5.747	1602	1604	1610	rBV3	433	387	0.03%	0.004%
53	5.805	1619	1622	1623	rBV	178	101	0.01%	0.001%
54	5.889	1633	1648	1669	rBV	377109	733111	63.58%	7.053%
55	6.107	1714	1716	1718	rBV3	351	120	0.01%	0.001%
56	6.152	1726	1730	1731	rBV3	431	267	0.02%	0.003%
57	6.194	1733	1743	1755	rVB9	4157	8462	0.73%	0.081%
58	6.333	1771	1786	1805	rBV	260669	520960	45.18%	5.012%
59	6.429	1814	1816	1819	rVB2	371	217	0.02%	0.002%
60	6.455	1819	1824	1825	rBV2	587	436	0.04%	0.004%
61	6.484	1832	1833	1838	rVB2	392	126	0.01%	0.001%
62	6.567	1856	1859	1863	rBV	501	388	0.03%	0.004%
63	6.725	1906	1908	1910	rBV	186	115	0.01%	0.001%
64	6.744	1911	1914	1917	rVV2	309	217	0.02%	0.002%
65	6.767	1917	1921	1924	rVB2	247	227	0.02%	0.002%
66	6.789	1924	1928	1931	rVB2	358	280	0.02%	0.003%
67	6.812	1931	1935	1939	rBV2	433	350	0.03%	0.003%
68	6.863	1944	1951	1956	rBV4	994	1202	0.10%	0.012%
69	6.911	1964	1966	1968	rBV	238	123	0.01%	0.001%
70	6.982	1985	1988	1991	rVB2	411	239	0.02%	0.002%
71	7.001	1991	1994	1995	rBV	246	152	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082518\
Data File : VU026377.D
Acq On : 25 Aug 2018 17:35
Operator : MD/SY
Sample : J4644-14DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOM4DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Title : VOC Analysis

72	7.104	2022	2026	2027	rBV	227	150	0.01%	0.001%
73	7.162	2039	2044	2048	rBV2	250	290	0.03%	0.003%
74	7.185	2048	2051	2053	rBV2	406	281	0.02%	0.003%
75	7.230	2053	2065	2084	rVV	144556	252708	21.92%	2.431%
76	7.455	2130	2135	2138	rBV4	457	437	0.04%	0.004%
77	7.477	2138	2142	2144	rVB	317	225	0.02%	0.002%
78	7.493	2145	2147	2152	rVB	360	248	0.02%	0.002%
79	7.567	2156	2170	2189	rBV	529894	907749	78.73%	8.733%
80	7.850	2247	2258	2273	rBV	106962	179547	15.57%	1.727%
81	8.185	2349	2362	2374	rBV2	41536	101853	8.83%	0.980%
82	8.313	2393	2402	2430	rVB	319408	548341	47.56%	5.275%
83	8.619	2490	2497	2503	rBV4	1434	2210	0.19%	0.021%
84	8.728	2529	2531	2532	rBV	288	97	0.01%	0.001%
85	8.882	2575	2579	2583	rVB3	329	253	0.02%	0.002%
86	9.091	2631	2644	2662	rBV	558563	908975	78.84%	8.744%
87	9.631	2809	2812	2819	rBV3	443	384	0.03%	0.004%
88	10.258	3004	3007	3012	rVB2	532	399	0.03%	0.004%
89	10.291	3012	3017	3019	rBV3	421	357	0.03%	0.003%
90	10.432	3050	3061	3086	rVB	366385	591485	51.30%	5.690%
91	10.612	3108	3117	3131	rVB4	9405	16986	1.47%	0.163%
92	11.239	3309	3312	3314	rBV2	337	221	0.02%	0.002%
93	11.426	3368	3370	3374	rBV	438	293	0.03%	0.003%
94	11.487	3376	3389	3413	rVV	548573	855685	74.22%	8.232%
95	11.860	3493	3505	3527	rBV	544183	888975	77.10%	8.552%


Sum of corrected areas: 10394959

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082518\
Data File : VU026377.D
Acq On : 25 Aug 2018 17:35
Operator : MD/SY
Sample : J4644-14DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOM4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

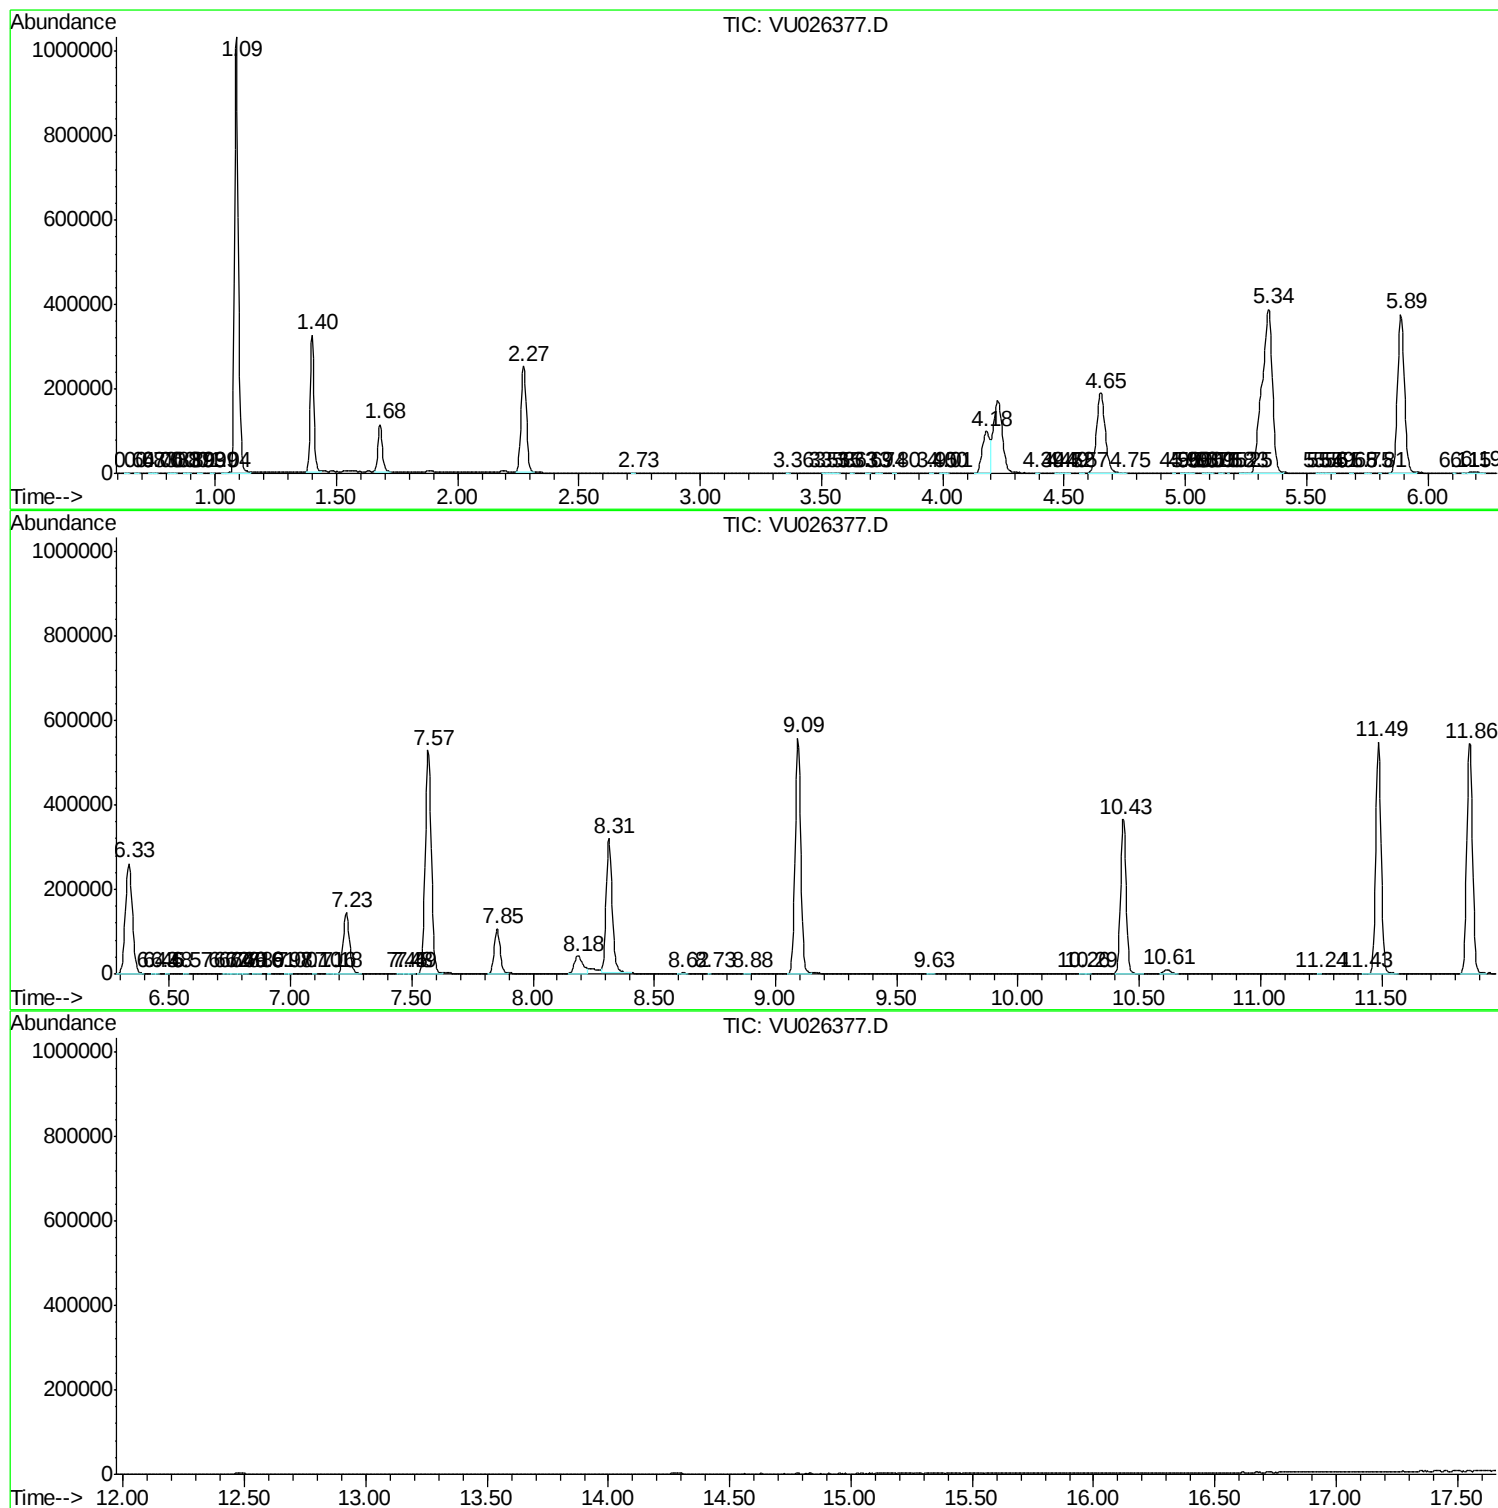

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082518\
Data File : VU026377.D
Acq On : 25 Aug 2018 17:35
Operator : MD/SY
Sample : J4644-14DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOM4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU082518\
Data File : VU026377.D
Acq On : 25 Aug 2018 17:35
Operator : MD/SY
Sample : J4644-14DL 200X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
ETOM4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc