


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082518\
 Data File : VU026357.D
 Acq On : 25 Aug 2018 09:39
 Operator : MD/SY
 Sample : BFB43
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB43

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 27 02:33:35 2018

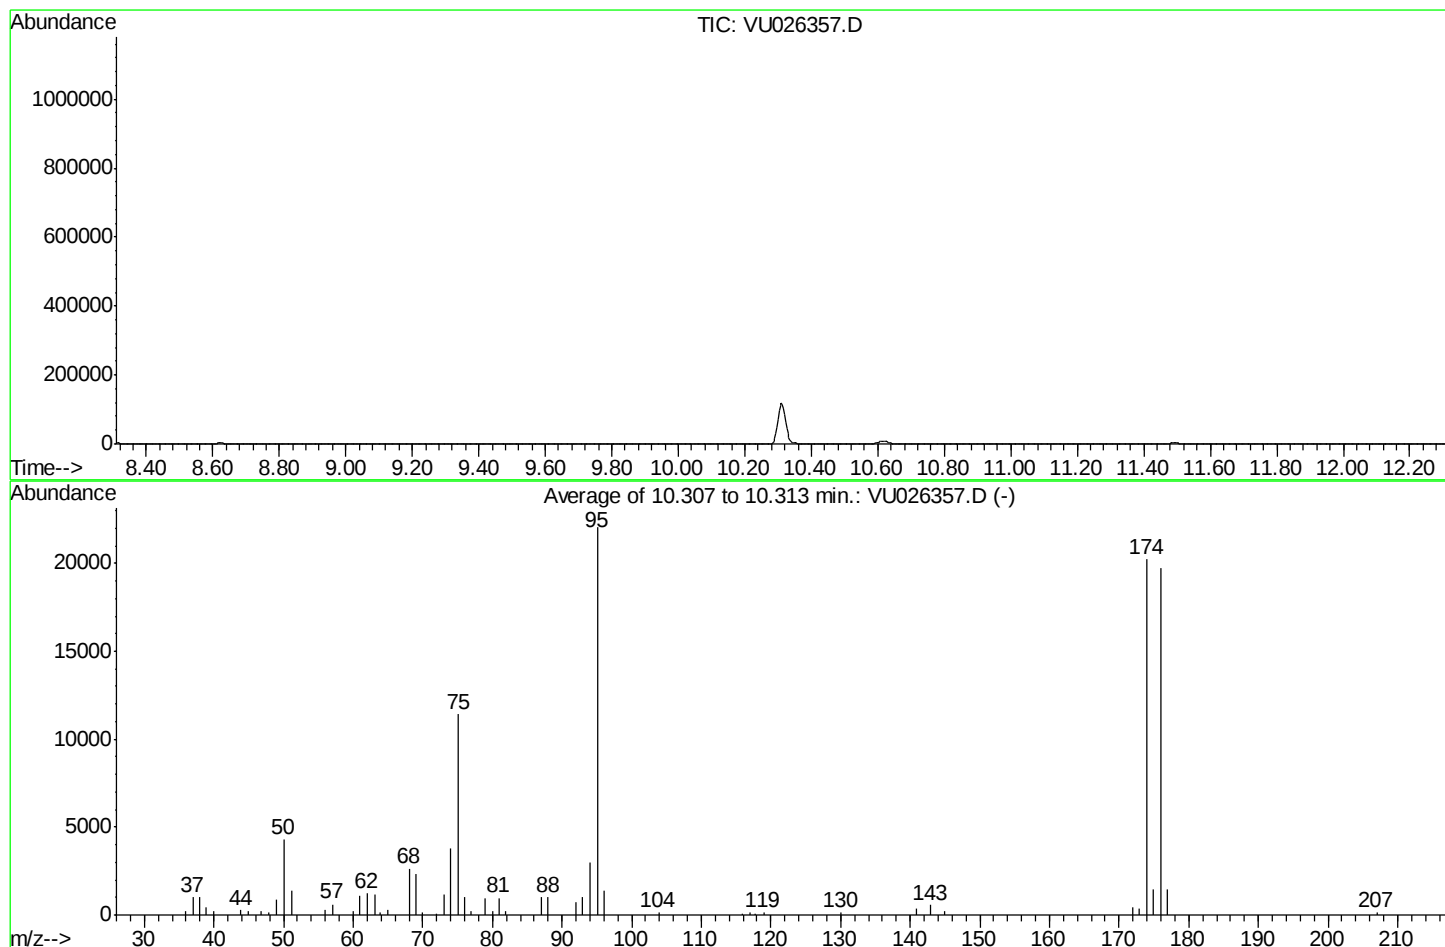

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	4262	PASS
75	95	30	80	51.7	11397	PASS
95	95	100	100	100.0	22048	PASS
96	95	5	9	6.4	1414	PASS
173	174	0.00	2	1.6	330	PASS
174	95	50	120	91.8	20232	PASS
175	174	5	9	7.3	1480	PASS
176	174	95	101	97.5	19722	PASS
177	176	5	9	7.4	1457	PASS

m/z	Abundance
44.00	360.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	180.0
37.00	1058.0
38.00	917.0
38.90	397.0
40.00	189.0
43.90	548.0
45.00	207.0
47.00	180.0
47.80	146.0
49.00	843.0
50.10	4140.0
51.10	1406.0
55.90	268.0
57.00	503.0
60.00	180.0
61.00	1096.0
62.00	1261.0
63.00	1259.0
63.90	137.0
65.00	317.0
68.00	2413.0
69.00	2344.0
69.90	123.0
73.10	1188.0
74.00	3715.0
75.10	11013.0
76.00	966.0
77.00	171.0
78.90	990.0
80.00	251.0
80.90	995.0
81.80	224.0
87.00	969.0
88.00	946.0
91.90	733.0
93.00	935.0
94.00	3016.0
95.10	21688.0
96.10	1373.0
103.90	107.0
115.80	145.0
117.00	107.0
119.00	146.0
130.10	115.0
140.90	335.0
143.00	526.0
144.80	211.0
171.90	388.0
173.00	317.0
174.00	19352.0
174.90	1500.0
176.00	18888.0
176.90	1328.0
207.00	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	239.0
37.00	1016.0
38.00	1045.0
38.90	414.0
40.00	240.0
43.90	657.0
44.90	230.0
46.80	252.0
47.80	150.0
49.00	902.0
50.00	4446.0
51.10	1462.0
55.90	266.0
57.00	615.0
60.00	199.0
61.00	1108.0
62.00	1246.0
63.00	1215.0
64.00	140.0
65.00	305.0
68.00	2727.0
69.00	2403.0
69.90	149.0
72.00	106.0
73.10	1241.0
74.00	3869.0
75.10	11828.0
76.00	1064.0
76.90	185.0
78.90	955.0
80.00	270.0
80.90	1011.0
81.80	246.0
87.00	979.0
88.00	1076.0
92.00	725.0
93.00	1009.0
94.00	3128.0
95.00	22640.0
96.10	1457.0
103.90	151.0
115.90	128.0
116.90	129.0
117.80	100.0
118.90	145.0
130.00	140.0
140.90	350.0
143.00	568.0
144.90	267.0
172.00	432.0
172.90	329.0
174.00	20672.0
175.00	1504.0
176.00	20216.0
176.90	1495.0
207.00	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	262.0
37.00	960.0
38.00	1001.0
39.00	425.0
40.00	264.0
43.90	693.0
44.90	205.0
46.80	300.0
47.90	107.0
49.00	833.0
50.00	4201.0
51.10	1375.0
55.90	250.0
57.00	691.0
60.00	231.0
61.00	1048.0
62.00	1109.0
63.10	1071.0
64.00	170.0
65.00	339.0
68.00	2778.0
69.00	2233.0
69.90	142.0
71.90	107.0
73.10	1057.0
74.00	3747.0
75.10	11352.0
76.10	1004.0
76.90	203.0
78.90	840.0
80.00	235.0
80.90	925.0
81.80	236.0
87.00	1031.0
88.00	1029.0
92.00	663.0
93.00	1021.0
94.00	2916.0
95.00	21816.0
96.10	1414.0
103.90	173.0
116.90	152.0
117.80	133.0
118.90	136.0
130.00	113.0
141.00	358.0
143.00	577.0
145.00	262.0
172.00	541.0
172.80	346.0
174.00	20672.0
175.00	1437.0
176.00	20064.0
176.90	1549.0
207.00	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43