


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082520\
Data File : VU039968.D
Acq On : 25 Aug 2020 15:20
Operator : SY/MD
Sample : L3777-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
F4Y24

Manual Integrations
APPROVED

sam
8/26/2020 5:20:07 PM

Quant Time: Aug 26 04:21:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 26 03:42:21 2020
Response via : Initial Calibration

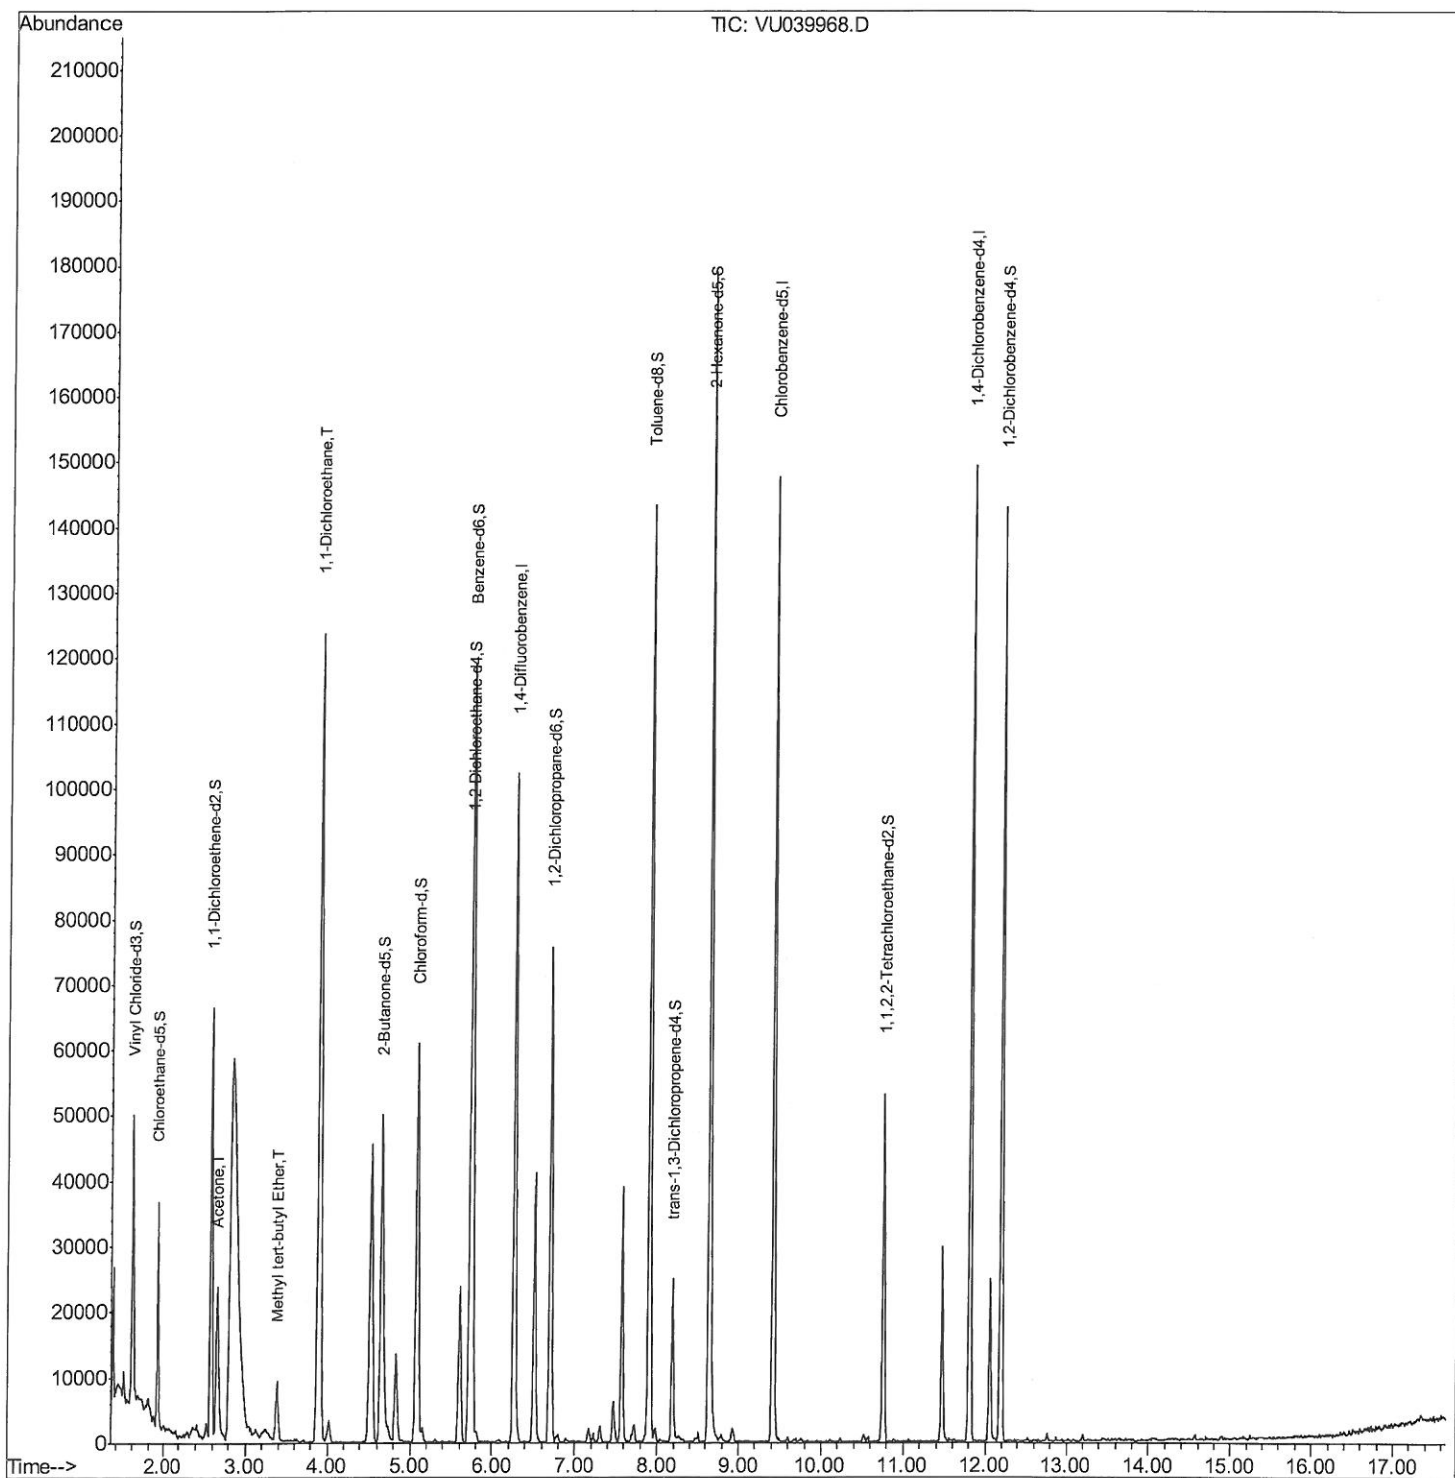

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082520\
 Data File : VU039968.D
 Acq On : 25 Aug 2020 15:20
 Operator : SY/MD
 Sample : L3777-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4Y24

Manual Integrations
 APPROVED

sam
 8/26/2020 5:20:07 PM

Quant Time: Aug 26 03:45:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 26 03:42:21 2020
 Response via : Initial Calibration

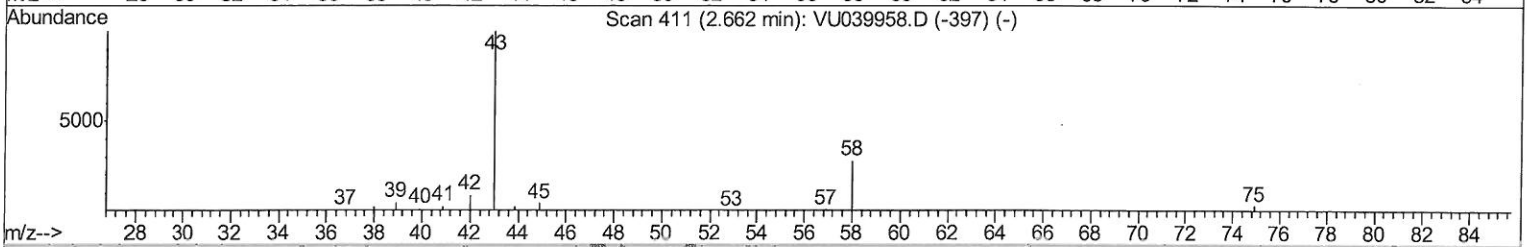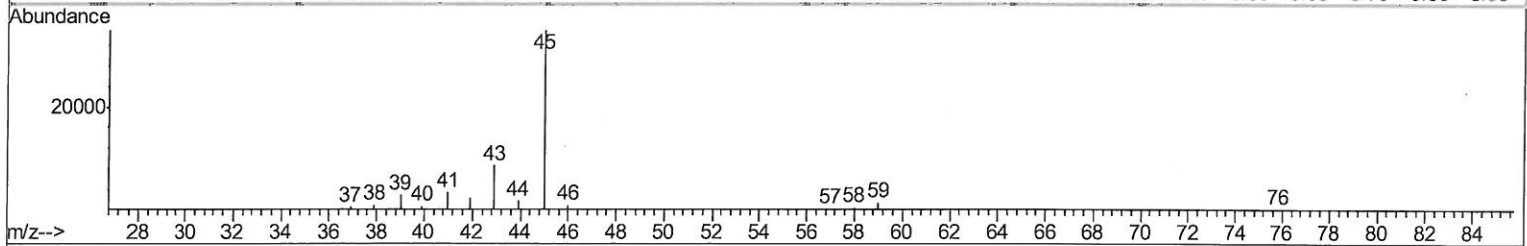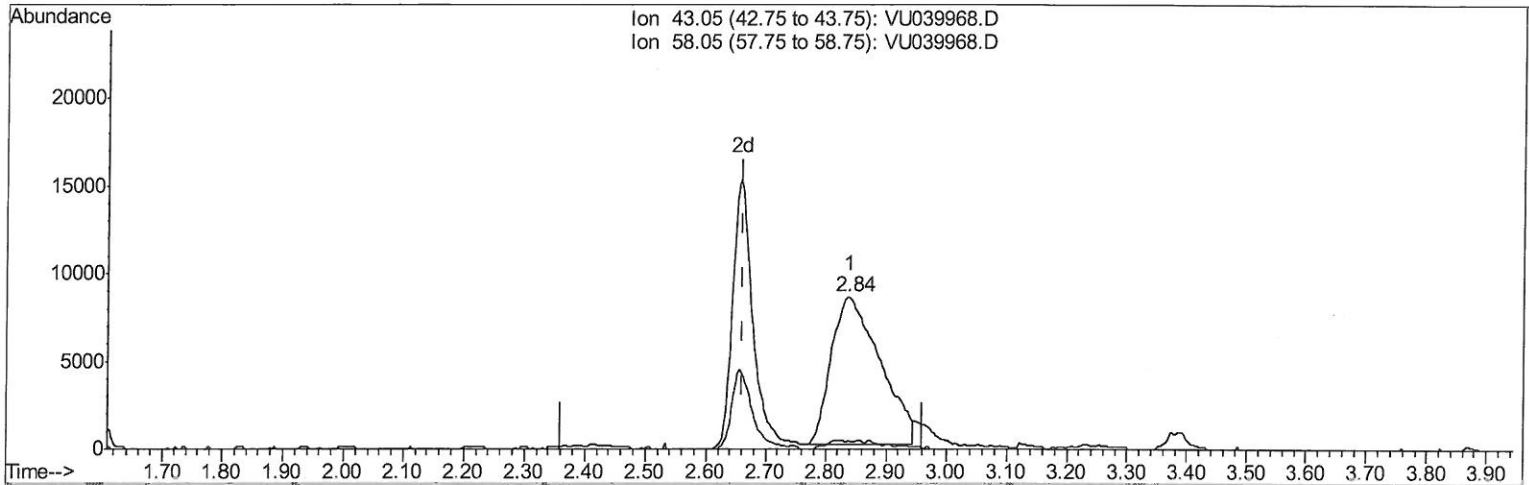

TIC: VU039968.D

(13) Acetone (T)

2.838min (+0.177) 32.68ug/L

response 47546

Ion	Exp%	Act%
43.05	100	100
58.05	9.50	2.22
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082520\
 Data File : VU039968.D
 Acq On : 25 Aug 2020 15:20
 Operator : SY/MD
 Sample : L3777-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4Y24

Manual Integrations
 APPROVED

sam
 8/26/2020 5:20:07 PM

Quant Time: Aug 26 03:45:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 26 03:42:21 2020
 Response via : Initial Calibration

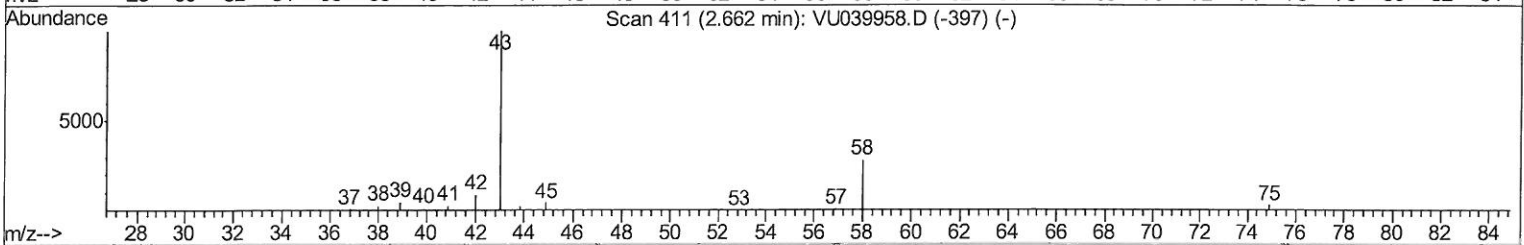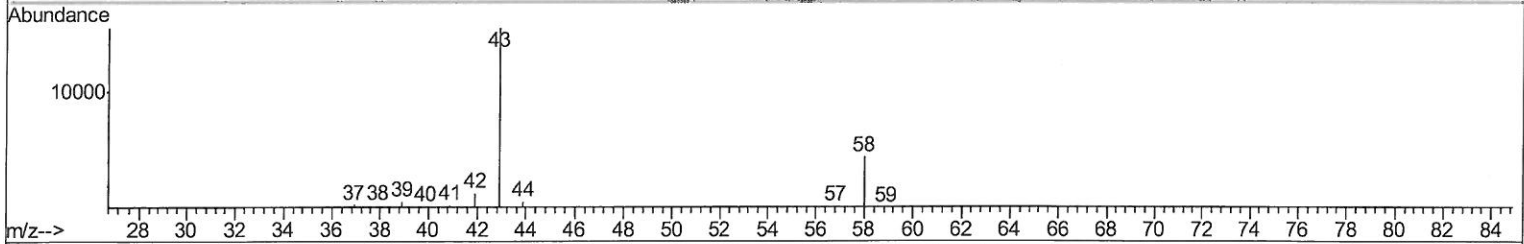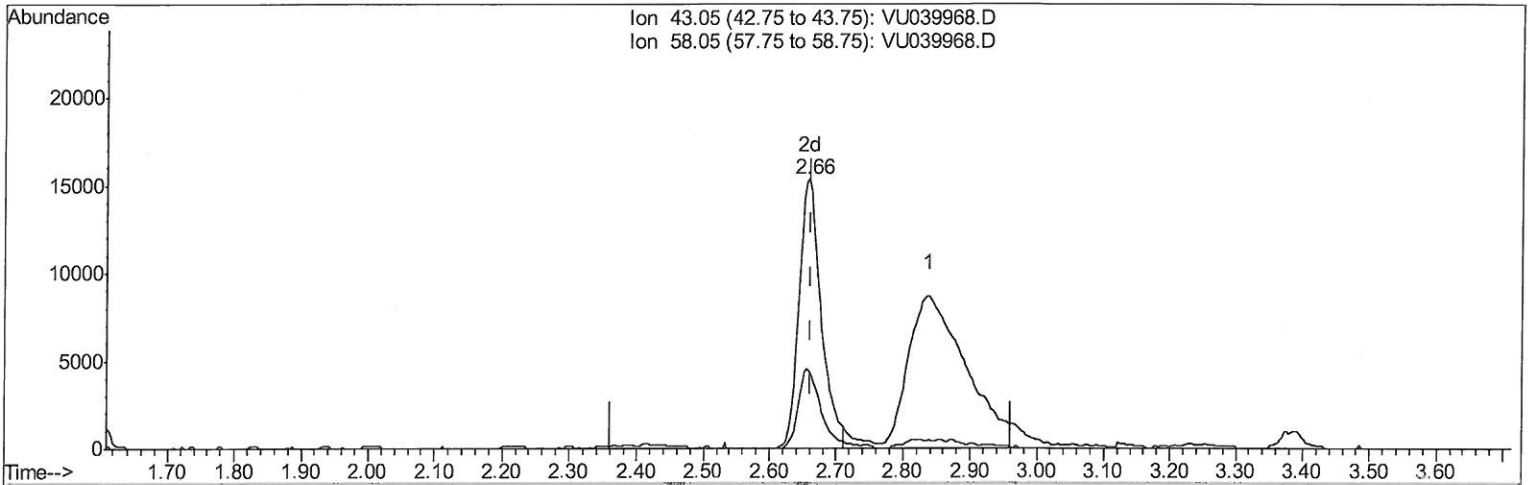

TIC: VU039968.D

(13) Acetone (T)

2.658min (-0.003) 24.21ug/L m

response 35220

Ion	Exp%	Act%
43.05	100	100
58.05	9.50	3.00
0.00	0.00	0.00
0.00	0.00	0.00

MD
8/31/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082520\
 Data File : VU039968.D
 Acq On : 25 Aug 2020 15:20
 Operator : SY/MD
 Sample : L3777-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4Y24

Manual Integrations
 APPROVED

sam
 8/26/2020 5:20:07 PM

Quant Time: Aug 26 04:21:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 26 03:42:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	76274	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	74177	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	35310	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	25903	3.89	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.80%
7) Chloroethane-d5	1.92	69	21582	3.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.40%
11) 1,1-Dichloroethene-d2	2.58	63	39428	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	4.65	46	81711	38.38	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	76.76%
24) Chloroform-d	5.09	84	52661	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
26) 1,2-Dichloroethane-d4	5.72	65	30766	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
32) Benzene-d6	5.75	84	100538	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.70	67	32391	4.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.80%
41) Toluene-d8	7.91	98	84421	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	8.19	79	12199	3.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.80%
46) 2-Hexanone-d5	8.64	63	57070	36.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.58%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	24851	3.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	76.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	34114	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%

Target Compounds

Target Compounds				Ovalue
13) Acetone	2.66	43	35220m	24.208 ug/L
17) Methyl tert-butyl Ether	3.38	73	8177	0.486 ug/L #
19) 1,1-Dichloroethane	3.89	63	136737	10.646 ug/L

2 MD
 8/31/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed