

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082520\
 Data File : VU039967.D
 Acq On : 25 Aug 2020 14:56
 Operator : SY/MD
 Sample : L3776-04DL 5000X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4Y03DL

Quant Time: Aug 26 04:17:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 26 03:42:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	70018	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	67688	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	30599	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	25839	4.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.60%
7) Chloroethane-d5	1.92	69	23227	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.58	63	41378	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	4.66	46	85533	43.76	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.52%
24) Chloroform-d	5.09	84	53585	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	5.72	65	32387	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.74	84	102148	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
36) 1,2-Dichloropropane-d6	6.71	67	33292	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.91	98	86330	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
43) trans-1,3-Dichloropropene-	8.19	79	12007	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
46) 2-Hexanone-d5	8.64	63	59729	42.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.38%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	25371	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	34054	5.64	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.80%


Target Compounds					Ovalue
33) Benzene	5.79	78	277557	11.283 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082520\
Data File : VU039967.D
Acq On : 25 Aug 2020 14:56
Operator : SY/MD
Sample : L3776-04DL 5000X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4Y03DL

Quant Time: Aug 26 04:17:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 26 03:42:21 2020
Response via : Initial Calibration

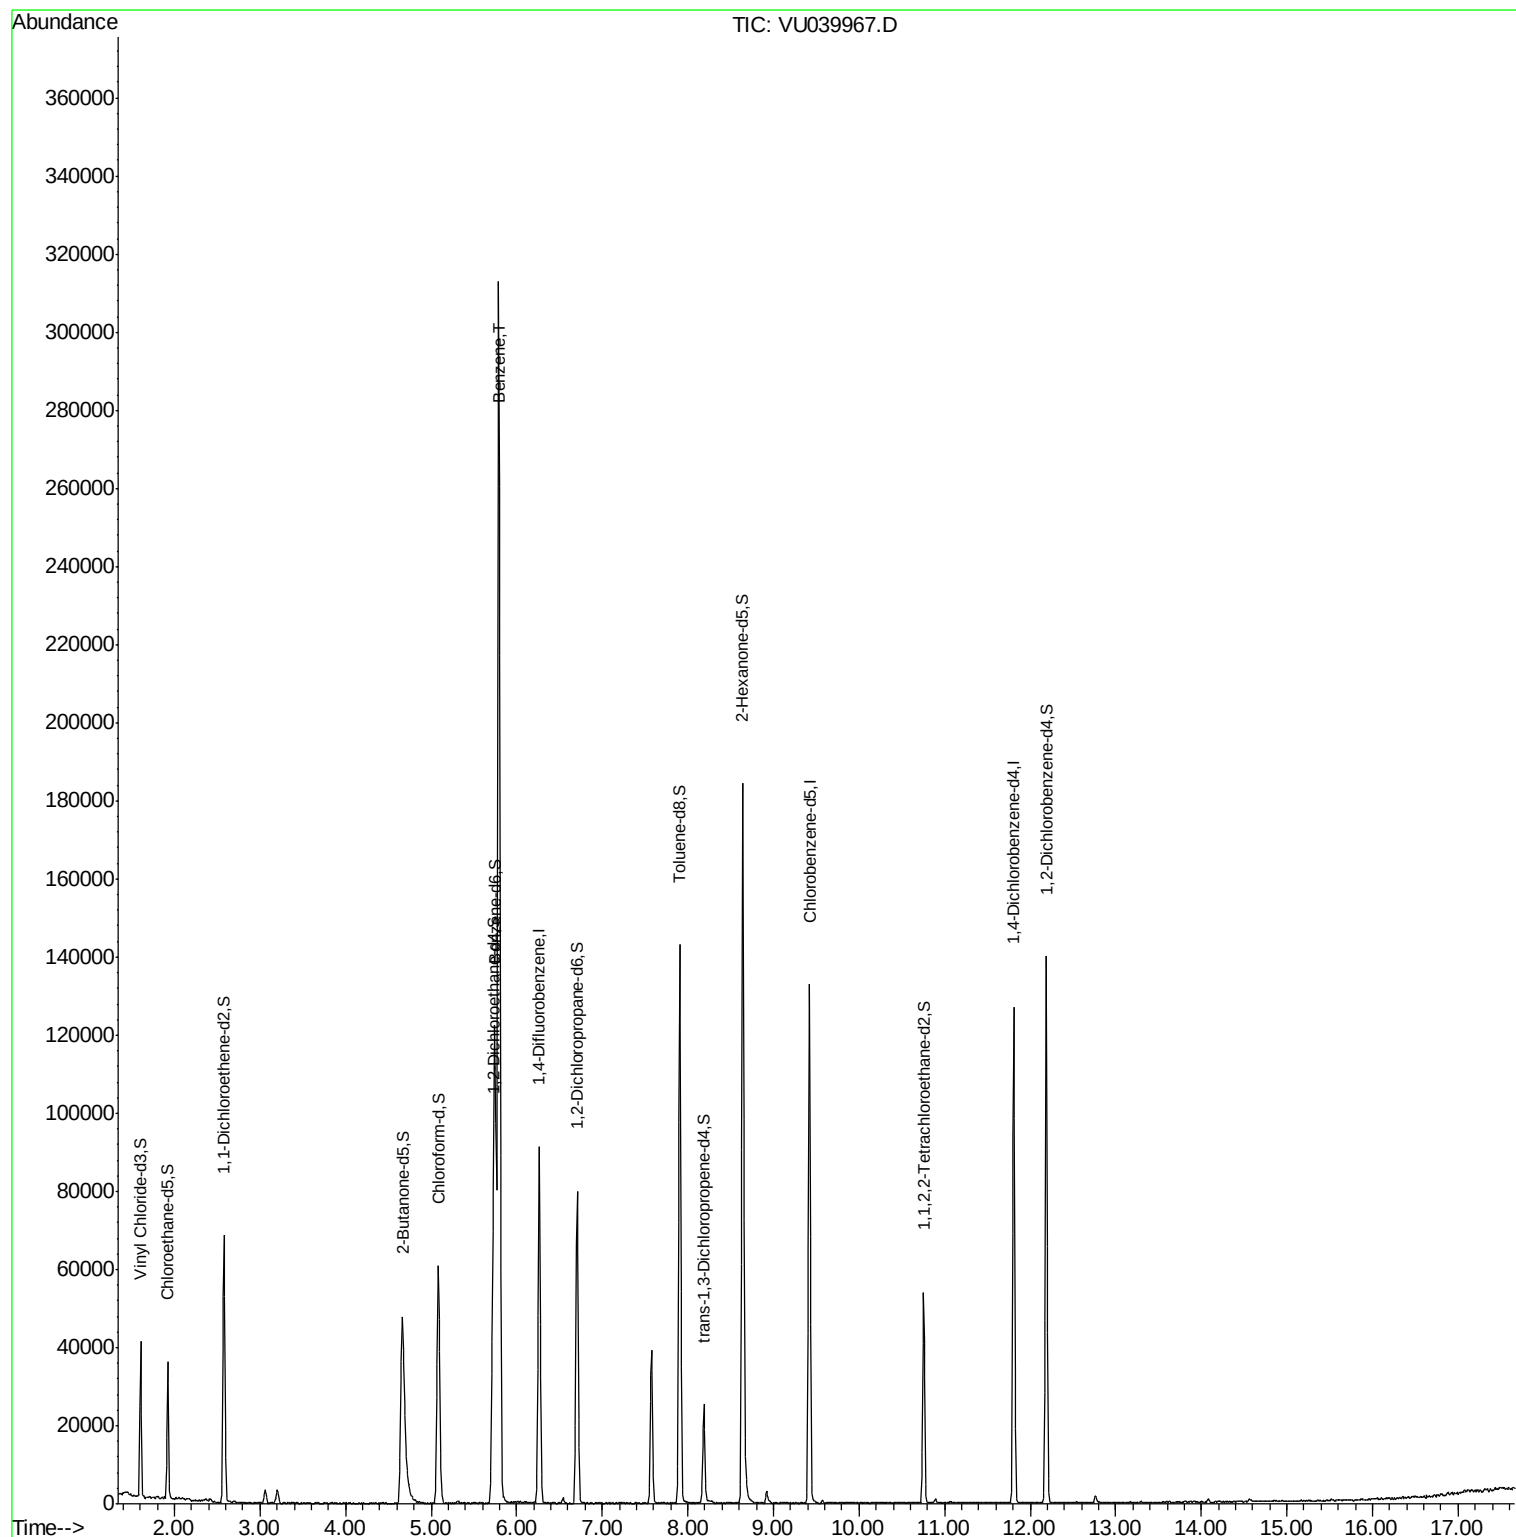

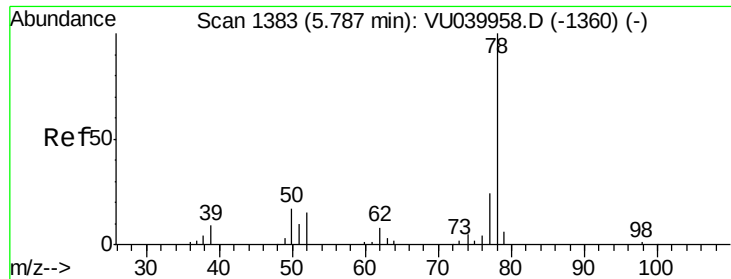

#33

Benzene

Concen: 11.283 ug/L

RT: 5.79 min Scan# 1385

Delta R.T. 0.01 min

Lab File: VU039967.D

Acq: 25 Aug 2020 14:56

Instrument :

MSVOA_U

ClientSampleId :

F4Y03DL

Tgt Ion: 78 Resp: 277557

