


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082520\
Data File : VU039957.D
Acq On : 25 Aug 2020 10:00
Operator : SY/MD
Sample : BFB21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB21

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 26 03:42:21 2020

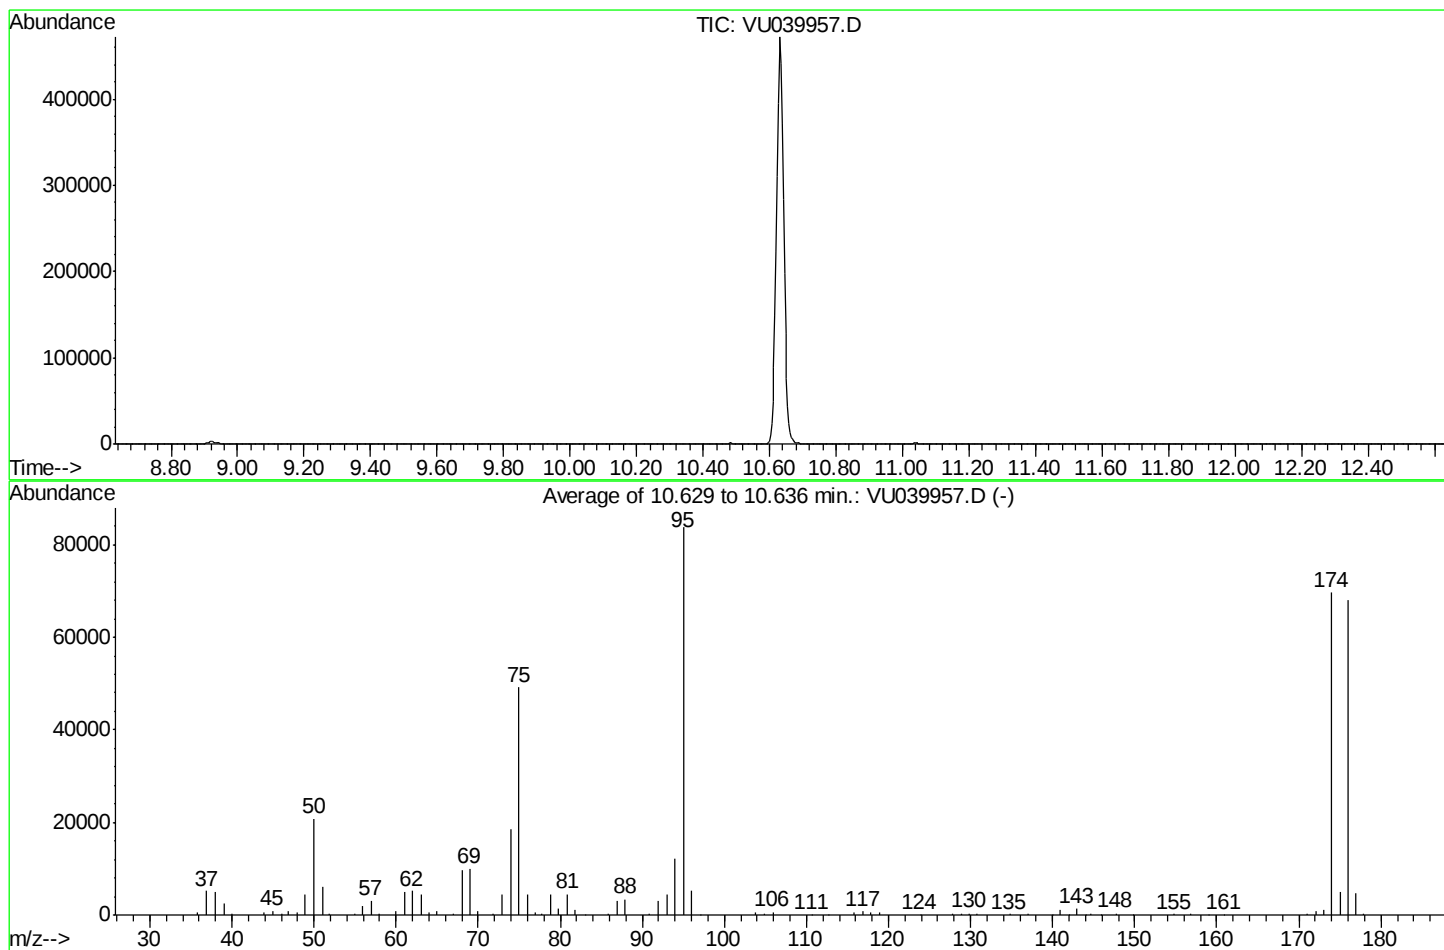

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	20786	PASS
75	95	30	80	58.7	49192	PASS
95	95	100	100	100.0	83741	PASS
96	95	5	9	6.3	5257	PASS
173	174	0.00	2	1.5	1029	PASS
174	95	50	120	83.2	69637	PASS
175	174	5	9	7.2	5031	PASS
176	174	95	101	97.6	67981	PASS
177	176	5	9	6.7	4583	PASS

m/z	Abundance
35.80	648.0
36.90	5369.0
37.90	5051.0
39.00	2549.0
40.00	191.0
43.90	901.0
44.90	992.0
46.00	185.0
46.80	891.0
47.90	595.0
48.90	4505.0
50.00	21272.0
51.00	6049.0
51.90	265.0
54.90	281.0
55.90	1846.0
56.90	3136.0
58.00	176.0
60.00	889.0
61.00	4952.0
62.00	5265.0
63.00	4567.0
63.90	652.0
64.90	850.0
67.00	419.0
68.00	10001.0
68.90	10126.0
69.90	755.0
71.90	391.0
72.90	4662.0
74.00	18488.0
75.00	49808.0
76.00	4509.0
76.90	585.0
77.80	383.0
78.90	4561.0
79.80	1225.0
80.90	4521.0
81.80	1104.0
85.80	249.0
86.90	3293.0
87.90	3295.0
90.80	426.0
91.90	3211.0
93.00	4310.0
94.00	12273.0
95.00	83576.0
96.00	5335.0
97.10	135.0
103.70	554.0
104.80	188.0
105.90	586.0
110.70	128.0
112.70	134.0
115.80	455.0
116.90	696.0
117.80	428.0
118.90	632.0
127.80	368.0
128.90	162.0
129.90	390.0
130.80	199.0
134.80	238.0
136.90	253.0
140.00	122.0
140.90	1078.0
142.00	129.0
142.90	1323.0
144.00	157.0
144.70	229.0
146.00	134.0
147.70	271.0
154.80	212.0
156.70	116.0
159.00	102.0
160.90	114.0
171.00	205.0
172.00	972.0
173.00	1110.0
174.00	67496.0
175.00	5068.0
176.00	66576.0
177.00	4596.0
177.90	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
35.80	672.0
36.90	5389.0
37.90	5086.0
39.00	2588.0
40.00	213.0
43.90	845.0
44.90	945.0
46.00	205.0
46.80	1005.0
47.90	523.0
48.90	4494.0
50.00	21520.0
51.00	6314.0
51.90	301.0
55.00	246.0
55.90	1956.0
56.90	3216.0
58.00	181.0
59.90	949.0
61.00	5137.0
62.00	5460.0
63.00	4663.0
63.90	602.0
64.90	790.0
67.00	404.0
68.00	10039.0
69.00	10470.0
70.00	872.0
71.80	387.0
72.90	4696.0
74.00	19208.0
75.00	50752.0
76.00	4579.0
77.00	533.0
77.80	357.0
78.90	4621.0
79.80	1301.0
80.90	4716.0
81.80	1218.0
83.00	157.0
85.90	251.0
86.90	3187.0
87.90	3379.0
90.80	388.0
91.90	3250.0
93.00	4484.0
94.00	12410.0
95.00	87112.0
96.00	5400.0
97.00	104.0
103.80	547.0
104.90	170.0
105.90	629.0
110.70	131.0
112.70	102.0
115.90	457.0
116.90	728.0
117.80	488.0
118.90	623.0
127.80	362.0
128.90	160.0
129.90	420.0
130.80	232.0
134.80	251.0
136.90	236.0
140.00	116.0
140.90	1197.0
142.00	135.0
143.00	1309.0
144.00	128.0
144.70	225.0
145.90	113.0
147.80	317.0
149.80	105.0
154.80	253.0
156.80	158.0
159.00	102.0
160.90	117.0
171.00	192.0
172.00	1004.0
173.00	1048.0
174.00	72024.0
175.00	5161.0
176.00	70360.0
177.00	4741.0
177.90	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
35.80	628.0
36.90	4857.0
37.90	4545.0
39.00	2307.0
40.00	206.0
44.00	852.0
45.00	820.0
46.00	211.0
46.80	953.0
47.90	439.0
48.90	3893.0
50.00	19568.0
51.00	6217.0
51.90	279.0
55.00	231.0
56.00	1756.0
57.00	3101.0
58.00	137.0
59.90	863.0
61.00	4675.0
61.90	4897.0
63.00	4201.0
64.00	481.0
64.90	595.0
66.90	316.0
68.00	9177.0
69.00	9650.0
70.00	875.0
71.70	398.0
72.90	4311.0
74.00	17752.0
75.00	47016.0
76.00	4465.0
77.00	451.0
77.80	326.0
78.80	4118.0
79.80	1277.0
80.90	4467.0
81.80	1122.0
83.00	190.0
85.90	198.0
86.90	2901.0
87.90	3314.0
90.80	325.0
91.90	2916.0
93.00	4215.0
94.00	11604.0
95.00	80536.0
96.00	5036.0
103.80	496.0
104.90	169.0
105.90	591.0
115.90	400.0
116.90	717.0
117.80	478.0
118.90	567.0
123.90	112.0
127.80	327.0
128.90	138.0
129.90	409.0
130.80	231.0
134.80	211.0
137.00	190.0
139.90	113.0
140.90	1232.0
142.00	123.0
142.90	1148.0
144.70	188.0
145.80	114.0
147.80	271.0
149.80	123.0
154.90	279.0
156.80	200.0
171.00	134.0
172.10	939.0
173.00	930.0
174.00	69392.0
175.00	4865.0
176.00	67008.0
177.00	4413.0
177.80	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
43.90	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21