

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082522\
 Data File : VU050439.D
 Acq On : 25 Aug 2022 10:47
 Operator : SY/MD
 Sample : VU0825WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0825WBL01

Quant Time: Aug 26 06:33:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Aug 25 14:01:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.108	96	37103	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	9583	0.759	ug/l	0.00
Spiked Amount 1.000			Recovery	=	76.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	10626	0.712	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082522\
Data File : VU050439.D
Acq On : 25 Aug 2022 10:47
Operator : SY/MD
Sample : VU0825WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0825WBL01


Quant Time: Aug 26 06:33:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Aug 25 14:01:59 2022
Response via : Initial Calibration

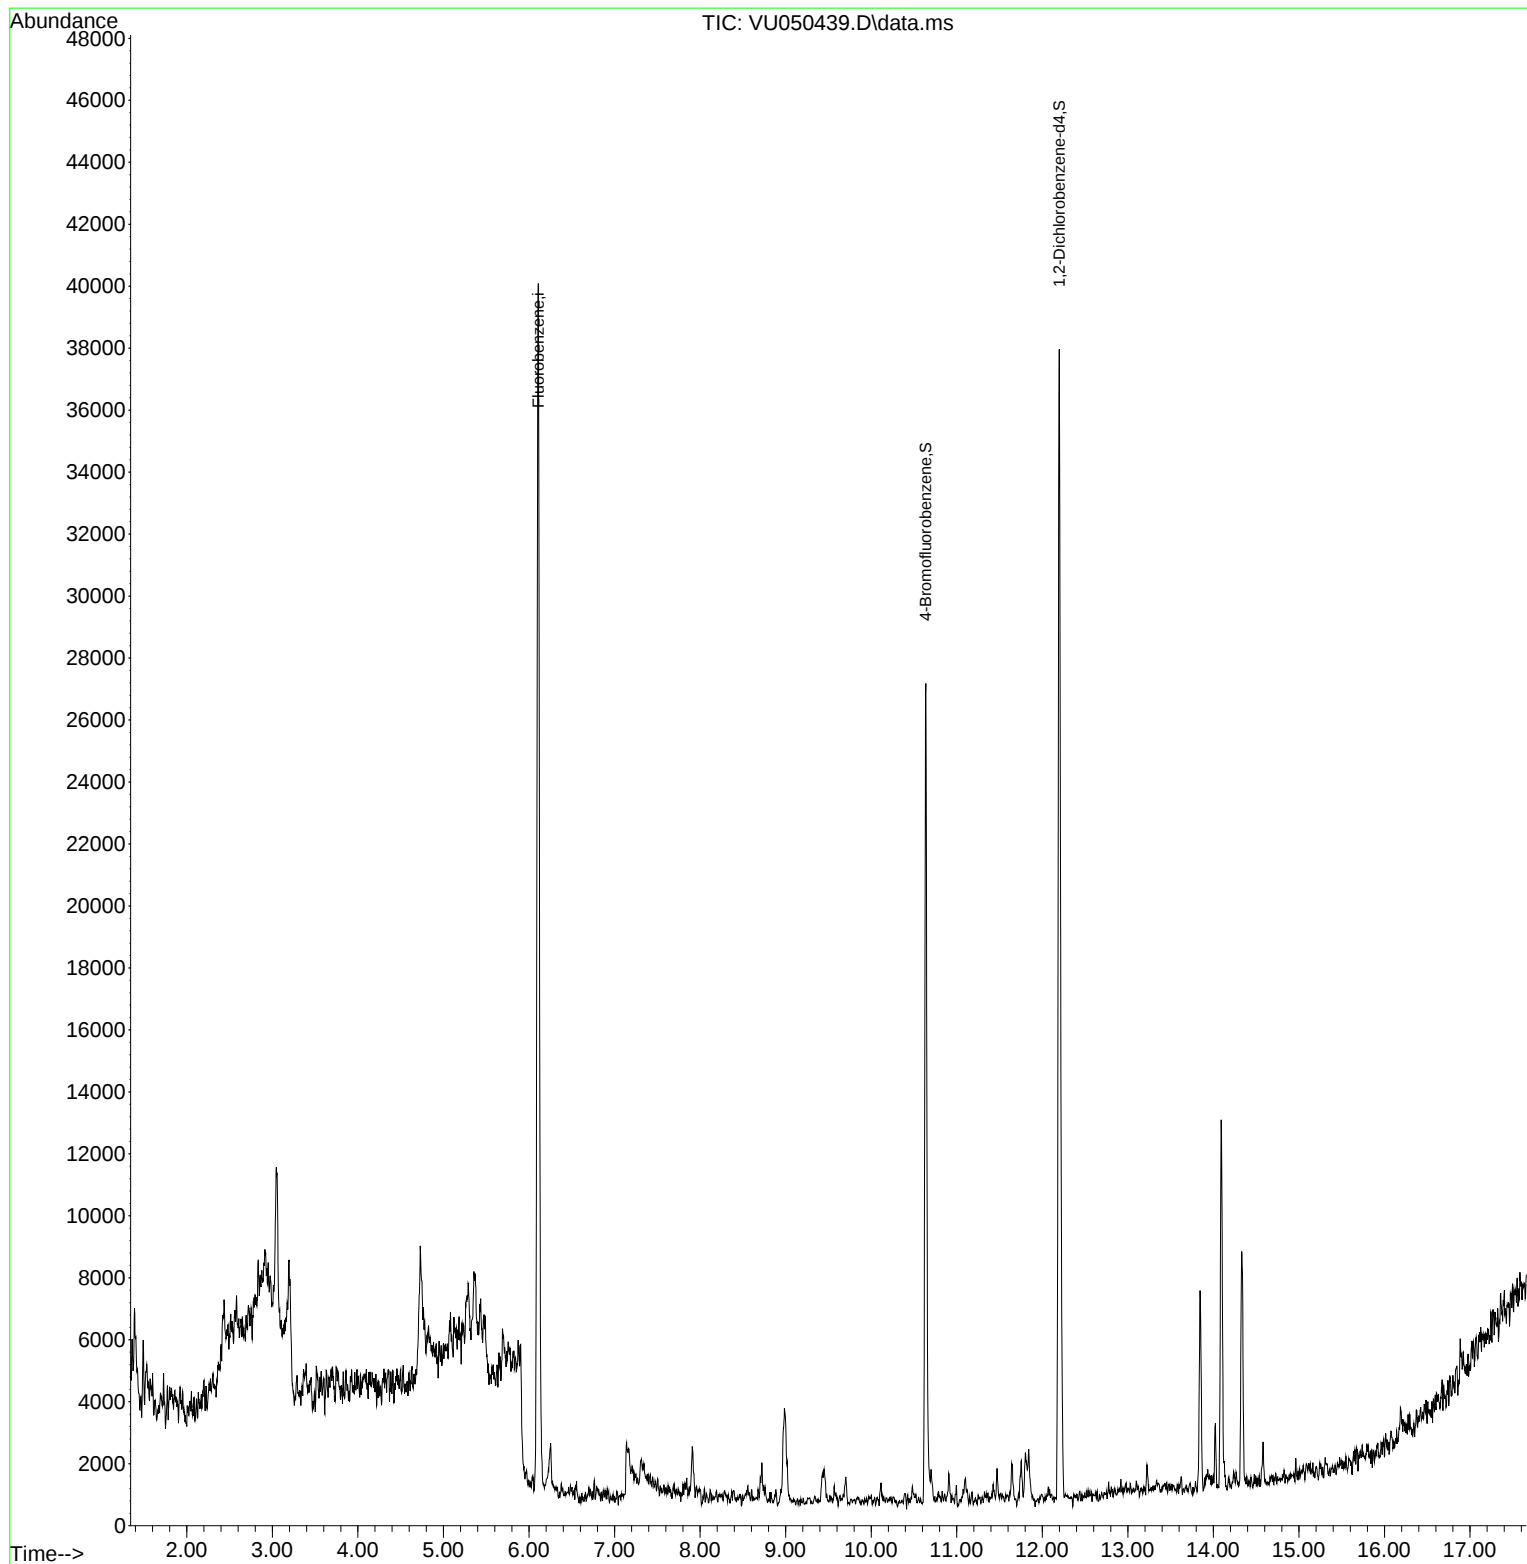

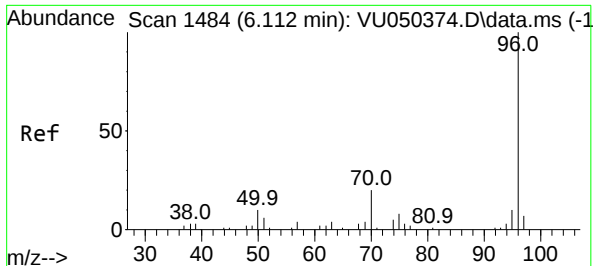




#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.108 min Scan# 1483
Delta R.T. -0.007 min
Lab File: VU050439.D
Acq: 25 Aug 2022 10:47

Instrument :
MSVOA_U
ClientSampleId :
VU0825WBL01

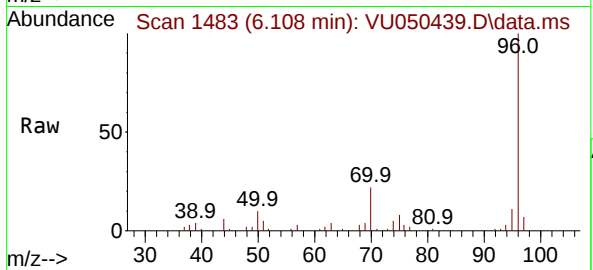

Tgt Ion: 96 Resp: 37103




Ion	Ratio	Lower	Upper
96	100		
70	21.6	16.7	25.1
95	10.0	7.4	11.0
97	6.5	0.0	0.0

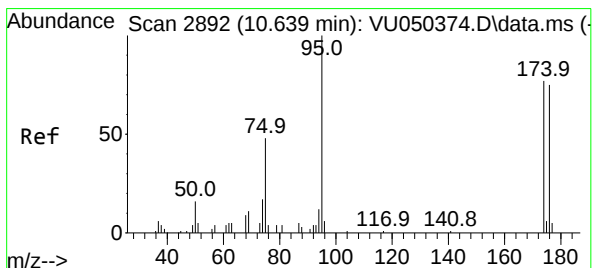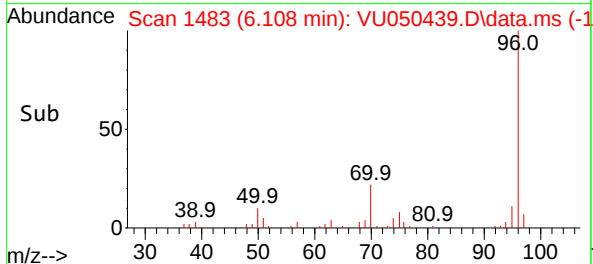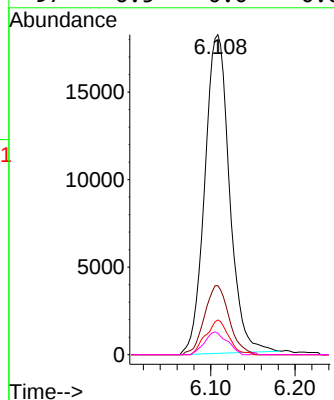


#57
4-Bromofluorobenzene
Concen: 0.759 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.006 min
Lab File: VU050439.D
Acq: 25 Aug 2022 10:47

Tgt Ion: 95 Resp: 9583


Ion	Ratio	Lower	Upper
95	100		
174	79.3	62.4	93.6
176	79.6	56.2	84.2

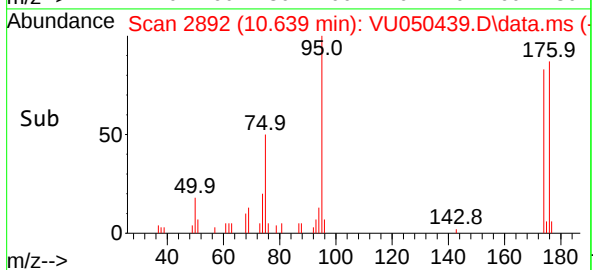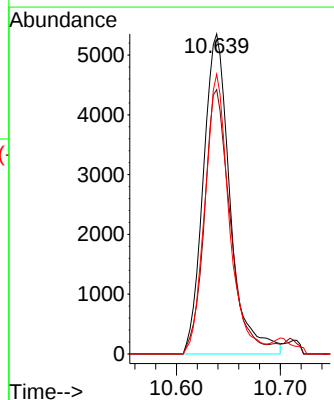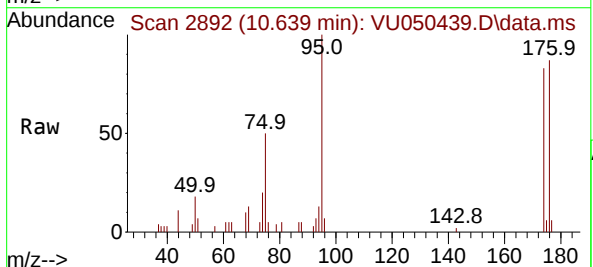

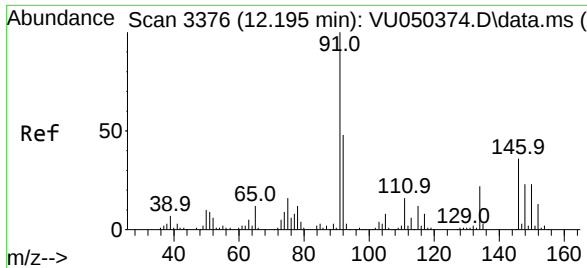

#68
1,2-Dichlorobenzene-d4
Concen: 0.712 ug/l
RT: 12.198 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU050439.D
Acq: 25 Aug 2022 10:47

Instrument :
MSVOA_U
ClientSampleId :
VU0825WBL01

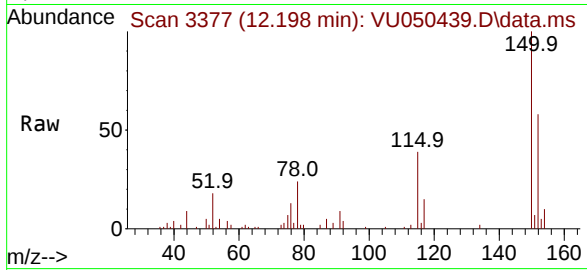

Tgt Ion:152 Resp: 10626
Ion Ratio Lower Upper
152 100
115 64.0 0.0 254.6
150 164.9 0.0 623.6

