


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082522\
 Data File : VU050437.D
 Acq On : 25 Aug 2022 08:57
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Aug 25 14:01:59 2022

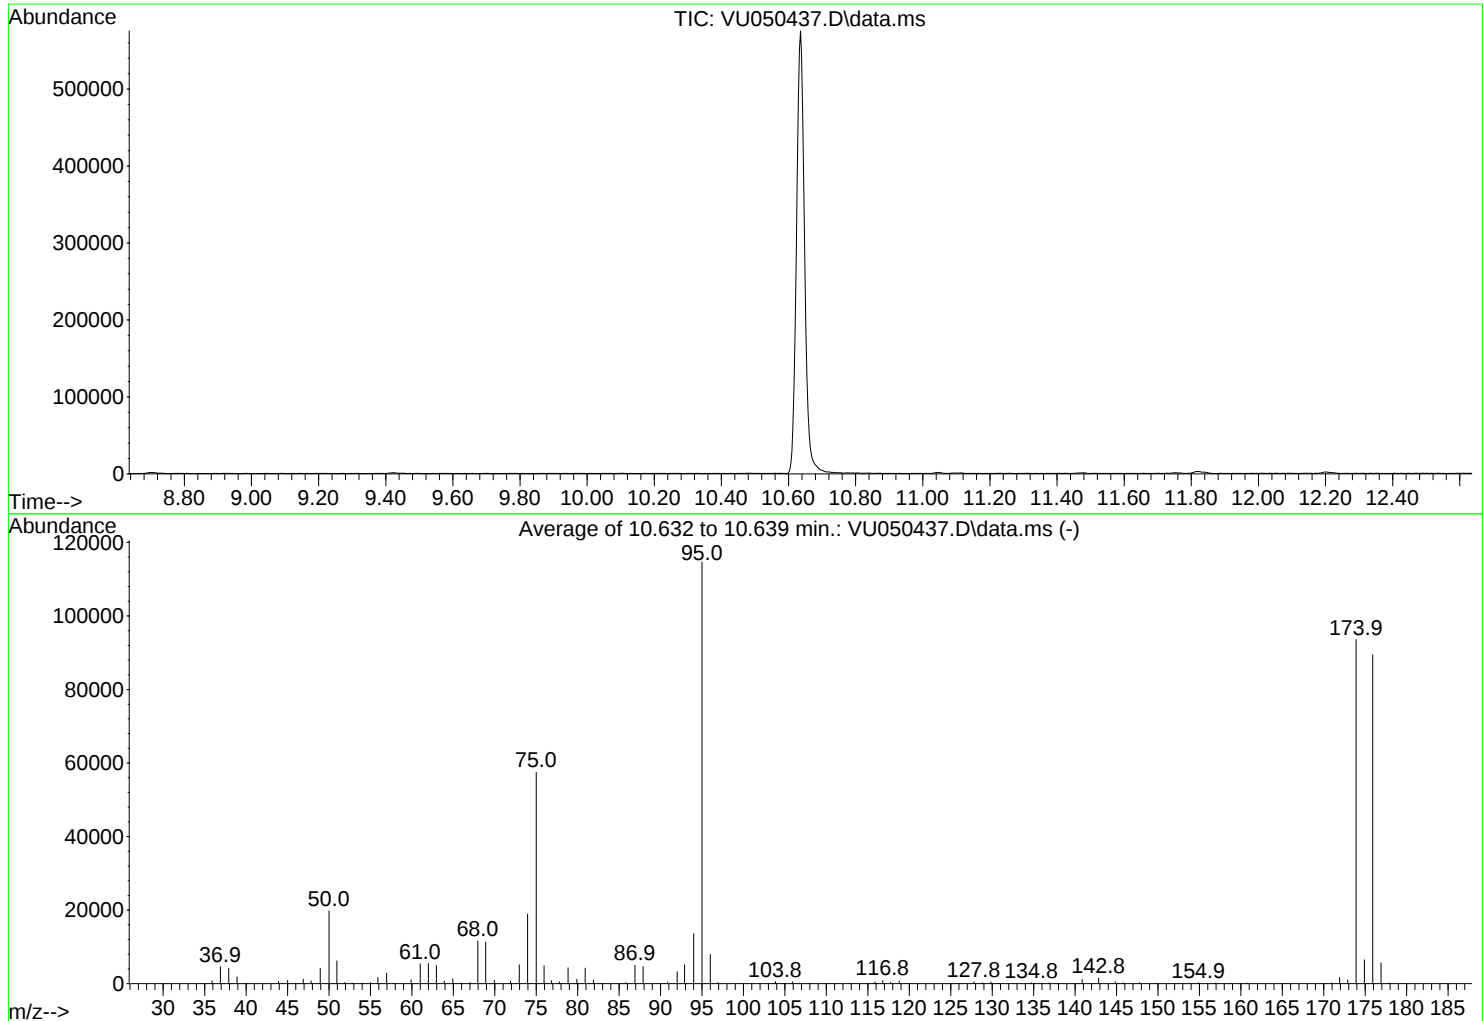

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	19792	PASS
75	95	30	60	50.1	57453	PASS
95	95	100	100	100.0	114717	PASS
96	95	5	9	7.0	7977	PASS
173	174	0.00	2	1.1	1004	PASS
174	95	50	100	81.6	93592	PASS
175	174	5	9	7.0	6507	PASS
176	174	95	101	95.5	89413	PASS
177	176	5	9	6.3	5656	PASS