


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU082619\
 Data File : VU033945.D
 Acq On : 26 Aug 2019 08:49
 Operator : JC/SP
 Sample : BFB05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082619WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Aug 27 01:58:06 2019

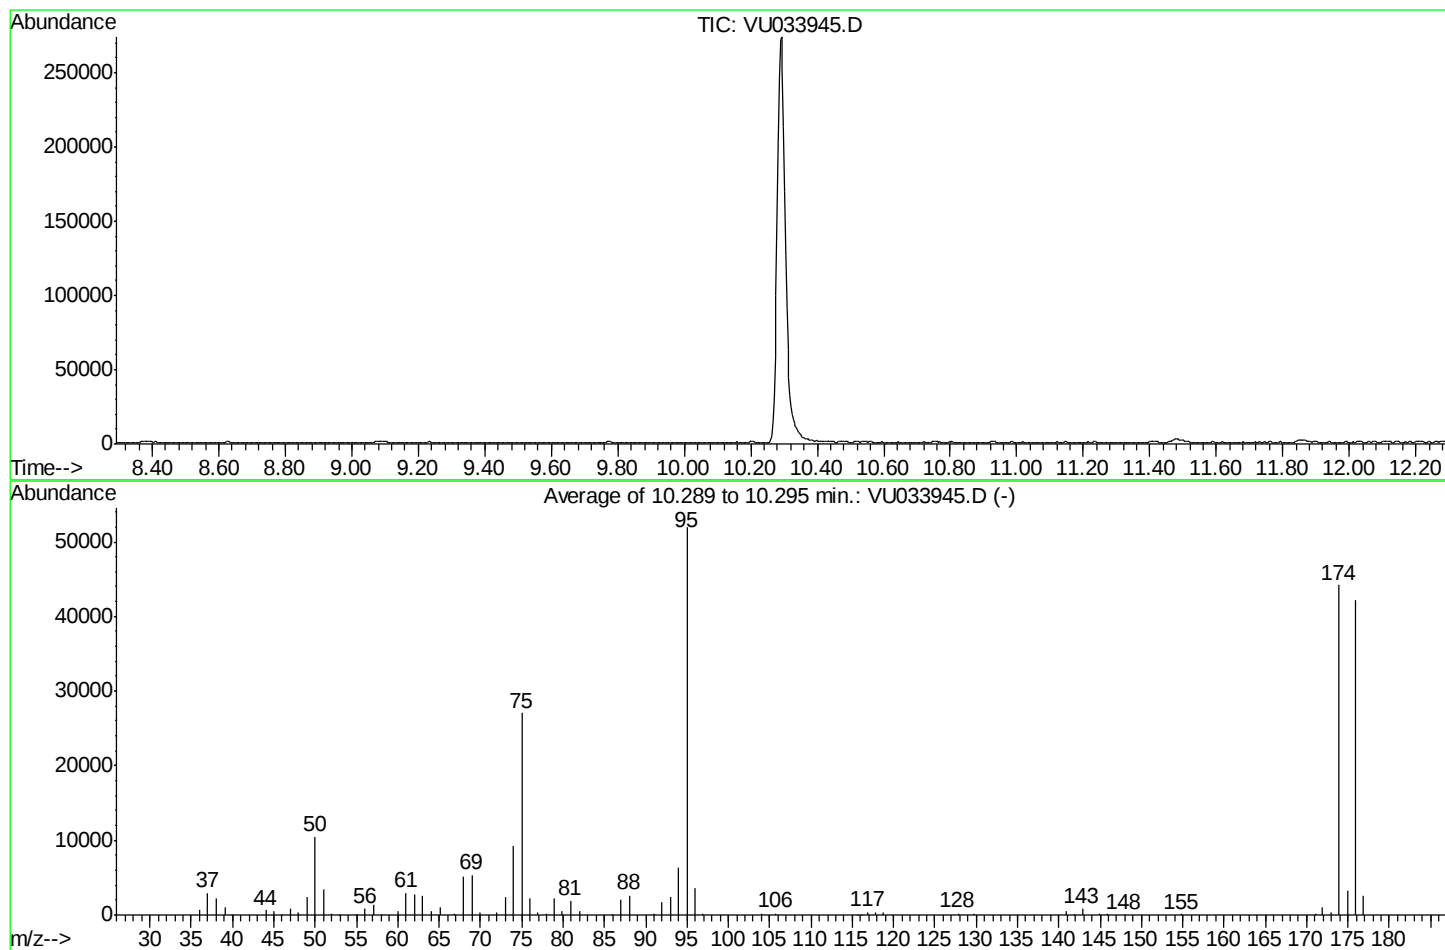

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	10470	PASS
75	95	30	80	52.0	27032	PASS
95	95	100	100	100.0	51944	PASS
96	95	5	9	6.9	3560	PASS
173	174	0.00	2	0.9	408	PASS
174	95	50	120	85.1	44205	PASS
175	174	5	9	7.3	3220	PASS
176	174	95	101	95.6	42258	PASS
177	176	5	9	6.3	2655	PASS

m/z	Abundance
39.90	557.0
44.00	495.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	681.0
37.00	3080.0
38.00	2387.0
39.10	1161.0
40.00	512.0
44.00	1159.0
45.00	478.0
46.00	124.0
47.00	852.0
48.00	383.0
49.00	2318.0
50.00	10882.0
51.00	3556.0
52.00	171.0
54.90	151.0
56.10	767.0
57.10	1449.0
60.00	501.0
61.00	3253.0
62.00	2938.0
63.00	2591.0
64.00	508.0
65.10	902.0
66.90	187.0
68.00	5549.0
69.00	5472.0
70.00	345.0
72.00	289.0
73.00	2495.0
74.00	9676.0
75.00	27912.0
76.00	2446.0
76.90	357.0
78.00	307.0
78.90	2194.0
79.90	543.0
80.90	1988.0
82.00	506.0
85.90	108.0
87.00	2254.0
88.00	2645.0
90.90	165.0
92.00	1678.0
93.00	2388.0
94.00	6570.0
95.00	53240.0
96.00	3645.0
96.90	153.0
104.00	211.0
105.80	218.0
115.70	123.0
116.90	400.0
117.80	269.0
118.80	294.0
127.80	237.0
129.80	230.0
140.90	650.0
141.80	113.0
142.90	804.0
144.80	254.0
145.80	143.0
148.00	153.0
154.90	154.0
171.10	139.0
171.90	844.0
173.90	44264.0
175.00	3474.0
175.90	42688.0
176.90	2757.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	667.0
37.00	3035.0
38.00	2339.0
39.10	1007.0
39.90	571.0
44.00	1107.0
45.00	552.0
45.90	109.0
47.00	842.0
48.00	351.0
49.00	2436.0
50.00	10815.0
51.00	3477.0
51.90	171.0
55.10	137.0
56.00	862.0
57.10	1364.0
60.00	545.0
61.00	2981.0
62.00	2822.0
63.00	2607.0
64.00	450.0
65.10	992.0
66.90	198.0
68.00	5333.0
69.00	5559.0
70.00	329.0
71.90	373.0
73.00	2390.0
74.00	9538.0
75.00	27832.0
76.00	2367.0
76.90	429.0
78.00	273.0
78.90	2269.0
79.90	502.0
80.90	2008.0
82.00	497.0
86.90	2195.0
88.00	2724.0
91.00	176.0
92.00	1689.0
93.00	2367.0
94.00	6599.0
95.00	53272.0
96.00	3622.0
96.90	160.0
103.90	215.0
105.80	265.0
115.70	107.0
116.00	101.0
117.00	421.0
117.80	291.0
118.80	317.0
127.80	215.0
129.80	205.0
140.90	552.0
142.80	798.0
144.90	244.0
145.90	141.0
148.00	113.0
154.90	139.0
171.00	138.0
171.90	1068.0
172.90	617.0
173.90	45800.0
175.00	3275.0
175.90	43440.0
176.90	2725.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
35.90	565.0
37.00	2721.0
38.00	2206.0
39.00	903.0
39.90	627.0
44.00	1046.0
45.00	566.0
47.00	708.0
48.00	315.0
49.00	2349.0
50.00	9713.0
51.00	3116.0
51.90	145.0
52.90	109.0
55.10	126.0
56.00	858.0
57.10	1145.0
58.00	111.0
60.00	504.0
61.00	2532.0
62.00	2486.0
63.00	2355.0
64.00	405.0
65.10	988.0
66.90	170.0
68.00	4738.0
69.00	4957.0
70.00	315.0
71.90	432.0
73.10	2191.0
74.00	8781.0
75.00	25352.0
76.00	2088.0
77.00	399.0
78.00	203.0
79.00	2039.0
79.90	447.0
80.90	1847.0
81.90	427.0
87.00	1960.0
88.00	2498.0
91.00	173.0
91.90	1617.0
93.00	2298.0
94.00	5967.0
95.00	49320.0
96.00	3413.0
96.90	119.0
103.90	198.0
105.80	275.0
116.10	163.0
116.90	414.0
117.80	254.0
118.80	369.0
127.90	169.0
129.80	182.0
140.90	455.0
142.80	794.0
144.90	236.0
145.90	107.0
171.00	115.0
171.90	1114.0
173.00	607.0
173.90	42552.0
175.00	2911.0
175.90	40648.0
176.90	2483.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05