

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082620\
 Data File : VU039983.D
 Acq On : 26 Aug 2020 15:05
 Operator : SY/MD
 Sample : L3807-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Quant Time: Aug 27 01:23:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Aug 27 00:51:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	71036	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	69356	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	31206	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	25900	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%
7) Chloroethane-d5	1.92	69	22399	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.20%
11) 1,1-Dichloroethene-d2	2.58	63	41199	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	4.65	46	91308	46.05	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.10%
24) Chloroform-d	5.08	84	55282	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.72	65	34393	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.75	84	104827	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.70	67	34711	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.91	98	87472	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
43) trans-1,3-Dichloropropene-	8.19	79	13762	4.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.20%
46) 2-Hexanone-d5	8.64	63	63649	43.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.76%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	27140	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	34549	5.61	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.20%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	2408	0.282 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082620\
Data File : VU039983.D
Acq On : 26 Aug 2020 15:05
Operator : SY/MD
Sample : L3807-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Time: Aug 27 01:23:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 27 00:51:02 2020
Response via : Initial Calibration

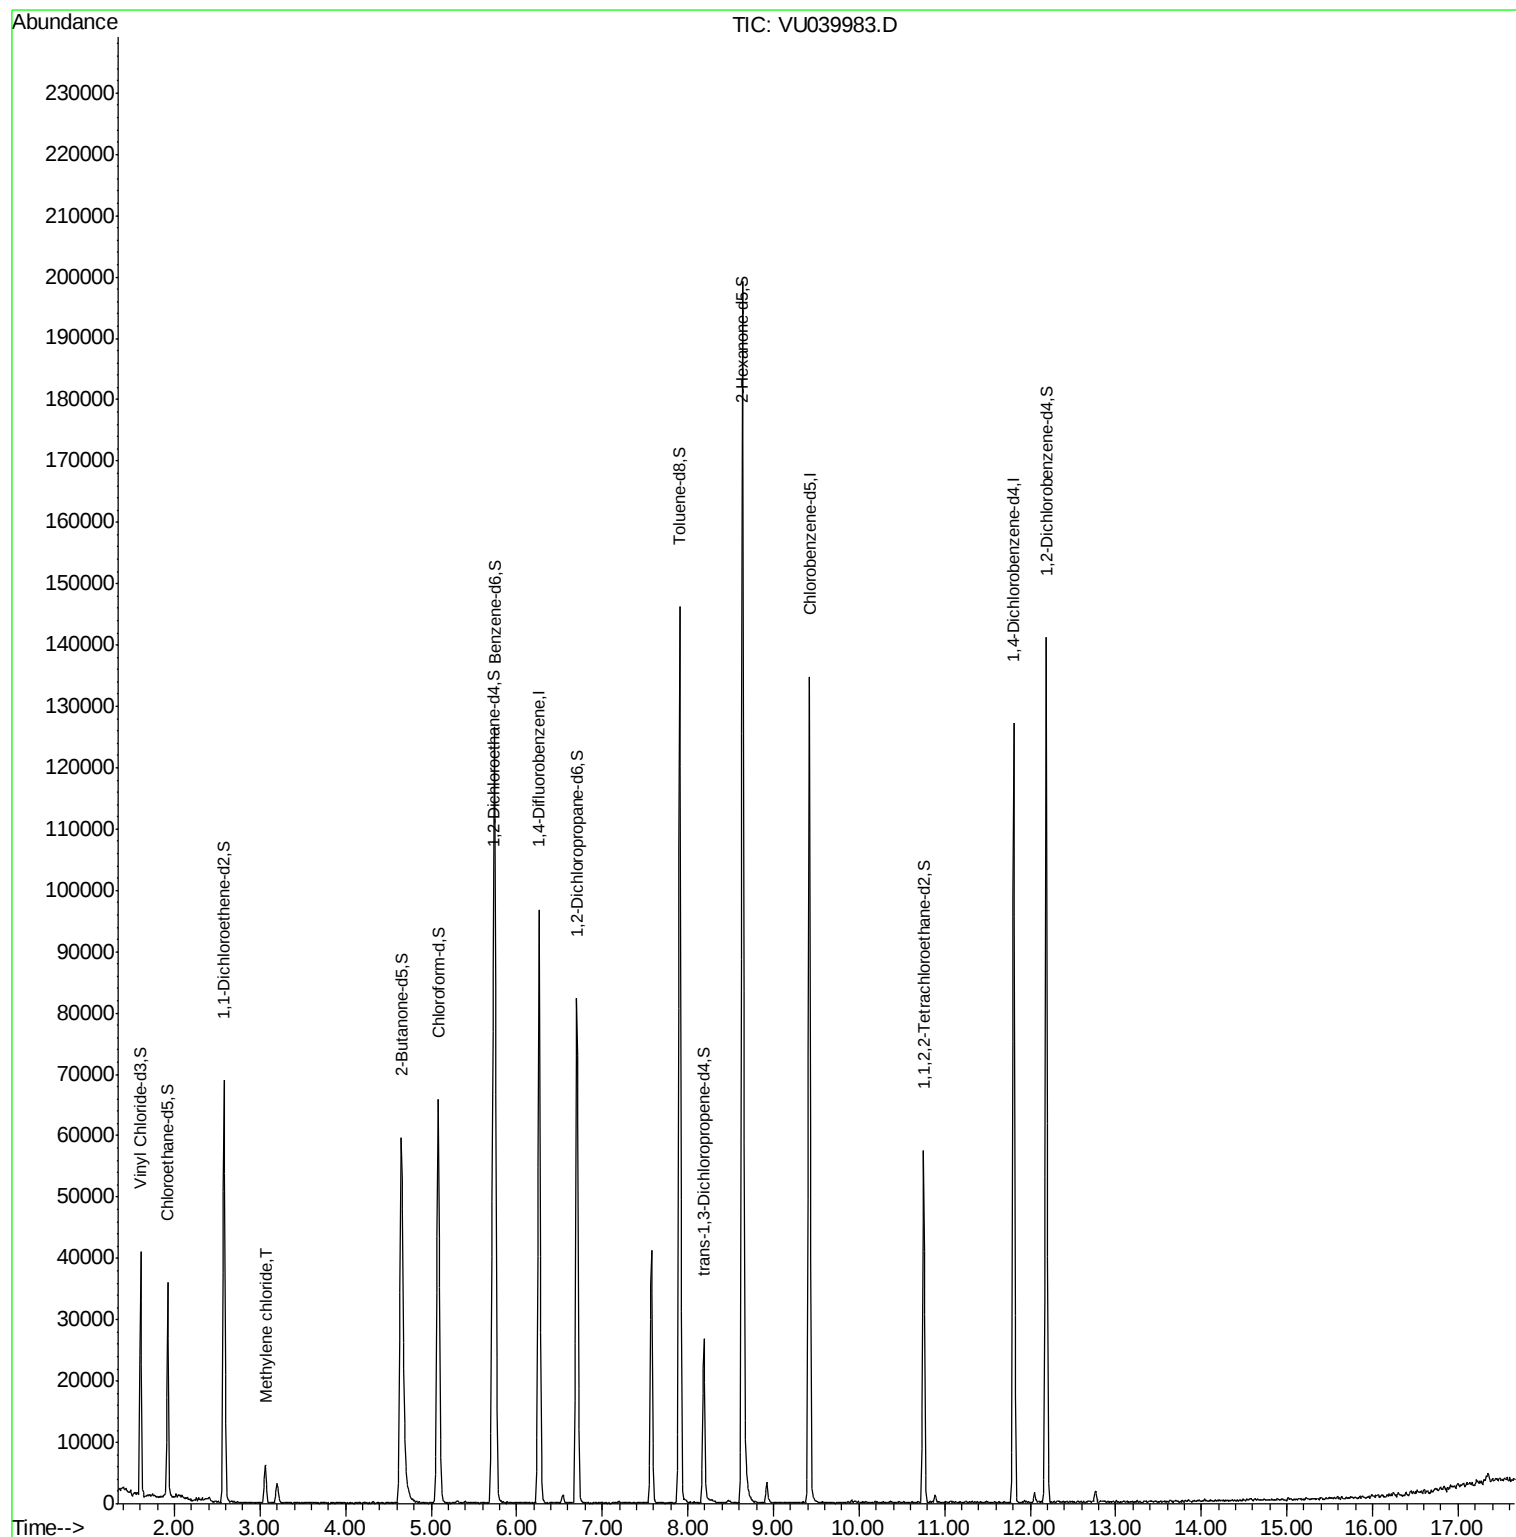

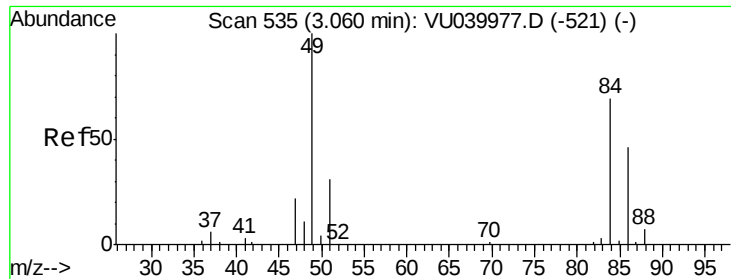

#16
 Methvlene chloride
 Concen: 0.282 ug/L
 RT: 3.06 min Scan# 535
 Delta R.T. 0.00 min
 Lab File: VU039983.D
 Acq: 26 Aug 2020 15:05

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Tot Ion: 84 Resp: 2408
 Ion Ratio Lower Upper
 84 100
 86 64.1 47.2 87.6
 49 137.5 99.8 185.4

