


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082620\
 Data File : VU039976.D
 Acq On : 26 Aug 2020 09:30
 Operator : SY/MD
 Sample : BFB22
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB22

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Aug 27 00:51:02 2020

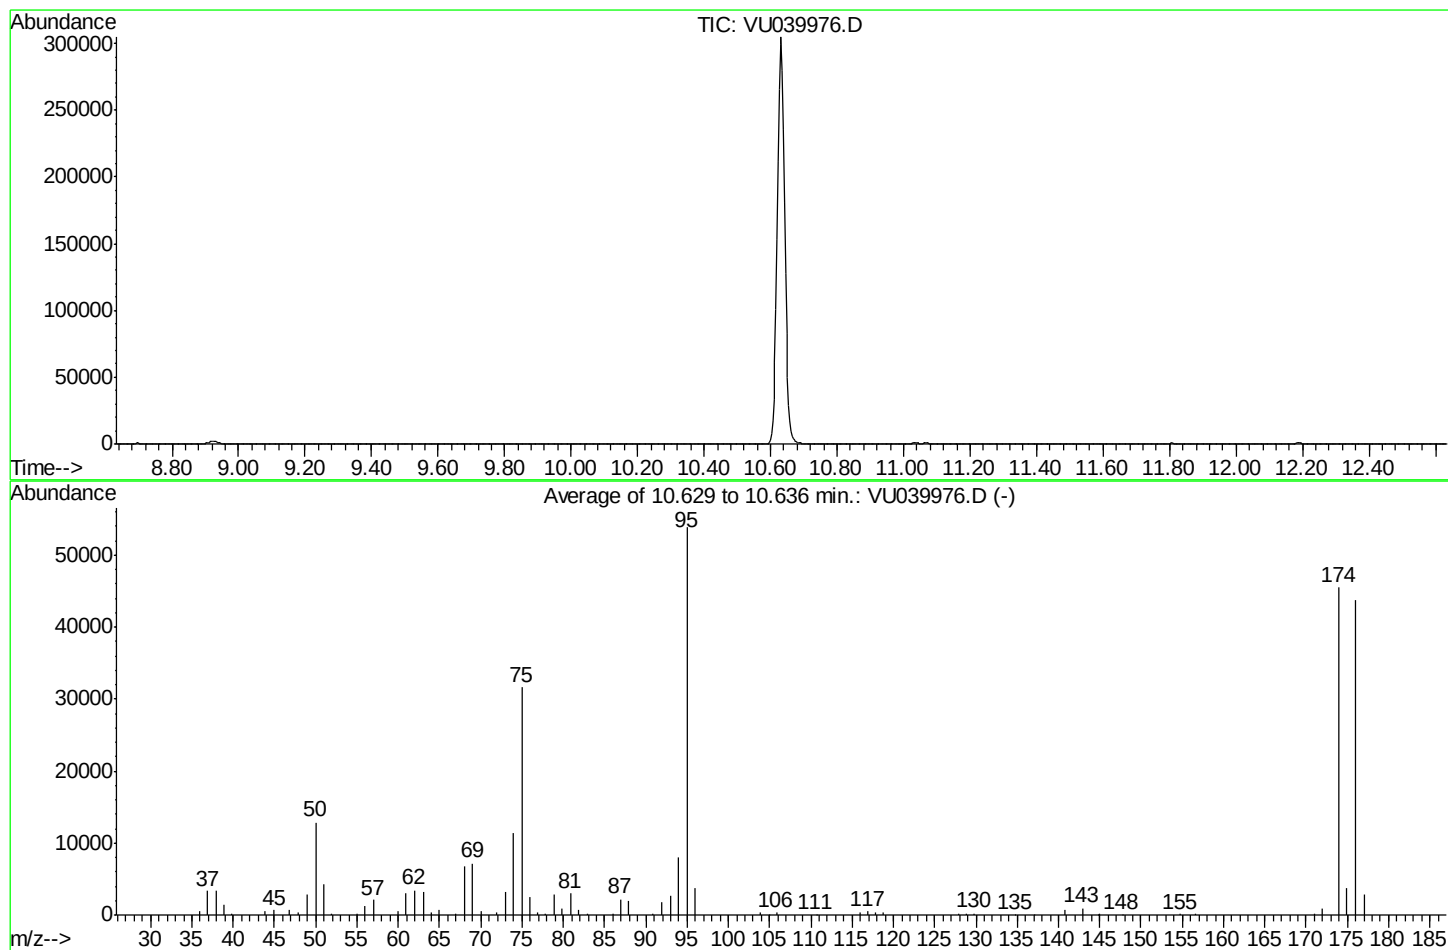

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	12851	PASS
75	95	30	80	58.7	31634	PASS
95	95	100	100	100.0	53864	PASS
96	95	5	9	6.8	3656	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.5	45514	PASS
175	174	5	9	8.1	3667	PASS
176	174	95	101	96.1	43722	PASS
177	176	5	9	6.5	2828	PASS

m/z	Abundance
35.90	548.0
36.90	3286.0
37.90	3545.0
38.90	1584.0
39.80	155.0
43.90	784.0
44.90	603.0
46.80	713.0
47.80	419.0
48.90	2980.0
50.00	13025.0
51.00	4370.0
51.90	167.0
55.00	271.0
55.90	1166.0
57.00	2245.0
59.90	553.0
60.90	3239.0
61.90	3500.0
63.00	3411.0
64.00	361.0
65.00	686.0
66.80	196.0
68.00	6965.0
69.00	7328.0
70.00	579.0
72.00	319.0
72.90	3369.0
74.00	11743.0
75.00	32600.0
76.00	2618.0
76.90	373.0
77.80	258.0
78.90	2999.0
79.80	1068.0
80.90	3081.0
81.90	796.0
82.90	136.0
85.90	168.0
86.90	2149.0
87.90	1866.0
90.80	271.0
91.90	1772.0
93.00	2737.0
94.00	8291.0
95.00	53984.0
96.00	3870.0
103.80	332.0
105.80	356.0
110.70	129.0
115.90	307.0
116.90	471.0
117.80	301.0
118.80	413.0
128.00	157.0
128.90	148.0
129.80	271.0
134.80	140.0
140.80	737.0
143.00	850.0
144.80	154.0
147.80	158.0
154.80	181.0
156.70	123.0
171.10	168.0
171.90	941.0
174.00	45144.0
174.90	3604.0
176.00	43728.0
177.00	2953.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
35.90	567.0
36.90	3408.0
37.90	3384.0
39.00	1465.0
39.80	157.0
43.90	742.0
44.90	668.0
46.90	715.0
47.80	379.0
48.90	3026.0
50.00	13261.0
51.00	4434.0
51.90	150.0
55.00	251.0
55.90	1243.0
57.00	2165.0
59.90	585.0
60.90	3132.0
61.90	3516.0
63.00	3467.0
63.90	374.0
65.00	657.0
66.90	197.0
68.00	6979.0
69.00	7408.0
70.00	621.0
72.00	342.0
73.00	3279.0
74.00	11735.0
75.00	32728.0
76.00	2659.0
76.90	348.0
77.80	240.0
78.80	2957.0
79.80	1019.0
80.90	3087.0
81.80	784.0
82.90	151.0
85.90	167.0
86.90	2320.0
87.90	1986.0
90.80	255.0
92.00	1838.0
92.90	2807.0
94.00	8339.0
95.00	55680.0
96.00	3802.0
103.90	314.0
105.00	105.0
105.80	368.0
110.60	106.0
115.90	322.0
116.90	509.0
117.80	301.0
118.80	463.0
127.90	164.0
128.90	138.0
129.80	266.0
134.80	103.0
140.80	778.0
142.90	908.0
145.00	151.0
147.70	127.0
154.80	148.0
156.60	140.0
171.10	167.0
171.90	909.0
174.00	47112.0
174.90	3806.0
176.00	45128.0
177.00	2903.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
35.90	531.0
36.90	3254.0
38.00	3012.0
39.00	1312.0
39.80	148.0
44.00	665.0
45.00	642.0
46.90	645.0
47.80	281.0
48.90	2760.0
50.00	12267.0
51.00	3912.0
51.90	131.0
54.90	189.0
55.90	1188.0
57.00	1919.0
60.00	575.0
60.90	2850.0
62.00	3229.0
63.00	2988.0
63.90	318.0
65.00	628.0
67.00	185.0
68.00	6211.0
69.00	6701.0
70.00	532.0
71.90	313.0
72.90	2892.0
74.00	10666.0
75.00	29576.0
76.00	2366.0
76.80	327.0
78.90	2636.0
79.80	841.0
80.90	2859.0
81.80	725.0
82.90	133.0
86.00	139.0
86.90	2138.0
87.80	1912.0
90.90	206.0
92.00	1703.0
92.90	2674.0
94.00	7568.0
95.00	51928.0
96.00	3298.0
103.90	284.0
105.80	340.0
115.90	284.0
116.90	464.0
117.70	238.0
118.80	423.0
127.90	164.0
128.90	104.0
129.80	252.0
137.00	119.0
140.80	777.0
142.90	925.0
144.90	149.0
154.70	106.0
156.70	110.0
171.00	140.0
171.90	773.0
174.00	44288.0
174.90	3593.0
176.00	42312.0
177.00	2630.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
43.90	178.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22