

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050458.D
 Acq On : 26 Aug 2022 15:37
 Operator : SY/MD
 Sample : N4322-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY176

Quant Time: Aug 27 02:47:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 27 02:44:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	317282	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	320367	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	113207	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	164718	43.906	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	87.820%	
7) Chloroethane-d5	1.899	69	134811	48.563	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	97.120%	
11) 1,1-Dichloroethene-d2	2.559	63	188688	35.589	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	71.180%	
21) 2-Butanone-d5	4.623	46	251724	102.510	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	102.510%	
24) Chloroform-d	5.063	84	275947	45.821	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.640%	
26) 1,2-Dichloroethane-d4	5.700	65	184202	49.214	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.420%	
32) Benzene-d6	5.726	84	566974	47.897	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.690	67	189849	48.412	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.820%	
41) Toluene-d8	7.899	98	457545	44.173	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.340%	
43) trans-1,3-Dichloroprop...	8.179	79	73768	45.096	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	90.200%	
47) 2-Hexanone-d5	8.636	63	142751	98.091	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	98.090%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	281211	46.493	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	92.980%	
66) 1,2-Dichlorobenzene-d4	12.195	152	145044	53.635	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	107.280%	
Target Compounds						
13) Acetone	2.629	43	3860	2.391	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050458.D
Acq On : 26 Aug 2022 15:37
Operator : SY/MD
Sample : N4322-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY176

Quant Time: Aug 27 02:47:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 27 02:44:18 2022
Response via : Initial Calibration

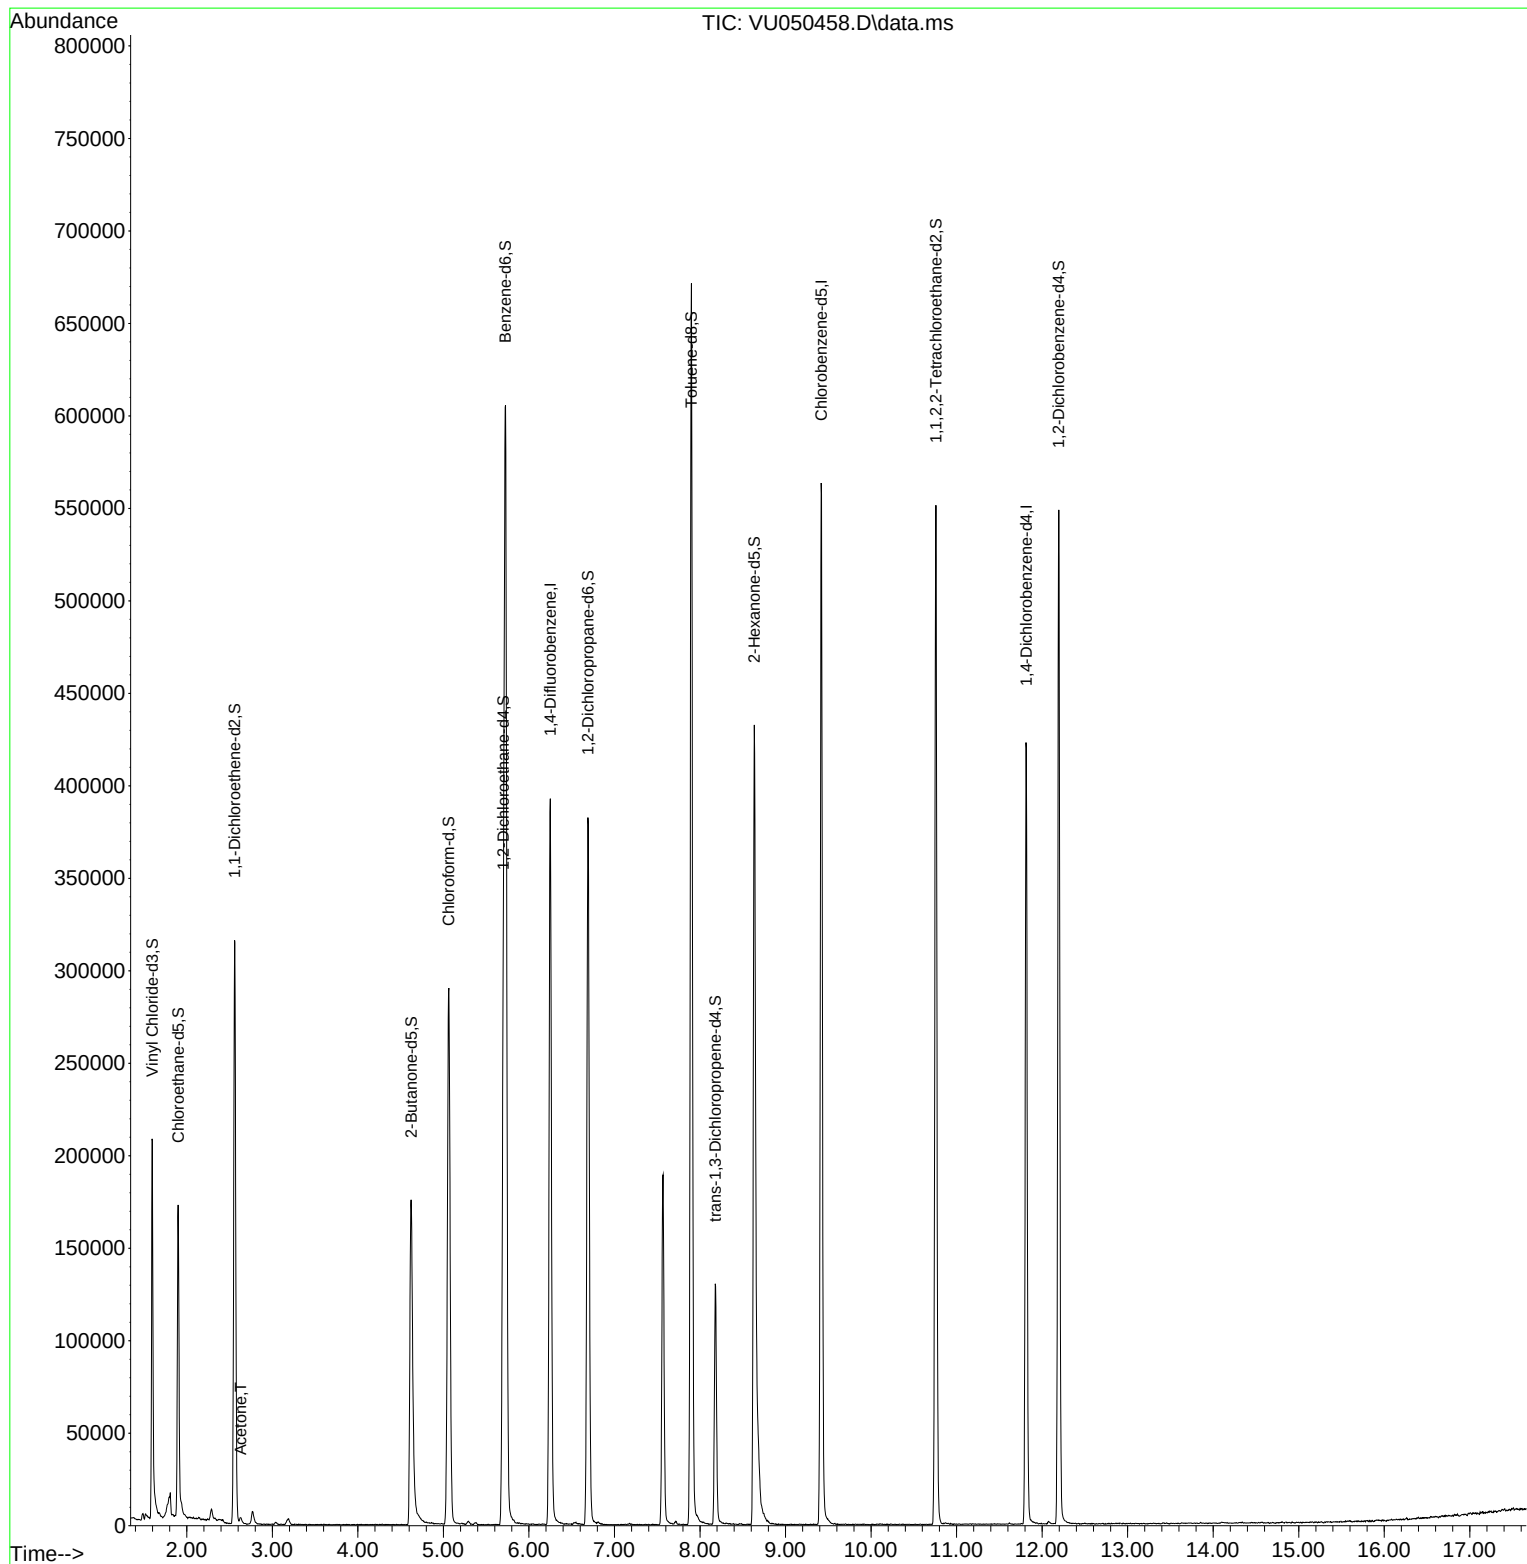

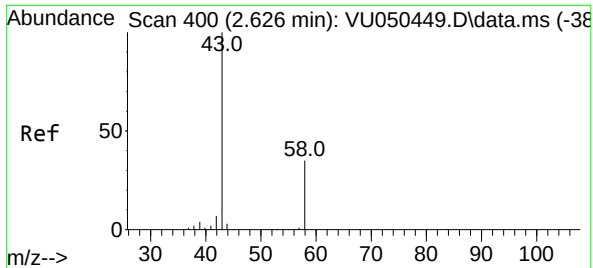

#13
 Acetone
 Concen: 2.391 ug/L
 RT: 2.629 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU050458.D
 Acq: 26 Aug 2022 15:37

Instrument :
 MSVOA_U
 ClientSampleId :
 EY176

Tgt Ion:	43	Resp:	3860
Ion	Ratio	Lower	Upper
43	100		
58	30.5	0.0	72.2

