

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050469.D
 Acq On : 26 Aug 2022 20:00
 Operator : SY/MD
 Sample : N4322-07ME
 Misc : 6.04g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY167ME

Quant Time: Aug 27 02:50:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 27 02:44:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	305185	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	298460	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	114959	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.591	65	52775	14.625	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	29.240%#	
7) Chloroethane-d5	1.877	69	22597	8.463	ug/L	-0.03
Spiked Amount	50.000	Range 70 - 130	Recovery	=	16.920%#	
11) 1,1-Dichloroethene-d2	2.517	63	110712	21.709	ug/L	-0.05
Spiked Amount	50.000	Range 60 - 125	Recovery	=	43.420%#	
21) 2-Butanone-d5	4.645	46	342291	144.917	ug/L	0.03
Spiked Amount	100.000	Range 40 - 130	Recovery	=	144.920%#	
24) Chloroform-d	5.060	84	242504	41.863	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.720%	
26) 1,2-Dichloroethane-d4	5.700	65	163997	45.552	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.100%	
32) Benzene-d6	5.719	84	390666	35.425	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	70.860%	
36) 1,2-Dichloropropane-d6	6.690	67	162581	44.502	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	89.000%	
41) Toluene-d8	7.896	98	262064	27.158	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	54.320%#	
43) trans-1,3-Dichloroprop...	8.182	79	54516	35.773	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	71.540%	
47) 2-Hexanone-d5	8.658	63	223607	164.930	ug/L	0.03
Spiked Amount	100.000	Range 45 - 130	Recovery	=	164.930%#	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	348795	61.899	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	123.800%#	
66) 1,2-Dichlorobenzene-d4	12.198	152	145215	52.880	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	105.760%	
Target Compounds						Qvalue
16) Methylene chloride	3.022	84	6110	2.342	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050469.D
Acq On : 26 Aug 2022 20:00
Operator : SY/MD
Sample : N4322-07ME
Misc : 6.04g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY167ME

Quant Time: Aug 27 02:50:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 27 02:44:18 2022
Response via : Initial Calibration

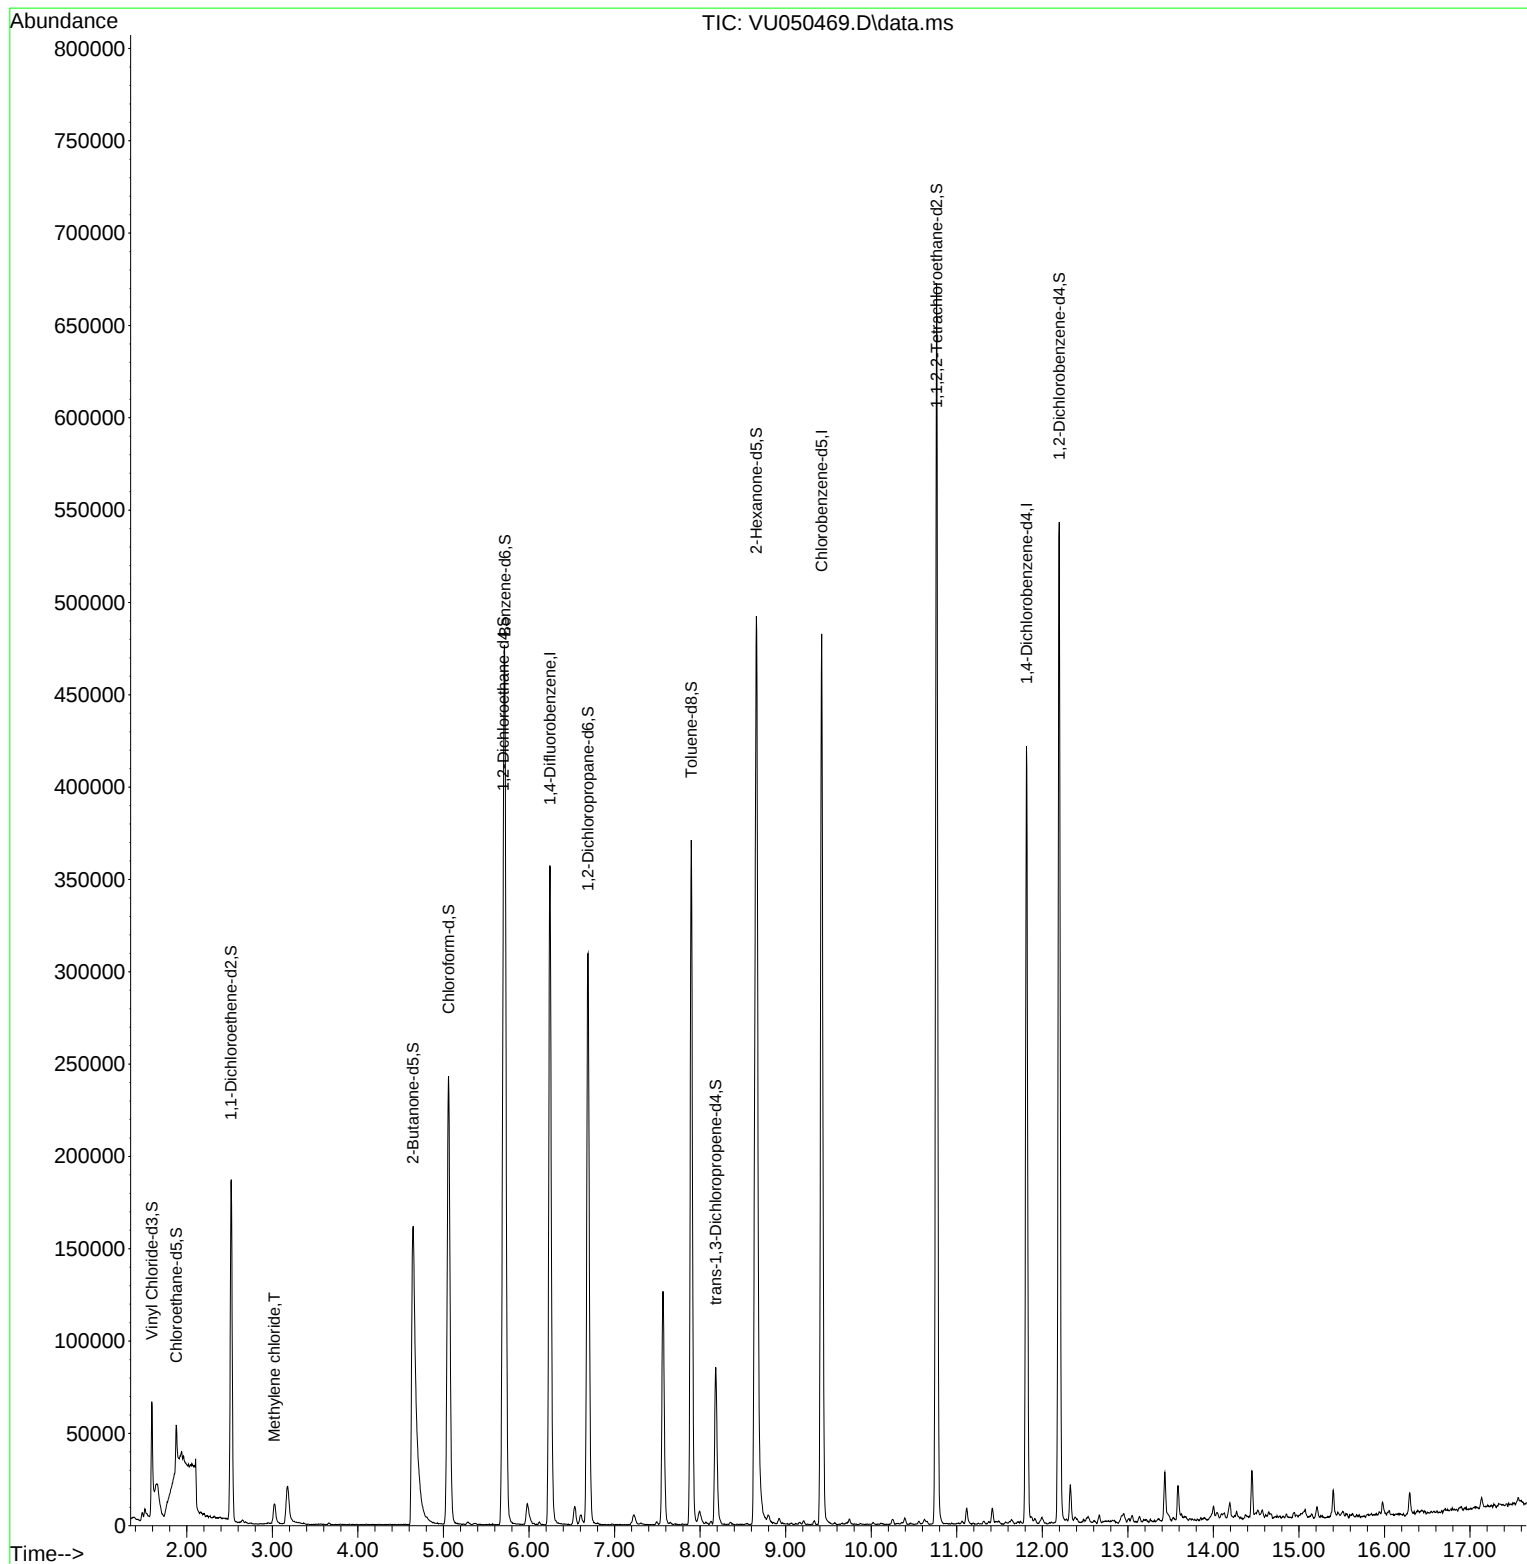

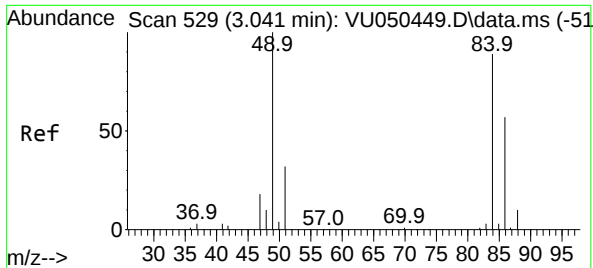

#16
Methylene chloride
Concen: 2.342 ug/L
RT: 3.022 min Scan# 51
Delta R.T. -0.019 min
Lab File: VU050469.D
Acq: 26 Aug 2022 20:00

Instrument :
MSVOA_U
ClientSampleId :
EY167ME

Tgt Ion:	84	Resp:	6110
Ion	Ratio	Lower	Upper
84	100		
86	59.5	43.9	81.5
49	121.7	80.4	149.4

