

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050450.D
 Acq On : 26 Aug 2022 12:06
 Operator : SY/MD
 Sample : VU0826MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	100	rBV	214314	250184	15.82%	2.286%
2	1.903	167	175	193	rVB	164757	223102	14.10%	2.038%
3	2.562	367	380	402	rBV	309101	500805	31.66%	4.576%
4	2.784	446	449	458	rVB3	989	1441	0.09%	0.013%
5	2.877	475	478	481	rBV2	363	312	0.02%	0.003%
6	3.041	520	529	541	rBV4	3326	6552	0.41%	0.060%
7	3.096	541	546	549	rBV3	274	257	0.02%	0.002%
8	3.131	555	557	559	rVB	266	98	0.01%	0.001%
9	3.182	561	573	590	rVB	6837	15335	0.97%	0.140%
10	3.247	590	593	599	rBV2	370	410	0.03%	0.004%
11	3.295	606	608	612	rVB2	196	125	0.01%	0.001%
12	3.324	615	617	621	rVB2	218	118	0.01%	0.001%
13	3.353	621	626	628	rBV3	466	363	0.02%	0.003%
14	3.475	661	664	670	rVB2	280	228	0.01%	0.002%
15	3.748	746	749	753	rBV2	215	178	0.01%	0.002%
16	3.829	770	774	775	rBV	153	108	0.01%	0.001%
17	3.854	780	782	787	rVB2	202	122	0.01%	0.001%
18	3.932	803	806	809	rBV2	226	160	0.01%	0.001%
19	4.005	827	829	832	rVB2	199	117	0.01%	0.001%
20	4.321	925	927	930	rBV2	253	142	0.01%	0.001%
21	4.333	930	931	935	rVV2	184	121	0.01%	0.001%
22	4.356	935	938	943	rVB2	254	230	0.01%	0.002%
23	4.385	943	947	950	rBV2	303	298	0.02%	0.003%
24	4.433	959	962	966	rVB2	264	210	0.01%	0.002%
25	4.485	975	978	981	rVB	370	277	0.02%	0.003%
26	4.517	981	988	990	rBV	319	436	0.03%	0.004%
27	4.623	1008	1021	1054	rBV	165997	423466	26.77%	3.869%
28	5.063	1141	1158	1188	rBV	279749	619091	39.14%	5.657%
29	5.292	1221	1229	1231	rBV2	1086	1500	0.09%	0.014%
30	5.356	1246	1249	1250	rBV	416	230	0.01%	0.002%
31	5.372	1250	1254	1255	rVV2	417	332	0.02%	0.003%
32	5.636	1328	1336	1341	rBV2	289	511	0.03%	0.005%
33	5.726	1341	1364	1400	rBV2	578955	1581765	100.00%	14.452%
34	6.250	1513	1527	1551	rBV	367121	705237	44.59%	6.444%
35	6.523	1608	1612	1614	rBV3	684	606	0.04%	0.006%
36	6.603	1634	1637	1639	rBV2	274	151	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050450.D
 Acq On : 26 Aug 2022 12:06
 Operator : SY/MD
 Sample : VU0826MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.639	1645	1648	1649	rBV2	206	116	0.01%	0.001%
38	6.690	1649	1664	1688	rBV	367475	721199	45.59%	6.589%
39	6.883	1722	1724	1727	rVB	234	138	0.01%	0.001%
40	6.912	1727	1733	1739	rBV3	245	334	0.02%	0.003%
41	6.970	1748	1751	1755	rBV2	219	169	0.01%	0.002%
42	7.144	1803	1805	1810	rVB2	187	107	0.01%	0.001%
43	7.173	1811	1814	1815	rBV	241	149	0.01%	0.001%
44	7.282	1844	1848	1855	rBV2	310	347	0.02%	0.003%
45	7.314	1856	1858	1862	rBV2	218	150	0.01%	0.001%
46	7.382	1877	1879	1885	rVB2	211	166	0.01%	0.002%
47	7.459	1900	1903	1907	rVB	153	120	0.01%	0.001%
48	7.565	1923	1936	1960	rBV	183196	325955	20.61%	2.978%
49	7.690	1971	1975	1977	rBV3	291	219	0.01%	0.002%
50	7.793	2001	2007	2015	rBV3	1118	1550	0.10%	0.014%
51	7.899	2025	2040	2064	rBV	647892	1138968	72.01%	10.407%
52	8.179	2116	2127	2150	rBV	126894	217779	13.77%	1.990%
53	8.388	2187	2192	2193	rBV	316	272	0.02%	0.002%
54	8.462	2213	2215	2221	rVB2	310	246	0.02%	0.002%
55	8.488	2221	2223	2226	rBV2	226	157	0.01%	0.001%
56	8.523	2232	2234	2236	rVB2	225	115	0.01%	0.001%
57	8.546	2238	2241	2242	rBV	195	111	0.01%	0.001%
58	8.636	2256	2269	2321	rBV2	386616	880627	55.67%	8.046%
59	8.973	2371	2374	2378	rVB	377	229	0.01%	0.002%
60	9.034	2389	2393	2394	rBV	322	246	0.02%	0.002%
61	9.105	2412	2415	2417	rBV2	231	147	0.01%	0.001%
62	9.156	2429	2431	2435	rVB	253	123	0.01%	0.001%
63	9.417	2499	2512	2531	rBV	534777	893999	56.52%	8.168%
64	9.610	2568	2572	2576	rBV3	388	364	0.02%	0.003%
65	9.825	2637	2639	2643	rVB2	294	183	0.01%	0.002%
66	9.951	2674	2678	2679	rBV	246	145	0.01%	0.001%
67	9.980	2684	2687	2689	rBV	208	132	0.01%	0.001%
68	10.105	2724	2726	2728	rBV3	440	277	0.02%	0.003%
69	10.250	2768	2771	2772	rBV	243	151	0.01%	0.001%
70	10.311	2784	2790	2794	rBV3	424	575	0.04%	0.005%
71	10.455	2833	2835	2838	rVB	254	130	0.01%	0.001%
72	10.491	2838	2846	2853	rBV3	677	902	0.06%	0.008%
73	10.700	2907	2911	2916	rBV	353	362	0.02%	0.003%
74	10.758	2916	2929	2953	rBV	518008	862086	54.50%	7.877%
75	10.915	2972	2978	2982	rBV	359	429	0.03%	0.004%
76	10.970	2993	2995	2998	rVB	347	171	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050450.D
 Acq On : 26 Aug 2022 12:06
 Operator : SY/MD
 Sample : VU0826MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.999	3001	3004	3006	rBV	313	226	0.01%	0.002%
78	11.089	3029	3032	3038	rVB4	583	626	0.04%	0.006%
79	11.394	3125	3127	3130	rVB3	196	110	0.01%	0.001%
80	11.442	3139	3142	3145	rBV	247	220	0.01%	0.002%
81	11.471	3146	3151	3157	rVB3	1156	1236	0.08%	0.011%
82	11.751	3231	3238	3244	rBV4	2209	2761	0.17%	0.025%
83	11.812	3244	3257	3279	rBV	394917	648094	40.97%	5.922%
84	11.970	3304	3306	3310	rVB2	482	340	0.02%	0.003%
85	12.089	3340	3343	3344	rBV	320	201	0.01%	0.002%
86	12.192	3362	3375	3399	rBV	517813	860441	54.40%	7.862%
87	12.359	3424	3427	3430	rBV3	372	246	0.02%	0.002%
88	12.526	3475	3479	3482	rBV3	585	453	0.03%	0.004%
89	12.565	3488	3491	3493	rBV2	471	329	0.02%	0.003%
90	12.606	3501	3504	3508	rBV2	287	275	0.02%	0.003%
91	12.729	3539	3542	3544	rBV2	423	258	0.02%	0.002%
92	12.979	3618	3620	3622	rBV	369	216	0.01%	0.002%
93	13.002	3625	3627	3632	rVB3	404	315	0.02%	0.003%
94	13.131	3664	3667	3672	rBV3	454	480	0.03%	0.004%
95	13.227	3688	3697	3709	rBV5	2615	4206	0.27%	0.038%
96	13.478	3772	3775	3778	rBV2	348	253	0.02%	0.002%
97	13.844	3880	3889	3900	rBV5	5105	8895	0.56%	0.081%
98	14.092	3957	3966	3979	rBV	11074	19346	1.22%	0.177%
99	14.330	4034	4040	4052	rVB7	6460	10510	0.66%	0.096%
100	15.336	4351	4353	4356	rBV3	556	387	0.02%	0.004%




Sum of corrected areas: 10944687

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050450.D
Acq On : 26 Aug 2022 12:06
Operator : SY/MD
Sample : VU0826MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

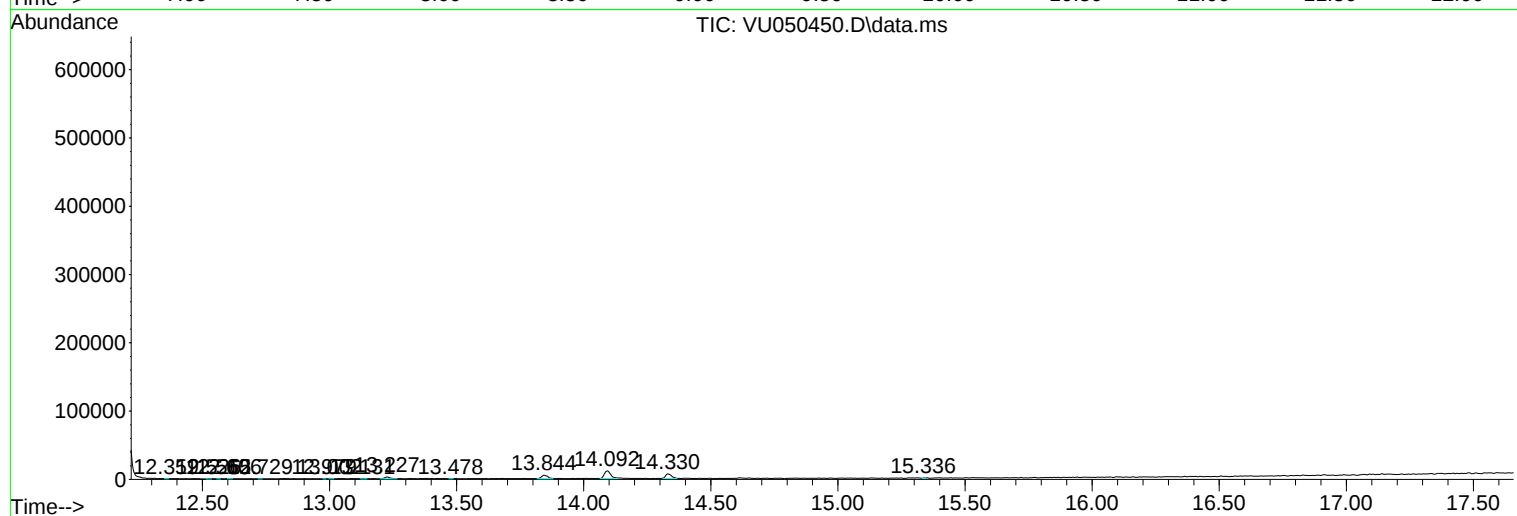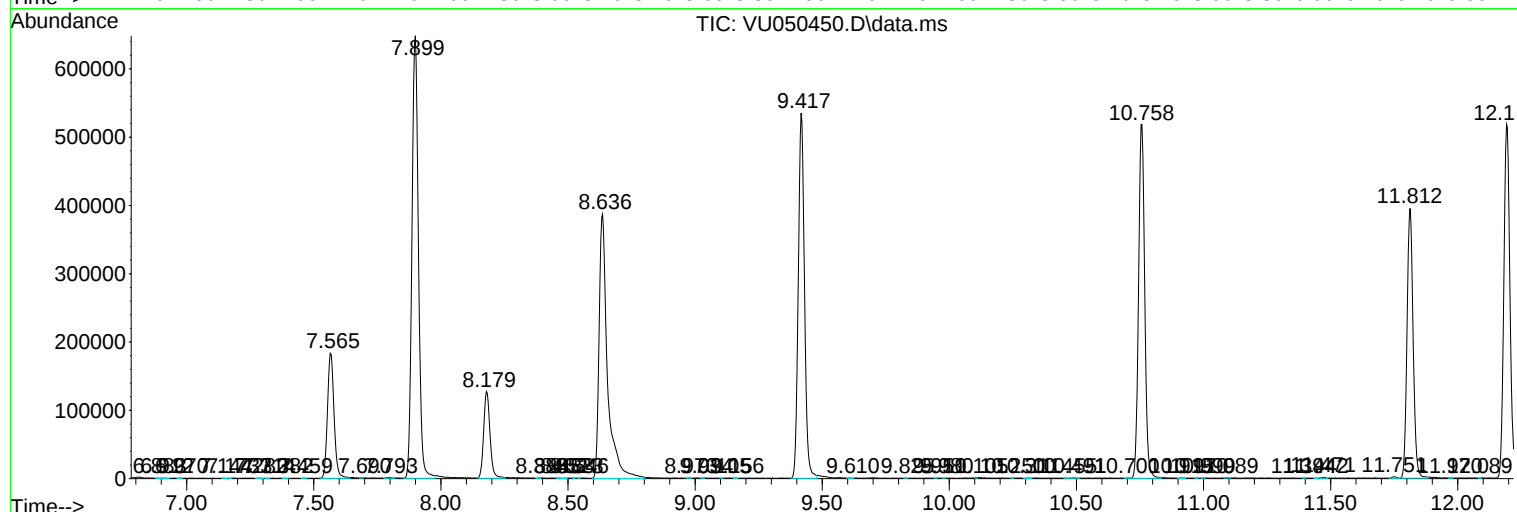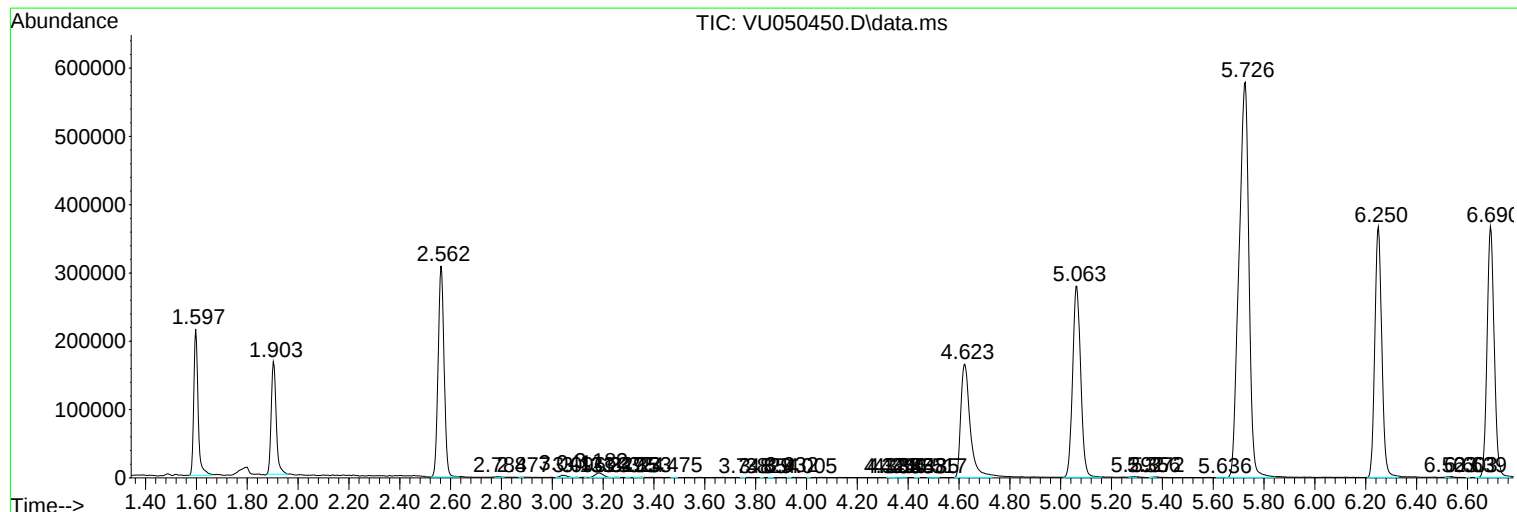

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050450.D
Acq On : 26 Aug 2022 12:06
Operator : SY/MD
Sample : VU0826MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050450.D
Acq On : 26 Aug 2022 12:06
Operator : SY/MD
Sample : VU0826MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc