

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050452.D
 Acq On : 26 Aug 2022 13:15
 Operator : SY/MD
 Sample : N4362-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	51	rVB3	4121	4364	0.28%	0.041%
2	1.517	51	55	59	rBV2	3204	3627	0.24%	0.034%
3	1.597	72	80	101	rBV	195018	233883	15.26%	2.215%
4	1.803	127	144	153	rBV5	11597	27989	1.83%	0.265%
5	1.899	166	174	200	rVB	160100	223242	14.56%	2.114%
6	2.562	367	380	393	rBV	289540	466316	30.42%	4.416%
7	2.626	395	400	412	rVB2	8248	13154	0.86%	0.125%
8	2.751	436	439	441	rBV2	562	421	0.03%	0.004%
9	2.851	465	470	472	rBV2	329	327	0.02%	0.003%
10	2.890	479	482	489	rVB2	327	352	0.02%	0.003%
11	2.941	495	498	500	rBV2	379	271	0.02%	0.003%
12	2.960	501	504	508	rVB	461	348	0.02%	0.003%
13	3.038	521	528	542	rVB6	1510	2785	0.18%	0.026%
14	3.185	560	574	591	rBV	11709	27190	1.77%	0.257%
15	3.285	601	605	606	rBV	270	179	0.01%	0.002%
16	3.555	684	689	693	rBV2	259	295	0.02%	0.003%
17	3.832	772	775	779	rBV	253	263	0.02%	0.002%
18	3.890	788	793	801	rVB	210	270	0.02%	0.003%
19	4.253	902	906	909	rVB	372	281	0.02%	0.003%
20	4.288	914	917	921	rVB	296	194	0.01%	0.002%
21	4.481	974	977	983	rVB2	278	279	0.02%	0.003%
22	4.623	1008	1021	1067	rBV	156918	402897	26.28%	3.815%
23	5.063	1140	1158	1178	rVV	274873	609766	39.77%	5.774%
24	5.295	1221	1230	1238	rVB4	1564	2645	0.17%	0.025%
25	5.333	1238	1242	1244	rBV2	294	194	0.01%	0.002%
26	5.446	1273	1277	1285	rVB2	283	371	0.02%	0.004%
27	5.494	1285	1292	1297	rVB2	249	266	0.02%	0.003%
28	5.726	1342	1364	1391	rBV2	567216	1533115	100.00%	14.518%
29	5.980	1440	1443	1448	rVB3	409	362	0.02%	0.003%
30	6.034	1458	1460	1465	rBV3	326	285	0.02%	0.003%
31	6.082	1468	1475	1477	rBV2	227	321	0.02%	0.003%
32	6.160	1496	1499	1502	rBV	405	294	0.02%	0.003%
33	6.250	1511	1527	1551	rBV	342629	660716	43.10%	6.257%
34	6.491	1599	1602	1604	rBV	261	190	0.01%	0.002%
35	6.526	1609	1613	1616	rBV2	466	482	0.03%	0.005%
36	6.690	1650	1664	1690	rBV	357881	707922	46.18%	6.704%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050452.D
 Acq On : 26 Aug 2022 13:15
 Operator : SY/MD
 Sample : N4362-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.841	1708	1711	1713	rBV2	379	284	0.02%	0.003%
38	6.873	1716	1721	1724	rBV2	378	335	0.02%	0.003%
39	6.983	1752	1755	1760	rVB2	197	183	0.01%	0.002%
40	7.053	1774	1777	1779	rBV2	311	210	0.01%	0.002%
41	7.070	1779	1782	1788	rVB2	257	230	0.02%	0.002%
42	7.105	1788	1793	1797	rBV2	270	237	0.02%	0.002%
43	7.176	1811	1815	1818	rBV2	464	341	0.02%	0.003%
44	7.430	1892	1894	1900	rVB2	300	228	0.01%	0.002%
45	7.568	1924	1937	1955	rBV	175156	312071	20.36%	2.955%
46	7.684	1970	1973	1975	rBV2	359	240	0.02%	0.002%
47	7.754	1992	1995	1997	rBV3	345	228	0.01%	0.002%
48	7.799	2003	2009	2015	rVB3	919	1062	0.07%	0.010%
49	7.835	2015	2020	2023	rBV2	253	277	0.02%	0.003%
50	7.899	2026	2040	2072	rBV	623537	1095883	71.48%	10.378%
51	8.179	2115	2127	2149	rBV	118303	202381	13.20%	1.916%
52	8.471	2211	2218	2226	rVB4	2332	3048	0.20%	0.029%
53	8.635	2256	2269	2310	rBV2	388840	833443	54.36%	7.892%
54	8.896	2348	2350	2353	rVB	594	341	0.02%	0.003%
55	8.922	2353	2358	2359	rBV	392	314	0.02%	0.003%
56	8.934	2359	2362	2364	rBV	289	174	0.01%	0.002%
57	9.024	2386	2390	2393	rBV2	240	193	0.01%	0.002%
58	9.185	2435	2440	2443	rBV3	323	337	0.02%	0.003%
59	9.230	2448	2454	2458	rBV2	199	236	0.02%	0.002%
60	9.282	2465	2470	2473	rBV2	192	213	0.01%	0.002%
61	9.362	2491	2495	2499	rBV2	390	330	0.02%	0.003%
62	9.417	2499	2512	2536	rBV	503812	843948	55.05%	7.992%
63	9.568	2557	2559	2566	rVB3	434	379	0.02%	0.004%
64	9.658	2583	2587	2590	rBV2	309	224	0.01%	0.002%
65	9.832	2637	2641	2645	rBV	176	189	0.01%	0.002%
66	10.063	2710	2713	2718	rVB2	235	205	0.01%	0.002%
67	10.092	2719	2722	2725	rBV	338	259	0.02%	0.002%
68	10.121	2728	2731	2735	rBV2	382	332	0.02%	0.003%
69	10.182	2746	2750	2753	rBV2	311	254	0.02%	0.002%
70	10.246	2757	2770	2776	rBV3	831	1451	0.09%	0.014%
71	10.484	2841	2844	2853	rVB2	369	436	0.03%	0.004%
72	10.558	2862	2867	2869	rBV2	364	284	0.02%	0.003%
73	10.577	2869	2873	2874	rBV2	285	224	0.01%	0.002%
74	10.758	2915	2929	2951	rVV	505714	837500	54.63%	7.931%
75	10.893	2963	2971	2980	rVB4	2660	4338	0.28%	0.041%
76	11.057	3015	3022	3025	rBV2	188	270	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050452.D
 Acq On : 26 Aug 2022 13:15
 Operator : SY/MD
 Sample : N4362-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.121	3036	3042	3048	rVB5	366	469	0.03%	0.004%
78	11.381	3120	3123	3126	rBV2	200	173	0.01%	0.002%
79	11.487	3152	3156	3164	rVB3	471	479	0.03%	0.005%
80	11.577	3180	3184	3190	rVB2	339	332	0.02%	0.003%
81	11.745	3232	3236	3237	rBV2	508	364	0.02%	0.003%
82	11.812	3245	3257	3278	rBV	384147	620338	40.46%	5.874%
83	11.957	3299	3302	3307	rVB2	639	469	0.03%	0.004%
84	12.069	3329	3337	3353	rVB6	3951	7951	0.52%	0.075%
85	12.192	3363	3375	3398	rBV	513612	851754	55.56%	8.066%
86	12.426	3446	3448	3452	rBV2	341	239	0.02%	0.002%
87	12.539	3481	3483	3487	rVB2	349	254	0.02%	0.002%
88	12.658	3517	3520	3522	rBV2	481	285	0.02%	0.003%
89	12.770	3547	3555	3556	rBV5	982	988	0.06%	0.009%
90	12.831	3571	3574	3578	rVB	324	227	0.01%	0.002%
91	12.954	3606	3612	3614	rBV2	492	427	0.03%	0.004%
92	13.220	3690	3695	3699	rBV5	764	914	0.06%	0.009%
93	13.317	3723	3725	3728	rVB2	377	218	0.01%	0.002%
94	13.500	3778	3782	3784	rBV	457	345	0.02%	0.003%
95	13.571	3801	3804	3806	rBV2	311	194	0.01%	0.002%
96	13.735	3852	3855	3857	rBV2	421	286	0.02%	0.003%
97	13.835	3883	3886	3887	rBV2	517	263	0.02%	0.002%
98	13.851	3888	3891	3893	rVV2	764	530	0.03%	0.005%
99	14.101	3960	3969	3977	rBV5	1793	3169	0.21%	0.030%
100	15.044	4260	4262	4265	rBV3	469	321	0.02%	0.003%




Sum of corrected areas: 10559957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050452.D
Acq On : 26 Aug 2022 13:15
Operator : SY/MD
Sample : N4362-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

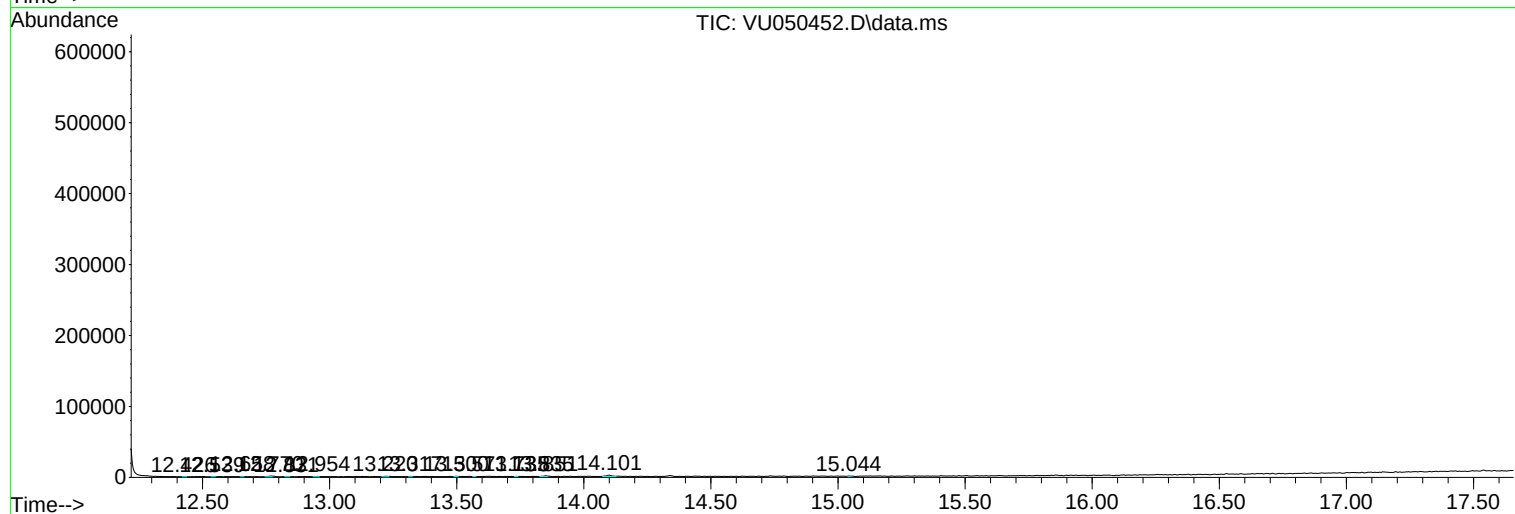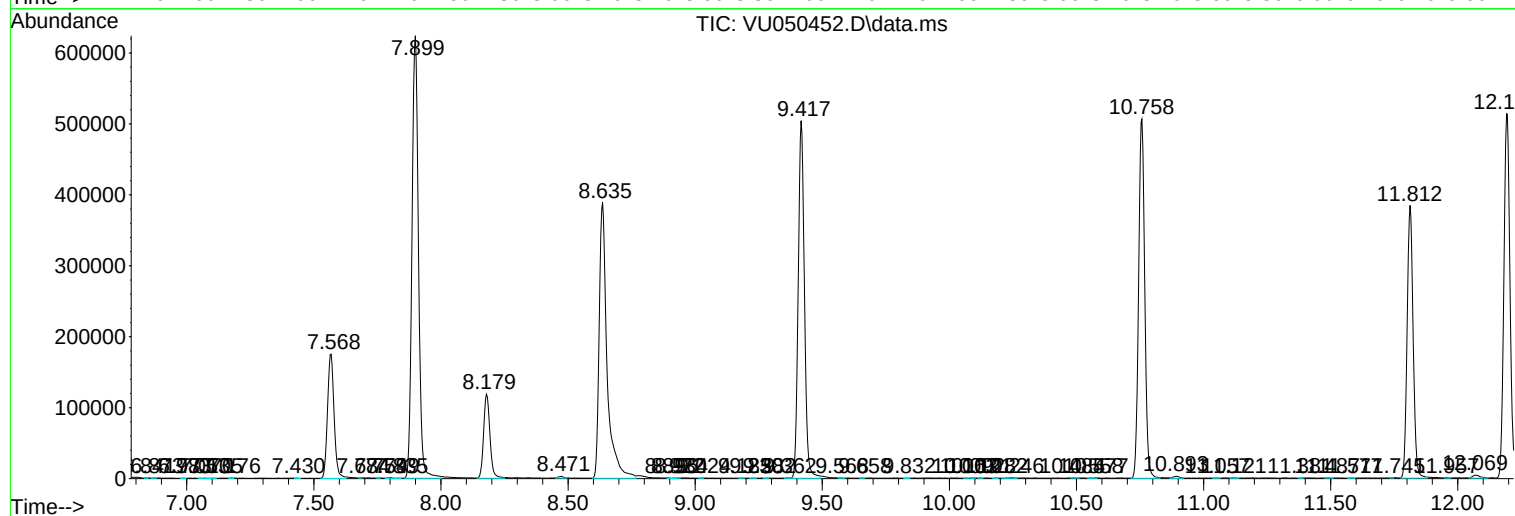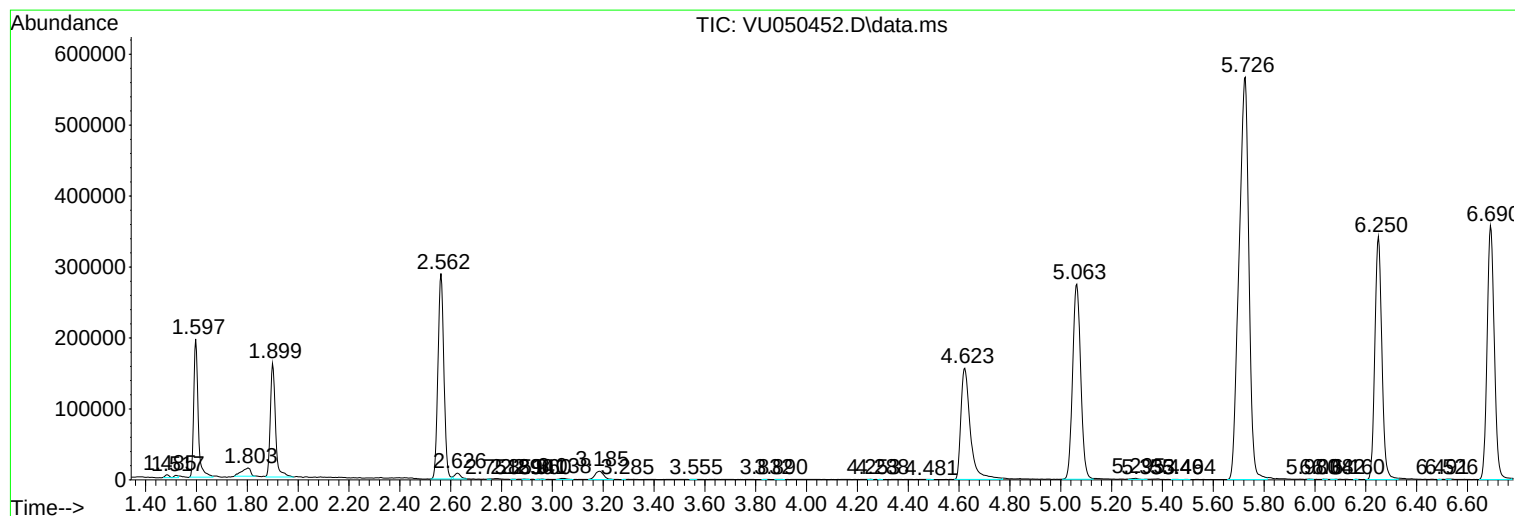

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050452.D
Acq On : 26 Aug 2022 13:15
Operator : SY/MD
Sample : N4362-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050452.D
Acq On : 26 Aug 2022 13:15
Operator : SY/MD
Sample : N4362-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc