

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050453.D
 Acq On : 26 Aug 2022 13:38
 Operator : SY/MD
 Sample : N4362-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	51	rVB3	2744	2630	0.16%	0.024%
2	1.517	52	55	58	rBV	1777	1485	0.09%	0.013%
3	1.597	72	80	103	rBV	217222	261904	16.37%	2.364%
4	1.899	166	174	195	rBV	169732	231736	14.48%	2.092%
5	2.324	302	306	308	rBV3	1257	1041	0.07%	0.009%
6	2.562	367	380	398	rBV	326444	523319	32.70%	4.724%
7	2.678	414	416	419	rVB2	421	251	0.02%	0.002%
8	2.723	428	430	433	rVB2	391	210	0.01%	0.002%
9	2.893	479	483	487	rBV4	359	304	0.02%	0.003%
10	3.041	520	529	539	rVV3	3912	6915	0.43%	0.062%
11	3.118	548	553	556	rBV	339	286	0.02%	0.003%
12	3.182	561	573	590	rBV	6499	13785	0.86%	0.124%
13	3.417	643	646	650	rVB	431	286	0.02%	0.003%
14	3.446	650	655	658	rBV2	205	169	0.01%	0.002%
15	3.800	759	765	772	rVB2	189	258	0.02%	0.002%
16	3.915	796	801	805	rBV2	275	268	0.02%	0.002%
17	3.957	811	814	817	rVB	254	177	0.01%	0.002%
18	4.115	859	863	870	rVB2	167	181	0.01%	0.002%
19	4.157	870	876	879	rBV2	278	240	0.01%	0.002%
20	4.259	903	908	910	rBV2	239	226	0.01%	0.002%
21	4.356	935	938	946	rBV	274	249	0.02%	0.002%
22	4.475	972	975	979	rBV	218	169	0.01%	0.002%
23	4.542	990	996	1000	rVB2	193	207	0.01%	0.002%
24	4.620	1008	1020	1047	rBV	168931	417878	26.11%	3.772%
25	4.845	1087	1090	1097	rVB4	467	444	0.03%	0.004%
26	5.063	1141	1158	1181	rBV	284853	628147	39.26%	5.670%
27	5.295	1220	1230	1235	rBV3	1630	2319	0.14%	0.021%
28	5.369	1245	1253	1254	rBV2	499	526	0.03%	0.005%
29	5.465	1279	1283	1289	rVV2	221	212	0.01%	0.002%
30	5.726	1341	1364	1392	rBV2	593032	1600161	100.00%	14.444%
31	5.874	1408	1410	1412	rBV	411	176	0.01%	0.002%
32	5.976	1439	1442	1444	rBV2	424	244	0.02%	0.002%
33	6.118	1481	1486	1491	rVB2	443	404	0.03%	0.004%
34	6.150	1491	1496	1501	rBV2	306	381	0.02%	0.003%
35	6.250	1511	1527	1555	rBV	370939	724720	45.29%	6.542%
36	6.517	1607	1610	1611	rBV	725	367	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050453.D
 Acq On : 26 Aug 2022 13:38
 Operator : SY/MD
 Sample : N4362-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.533	1611	1615	1619	rVV4	1129	1038	0.06%	0.009%
38	6.690	1649	1664	1690	rBV	369802	726288	45.39%	6.556%
39	6.806	1697	1700	1711	rVB4	1122	1550	0.10%	0.014%
40	6.877	1719	1722	1726	rVB3	366	297	0.02%	0.003%
41	7.063	1778	1780	1783	rVV	243	178	0.01%	0.002%
42	7.089	1786	1788	1794	rVV2	288	241	0.02%	0.002%
43	7.179	1812	1816	1820	rBV2	283	235	0.01%	0.002%
44	7.417	1887	1890	1895	rBV2	182	176	0.01%	0.002%
45	7.500	1912	1916	1920	rVB	382	297	0.02%	0.003%
46	7.565	1924	1936	1957	rBV	178334	318080	19.88%	2.871%
47	7.729	1982	1987	1990	rVB2	354	309	0.02%	0.003%
48	7.764	1993	1998	1999	rBV2	598	407	0.03%	0.004%
49	7.899	2026	2040	2062	rBV	661955	1153481	72.09%	10.412%
50	8.179	2115	2127	2148	rVV	125001	212225	13.26%	1.916%
51	8.388	2189	2192	2196	rBV3	231	219	0.01%	0.002%
52	8.433	2204	2206	2209	rBV	385	223	0.01%	0.002%
53	8.462	2213	2215	2218	rVB2	365	164	0.01%	0.001%
54	8.484	2219	2222	2228	rBV	338	273	0.02%	0.002%
55	8.517	2228	2232	2235	rBV3	272	246	0.02%	0.002%
56	8.635	2256	2269	2322	rBV3	404925	883899	55.24%	7.979%
57	8.851	2334	2336	2338	rBV2	372	205	0.01%	0.002%
58	8.877	2342	2344	2350	rVB3	333	260	0.02%	0.002%
59	8.960	2368	2370	2374	rVB	374	235	0.01%	0.002%
60	9.063	2399	2402	2407	rVB	395	332	0.02%	0.003%
61	9.092	2407	2411	2416	rBV2	169	176	0.01%	0.002%
62	9.150	2421	2429	2431	rBV2	310	373	0.02%	0.003%
63	9.317	2476	2481	2485	rBV2	161	207	0.01%	0.002%
64	9.417	2498	2512	2550	rBV	539025	917180	57.32%	8.279%
65	9.561	2555	2557	2560	rBV	341	248	0.02%	0.002%
66	9.693	2594	2598	2602	rBV2	249	253	0.02%	0.002%
67	9.973	2678	2685	2689	rBV2	300	387	0.02%	0.003%
68	9.999	2690	2693	2694	rVV	344	179	0.01%	0.002%
69	10.070	2711	2715	2717	rBV	314	239	0.01%	0.002%
70	10.143	2733	2738	2742	rVB2	249	248	0.02%	0.002%
71	10.758	2914	2929	2950	rBV	539057	873707	54.60%	7.887%
72	10.860	2957	2961	2962	rBV2	376	201	0.01%	0.002%
73	11.108	3034	3038	3043	rBV	279	342	0.02%	0.003%
74	11.266	3084	3087	3094	rBV	586	582	0.04%	0.005%
75	11.298	3094	3097	3100	rBV	241	166	0.01%	0.001%
76	11.423	3133	3136	3139	rVB2	329	201	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050453.D
 Acq On : 26 Aug 2022 13:38
 Operator : SY/MD
 Sample : N4362-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.475	3148	3152	3157	rBV2	402	468	0.03%	0.004%
78	11.616	3192	3196	3200	rBV	454	404	0.03%	0.004%
79	11.713	3218	3226	3228	rBV2	250	366	0.02%	0.003%
80	11.745	3234	3236	3242	rBV3	263	271	0.02%	0.002%
81	11.812	3244	3257	3281	rBV	412300	666410	41.65%	6.015%
82	12.034	3324	3326	3330	rVB2	346	220	0.01%	0.002%
83	12.066	3331	3336	3339	rBV5	547	571	0.04%	0.005%
84	12.108	3346	3349	3351	rBV2	383	193	0.01%	0.002%
85	12.121	3351	3353	3356	rBV	255	173	0.01%	0.002%
86	12.195	3362	3376	3400	rBV	536792	887005	55.43%	8.007%
87	12.729	3540	3542	3547	rVB3	479	395	0.02%	0.004%
88	12.931	3602	3605	3609	rVB4	401	289	0.02%	0.003%
89	13.153	3671	3674	3675	rBV	352	166	0.01%	0.001%
90	13.188	3682	3685	3688	rBV3	507	399	0.02%	0.004%
91	13.227	3694	3697	3700	rBV3	436	228	0.01%	0.002%
92	13.243	3700	3702	3704	rBV2	318	205	0.01%	0.002%
93	13.317	3721	3725	3727	rBV2	317	253	0.02%	0.002%
94	13.378	3742	3744	3746	rBV2	322	208	0.01%	0.002%
95	13.593	3807	3811	3815	rBV2	566	579	0.04%	0.005%
96	14.092	3964	3966	3967	rBV	553	228	0.01%	0.002%
97	14.134	3976	3979	3982	rBV2	424	328	0.02%	0.003%
98	14.327	4036	4039	4040	rBV2	654	413	0.03%	0.004%
99	14.870	4205	4208	4210	rBV	397	262	0.02%	0.002%
100	15.413	4374	4377	4379	rBV2	674	450	0.03%	0.004%




Sum of corrected areas: 11078306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050453.D
Acq On : 26 Aug 2022 13:38
Operator : SY/MD
Sample : N4362-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

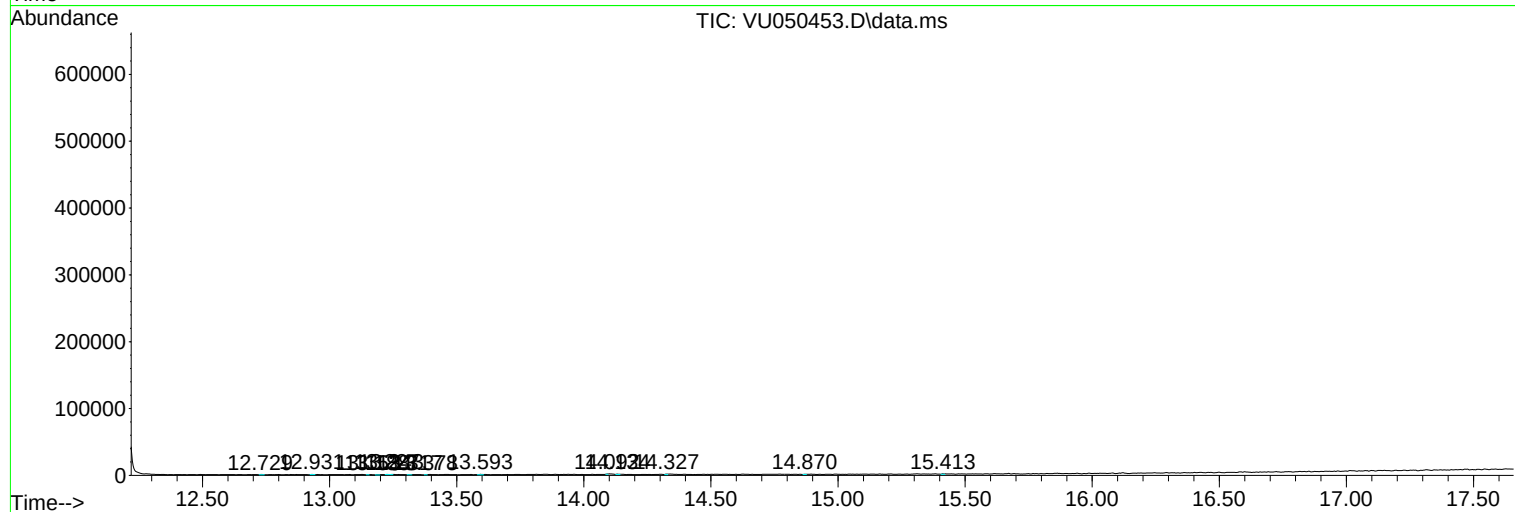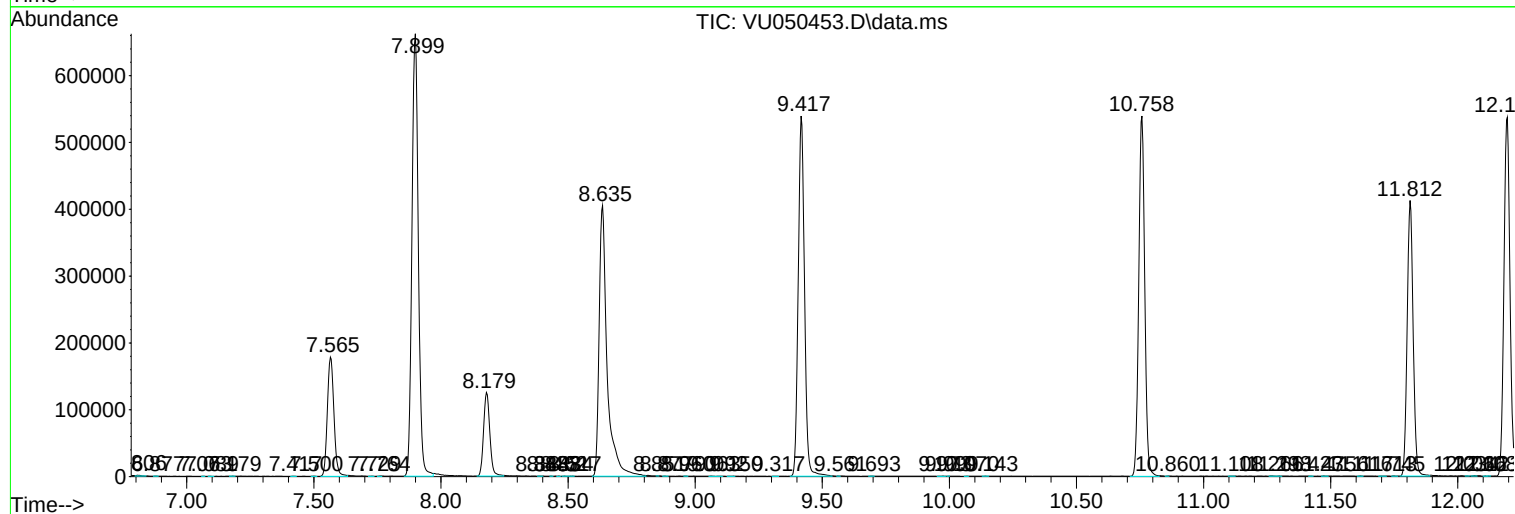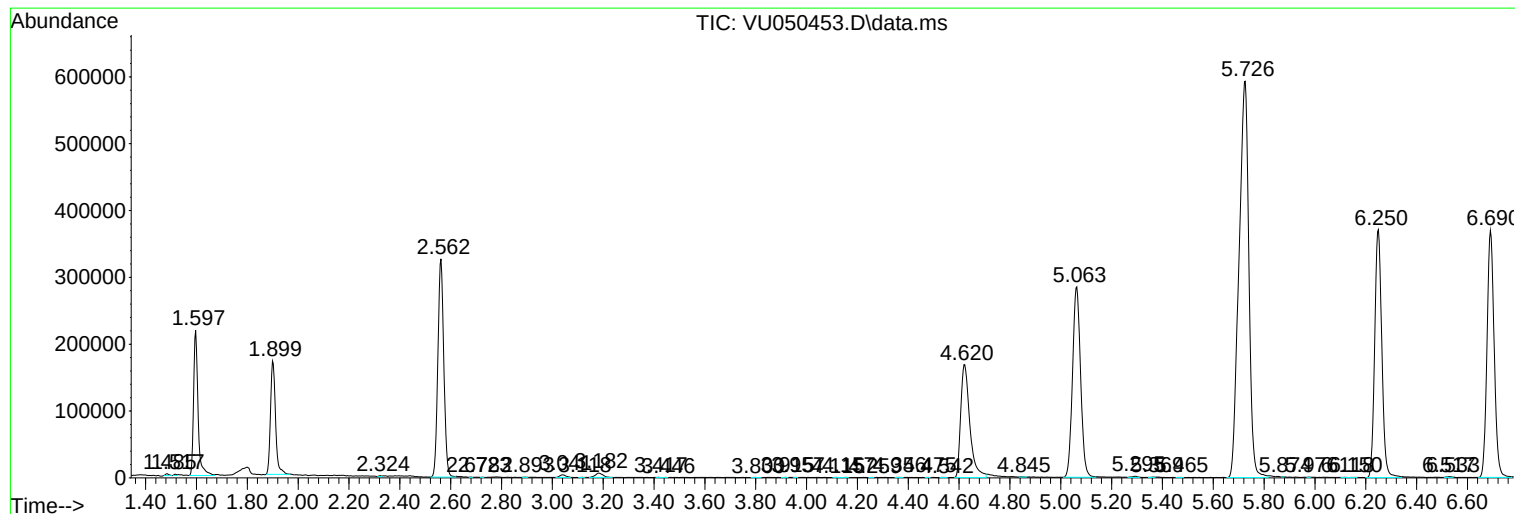

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050453.D
Acq On : 26 Aug 2022 13:38
Operator : SY/MD
Sample : N4362-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050453.D
Acq On : 26 Aug 2022 13:38
Operator : SY/MD
Sample : N4362-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
