

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050456.D
 Acq On : 26 Aug 2022 14:50
 Operator : SY/MD
 Sample : N4365-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	51	rBV3	3981	5178	0.41%	0.052%
2	1.520	51	56	60	rBV2	2701	2881	0.23%	0.029%
3	1.597	73	80	103	rBV	140497	169202	13.46%	1.684%
4	1.800	125	143	150	rBV5	12050	31183	2.48%	0.310%
5	1.900	166	174	204	rVB	128007	183593	14.61%	1.828%
6	2.562	368	380	394	rBV	195052	315516	25.10%	3.141%
7	2.764	432	443	456	rBV3	3454	7765	0.62%	0.077%
8	2.864	468	474	478	rBV2	375	341	0.03%	0.003%
9	2.954	498	502	505	rBV2	447	464	0.04%	0.005%
10	3.047	523	531	537	rVB4	1059	1701	0.14%	0.017%
11	3.083	540	542	548	rVB2	259	204	0.02%	0.002%
12	3.125	550	555	560	rBV	220	189	0.02%	0.002%
13	3.182	560	573	591	rVB	11510	25716	2.05%	0.256%
14	3.269	598	600	605	rVB3	342	290	0.02%	0.003%
15	3.305	605	611	613	rBV2	230	232	0.02%	0.002%
16	3.433	645	651	652	rBV	178	169	0.01%	0.002%
17	3.494	666	670	677	rVB3	207	228	0.02%	0.002%
18	3.549	683	687	689	rBV	237	185	0.01%	0.002%
19	3.584	694	698	701	rVB2	293	180	0.01%	0.002%
20	3.639	710	715	717	rBV2	258	180	0.01%	0.002%
21	3.662	717	722	729	rBV3	260	240	0.02%	0.002%
22	3.697	731	733	738	rVB	315	182	0.01%	0.002%
23	3.732	738	744	747	rBV	227	203	0.02%	0.002%
24	3.806	764	767	770	rVB	283	184	0.01%	0.002%
25	3.883	784	791	796	rVB	271	295	0.02%	0.003%
26	3.983	814	822	828	rBV2	339	512	0.04%	0.005%
27	4.147	868	873	876	rVV2	203	220	0.02%	0.002%
28	4.208	887	892	893	rBV	256	174	0.01%	0.002%
29	4.218	893	895	901	rVB2	273	260	0.02%	0.003%
30	4.266	904	910	913	rBV2	181	176	0.01%	0.002%
31	4.379	940	945	947	rBV	482	394	0.03%	0.004%
32	4.623	1008	1021	1047	rBV	209681	520309	41.40%	5.179%
33	5.060	1141	1157	1176	rBV	262578	573902	45.66%	5.713%
34	5.285	1218	1227	1228	rBV3	1287	1332	0.11%	0.013%
35	5.366	1248	1252	1254	rBV	868	782	0.06%	0.008%
36	5.581	1315	1319	1321	rBV2	228	169	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050456.D
 Acq On : 26 Aug 2022 14:50
 Operator : SY/MD
 Sample : N4365-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	5.723	1343	1363	1393	rBV2	442084	1256847	100.00%	12.511%
38	5.973	1437	1441	1446	rVB3	365	350	0.03%	0.003%
39	6.038	1455	1461	1463	rBV2	327	292	0.02%	0.003%
40	6.121	1481	1487	1489	rBV	384	338	0.03%	0.003%
41	6.250	1512	1527	1553	rBV	388263	742440	59.07%	7.391%
42	6.526	1609	1613	1617	rVV4	543	633	0.05%	0.006%
43	6.594	1630	1634	1639	rVB3	467	506	0.04%	0.005%
44	6.690	1649	1664	1691	rBV	321201	633101	50.37%	6.302%
45	6.845	1710	1712	1715	rVB	575	235	0.02%	0.002%
46	6.986	1748	1756	1758	rBV	247	243	0.02%	0.002%
47	7.018	1764	1766	1771	rVV2	364	267	0.02%	0.003%
48	7.179	1810	1816	1818	rBV2	526	429	0.03%	0.004%
49	7.565	1924	1936	1964	rBV	150897	265302	21.11%	2.641%
50	7.742	1988	1991	1994	rVB2	355	221	0.02%	0.002%
51	7.796	2002	2008	2012	rBV4	741	863	0.07%	0.009%
52	7.899	2026	2040	2068	rBV	405855	707689	56.31%	7.045%
53	8.179	2116	2127	2145	rVV	103683	176730	14.06%	1.759%
54	8.465	2213	2216	2219	rBV4	445	365	0.03%	0.004%
55	8.565	2242	2247	2250	rBV2	384	377	0.03%	0.004%
56	8.636	2255	2269	2324	rBV3	493491	1073802	85.44%	10.689%
57	8.909	2351	2354	2356	rVB3	546	286	0.02%	0.003%
58	8.999	2379	2382	2383	rBV2	321	188	0.01%	0.002%
59	9.105	2413	2415	2419	rBV	273	196	0.02%	0.002%
60	9.153	2426	2430	2431	rBV	275	207	0.02%	0.002%
61	9.205	2441	2446	2447	rBV	242	187	0.01%	0.002%
62	9.417	2499	2512	2553	rVV	550402	924404	73.55%	9.202%
63	9.603	2568	2570	2573	rBV	313	176	0.01%	0.002%
64	9.623	2573	2576	2581	rVB2	240	180	0.01%	0.002%
65	9.681	2588	2594	2595	rBV	346	306	0.02%	0.003%
66	9.783	2623	2626	2628	rBV2	376	250	0.02%	0.002%
67	9.835	2636	2642	2643	rBV2	276	219	0.02%	0.002%
68	9.983	2684	2688	2692	rBV2	210	220	0.02%	0.002%
69	10.465	2835	2838	2842	rVB	309	250	0.02%	0.002%
70	10.491	2842	2846	2850	rBV3	325	271	0.02%	0.003%
71	10.700	2908	2911	2914	rBV2	314	187	0.01%	0.002%
72	10.758	2914	2929	2955	rBV	591561	980092	77.98%	9.756%
73	11.279	3089	3091	3097	rBV2	241	182	0.01%	0.002%
74	11.394	3121	3127	3130	rBV	427	527	0.04%	0.005%
75	11.410	3130	3132	3136	rVV2	342	241	0.02%	0.002%
76	11.430	3136	3138	3142	rVV2	216	202	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050456.D
 Acq On : 26 Aug 2022 14:50
 Operator : SY/MD
 Sample : N4365-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.459	3145	3147	3151	rBV	202	186	0.01%	0.002%
78	11.533	3165	3170	3174	rBV2	294	311	0.02%	0.003%
79	11.745	3232	3236	3243	rBV2	799	912	0.07%	0.009%
80	11.812	3244	3257	3278	rBV	395232	642993	51.16%	6.401%
81	12.031	3320	3325	3328	rBV3	332	405	0.03%	0.004%
82	12.073	3333	3338	3347	rVV4	1328	1939	0.15%	0.019%
83	12.195	3362	3376	3402	rBV	460706	774654	61.63%	7.711%
84	12.410	3440	3443	3444	rBV2	387	260	0.02%	0.003%
85	12.500	3468	3471	3475	rBV3	274	250	0.02%	0.002%
86	12.542	3480	3484	3487	rBV2	611	404	0.03%	0.004%
87	12.574	3491	3494	3497	rBV	368	276	0.02%	0.003%
88	12.658	3518	3520	3523	rBV2	249	195	0.02%	0.002%
89	12.706	3533	3535	3538	rBV2	378	278	0.02%	0.003%
90	12.861	3580	3583	3587	rBV3	330	320	0.03%	0.003%
91	12.951	3607	3611	3614	rBV3	338	277	0.02%	0.003%
92	12.996	3622	3625	3628	rBV4	441	332	0.03%	0.003%
93	13.320	3721	3726	3727	rBV	259	196	0.02%	0.002%
94	13.552	3793	3798	3801	rBV3	551	535	0.04%	0.005%
95	13.581	3804	3807	3810	rBV3	780	648	0.05%	0.006%
96	13.645	3825	3827	3829	rBV2	321	183	0.01%	0.002%
97	13.838	3884	3887	3888	rBV2	428	252	0.02%	0.003%
98	14.102	3963	3969	3977	rVB5	1717	2318	0.18%	0.023%
99	14.333	4036	4041	4049	rBV4	1511	2205	0.18%	0.022%
100	14.716	4156	4160	4168	rBV2	493	718	0.06%	0.007%




Sum of corrected areas: 10045579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050456.D
Acq On : 26 Aug 2022 14:50
Operator : SY/MD
Sample : N4365-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

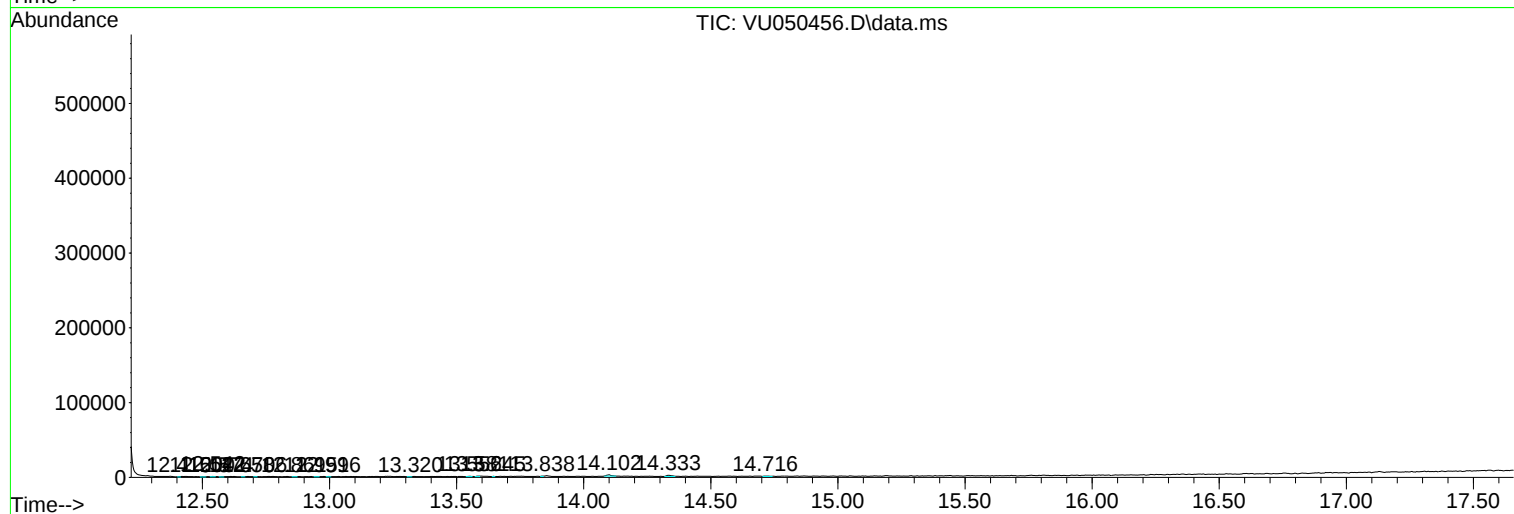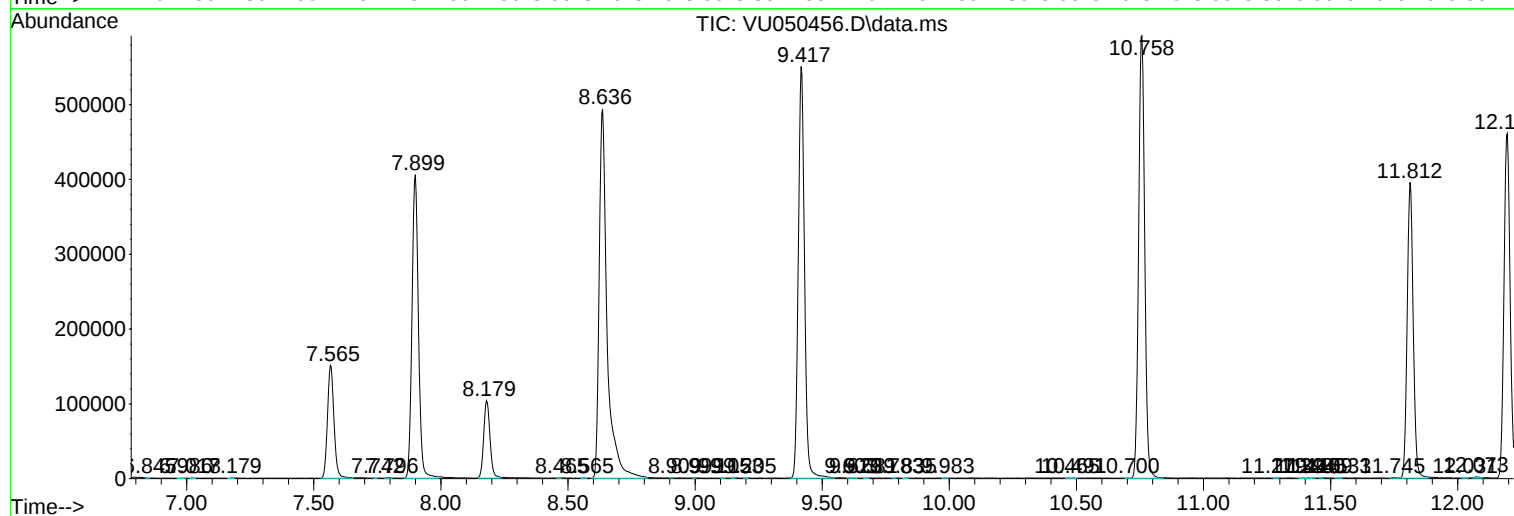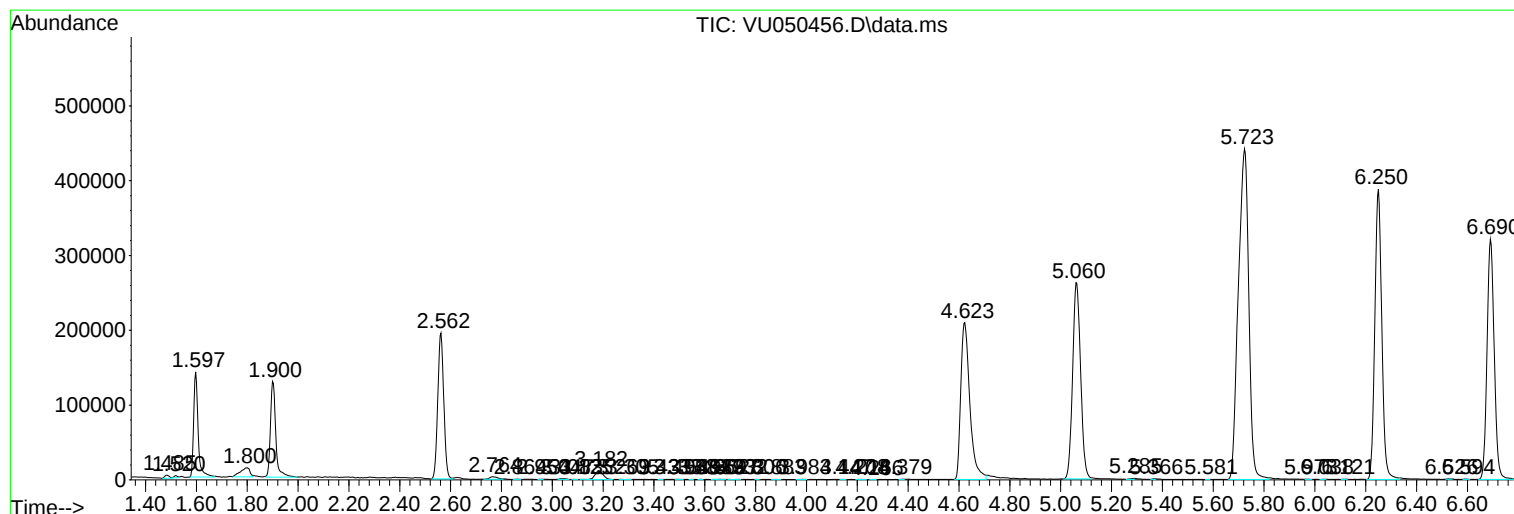

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050456.D
Acq On : 26 Aug 2022 14:50
Operator : SY/MD
Sample : N4365-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050456.D
Acq On : 26 Aug 2022 14:50
Operator : SY/MD
Sample : N4365-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------