

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050460.D
 Acq On : 26 Aug 2022 16:25
 Operator : SY/MD
 Sample : N4322-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY178

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	52	56	64	rBV4	2392	3204	0.01%	0.008%
2	1.597	72	80	111	rBV	200778	257628	0.88%	0.624%
3	1.899	166	174	197	rBV	160792	222548	0.76%	0.539%
4	2.562	367	380	396	rBV2	314837	529497	1.81%	1.283%
5	2.764	439	443	444	rBB2	257	429	0.00%	0.001%
6	2.848	467	469	479	rVB2	309	389	0.00%	0.001%
7	2.915	485	490	493	rVB2	348	258	0.00%	0.001%
8	2.954	498	502	507	rVB2	359	324	0.00%	0.001%
9	3.041	523	529	536	rVB4	1183	1726	0.01%	0.004%
10	3.186	561	574	584	rBV4	1691	4020	0.01%	0.010%
11	3.350	611	625	648	rBV	84595	167498	0.57%	0.406%
12	3.481	663	666	669	rBV2	267	192	0.00%	0.000%
13	3.497	669	671	677	rVB2	239	236	0.00%	0.001%
14	3.639	709	715	719	rVB3	418	438	0.00%	0.001%
15	3.681	724	728	731	rBV2	277	274	0.00%	0.001%
16	3.867	767	786	812	rBV2	278702	661554	2.26%	1.603%
17	4.031	835	837	843	rVB4	269	259	0.00%	0.001%
18	4.115	857	863	867	rVB4	339	431	0.00%	0.001%
19	4.234	897	900	904	rVB	308	236	0.00%	0.001%
20	4.298	917	920	923	rBV2	247	210	0.00%	0.001%
21	4.372	940	943	947	rBV2	267	216	0.00%	0.001%
22	4.443	960	965	969	rBV2	254	188	0.00%	0.000%
23	4.468	971	973	979	rBV2	262	283	0.00%	0.001%
24	4.626	1008	1022	1024	rBV	177842	282596	0.96%	0.685%
25	4.931	1114	1117	1120	rVB	462	317	0.00%	0.001%
26	4.970	1126	1129	1132	rBV3	307	217	0.00%	0.001%
27	5.063	1141	1158	1192	rBV	282809	620653	2.12%	1.504%
28	5.314	1219	1236	1252	rBV3	78291	183546	0.63%	0.445%
29	5.520	1296	1300	1304	rVB2	257	188	0.00%	0.000%
30	5.552	1307	1310	1312	rBV3	312	230	0.00%	0.001%
31	5.726	1342	1364	1400	rBV2	587258	1588107	5.42%	3.849%
32	5.886	1412	1414	1418	rVB3	633	373	0.00%	0.001%
33	5.909	1418	1421	1424	rBV2	312	256	0.00%	0.001%
34	5.976	1440	1442	1446	rVB2	566	331	0.00%	0.001%
35	6.108	1479	1483	1484	rBV	302	221	0.00%	0.001%
36	6.121	1484	1487	1494	rVB2	492	525	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050460.D
 Acq On : 26 Aug 2022 16:25
 Operator : SY/MD
 Sample : N4322-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY178

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.163	1494	1500	1503	rBV2	406	312	0.00%	0.001%
38	6.179	1503	1505	1511	rVB2	431	302	0.00%	0.001%
39	6.250	1511	1527	1551	rBV	404562	772850	2.64%	1.873%
40	6.359	1558	1561	1563	rBV3	451	244	0.00%	0.001%
41	6.484	1596	1600	1601	rBV2	365	241	0.00%	0.001%
42	6.546	1601	1619	1651	rBV	15991592	29289075	100.00%	70.985%
43	6.693	1654	1665	1692	rVB	374459	760078	2.60%	1.842%
44	7.044	1769	1774	1777	rBV5	481	459	0.00%	0.001%
45	7.086	1784	1787	1788	rBV	452	265	0.00%	0.001%
46	7.173	1810	1814	1815	rBV2	509	359	0.00%	0.001%
47	7.353	1864	1870	1872	rBV2	241	250	0.00%	0.001%
48	7.481	1907	1910	1914	rVB2	318	216	0.00%	0.001%
49	7.568	1924	1937	1963	rBV	181910	325865	1.11%	0.790%
50	7.761	1994	1997	1999	rBV2	335	197	0.00%	0.000%
51	7.787	2002	2005	2010	rVB4	405	361	0.00%	0.001%
52	7.899	2025	2040	2068	rBV	643119	1129263	3.86%	2.737%
53	8.179	2116	2127	2149	rBV	124526	213462	0.73%	0.517%
54	8.282	2157	2159	2162	rVB2	650	326	0.00%	0.001%
55	8.635	2256	2269	2316	rBV3	435981	902420	3.08%	2.187%
56	8.899	2348	2351	2352	rBV3	354	180	0.00%	0.000%
57	8.963	2367	2371	2372	rBV	264	196	0.00%	0.000%
58	9.002	2380	2383	2387	rBV2	304	298	0.00%	0.001%
59	9.021	2387	2389	2396	rVB3	572	548	0.00%	0.001%
60	9.057	2396	2400	2403	rBV3	310	314	0.00%	0.001%
61	9.121	2418	2420	2423	rBV	414	267	0.00%	0.001%
62	9.166	2431	2434	2436	rVB2	393	196	0.00%	0.000%
63	9.208	2443	2447	2454	rBV3	367	474	0.00%	0.001%
64	9.420	2499	2513	2554	rBV	563659	960672	3.28%	2.328%
65	9.700	2595	2600	2608	rBV4	532	737	0.00%	0.002%
66	9.742	2608	2613	2616	rBV	396	368	0.00%	0.001%
67	9.848	2640	2646	2650	rBV	275	355	0.00%	0.001%
68	9.989	2686	2690	2692	rBV2	249	202	0.00%	0.000%
69	10.041	2703	2706	2709	rBV2	273	186	0.00%	0.000%
70	10.105	2723	2726	2732	rBV	296	311	0.00%	0.001%
71	10.156	2738	2742	2747	rVB	240	180	0.00%	0.000%
72	10.188	2747	2752	2758	rBV2	426	415	0.00%	0.001%
73	10.571	2867	2871	2874	rBV2	395	311	0.00%	0.001%
74	10.635	2888	2891	2894	rBV2	283	197	0.00%	0.000%
75	10.655	2894	2897	2900	rVB2	361	247	0.00%	0.001%
76	10.758	2915	2929	2957	rBV	527472	848153	2.90%	2.056%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050460.D
 Acq On : 26 Aug 2022 16:25
 Operator : SY/MD
 Sample : N4322-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY178

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.934	2978	2984	2986	rBV3	375	469	0.00%	0.001%
78	11.262	3082	3086	3089	rBV2	225	234	0.00%	0.001%
79	11.291	3093	3095	3099	rBV2	242	227	0.00%	0.001%
80	11.430	3132	3138	3141	rBV2	286	346	0.00%	0.001%
81	11.536	3168	3171	3176	rBV	327	269	0.00%	0.001%
82	11.629	3198	3200	3204	rBV3	420	343	0.00%	0.001%
83	11.764	3238	3242	3244	rBV3	273	217	0.00%	0.001%
84	11.815	3245	3258	3277	rBV	422703	680917	2.32%	1.650%
85	12.147	3356	3361	3363	rBV2	740	644	0.00%	0.002%
86	12.195	3363	3376	3396	rVV	510099	831328	2.84%	2.015%
87	12.458	3455	3458	3459	rBV2	336	182	0.00%	0.000%
88	12.568	3487	3492	3496	rBV4	407	426	0.00%	0.001%
89	12.867	3580	3585	3586	rBV	629	493	0.00%	0.001%
90	12.915	3597	3600	3606	rBV2	440	365	0.00%	0.001%
91	13.034	3633	3637	3638	rBV2	490	400	0.00%	0.001%
92	13.073	3646	3649	3653	rBV4	401	409	0.00%	0.001%
93	13.266	3707	3709	3712	rBV2	345	189	0.00%	0.000%
94	13.542	3792	3795	3800	rBV3	446	450	0.00%	0.001%
95	13.597	3809	3812	3813	rBV2	290	200	0.00%	0.000%
96	13.606	3813	3815	3823	rVV3	509	456	0.00%	0.001%
97	13.642	3823	3826	3829	rVV2	348	233	0.00%	0.001%
98	14.101	3964	3969	3970	rBV2	558	495	0.00%	0.001%
99	14.372	4048	4053	4057	rBV2	416	519	0.00%	0.001%
100	15.143	4290	4293	4295	rBV2	535	321	0.00%	0.001%




Sum of corrected areas: 41261082

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050460.D
Acq On : 26 Aug 2022 16:25
Operator : SY/MD
Sample : N4322-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY178

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

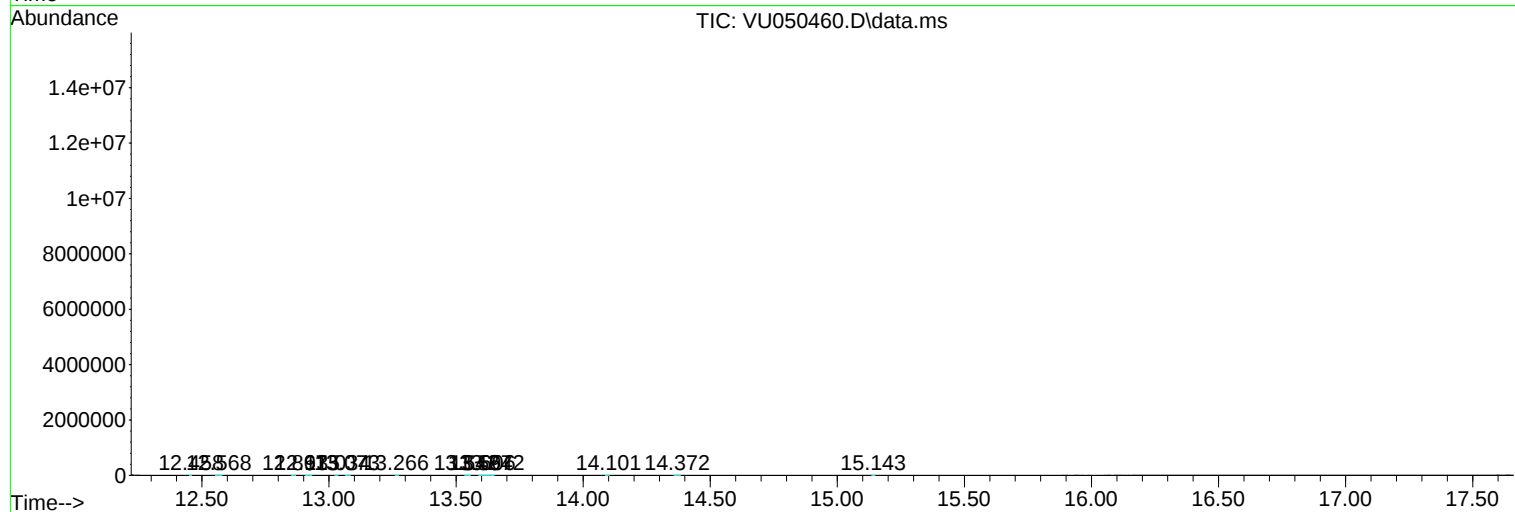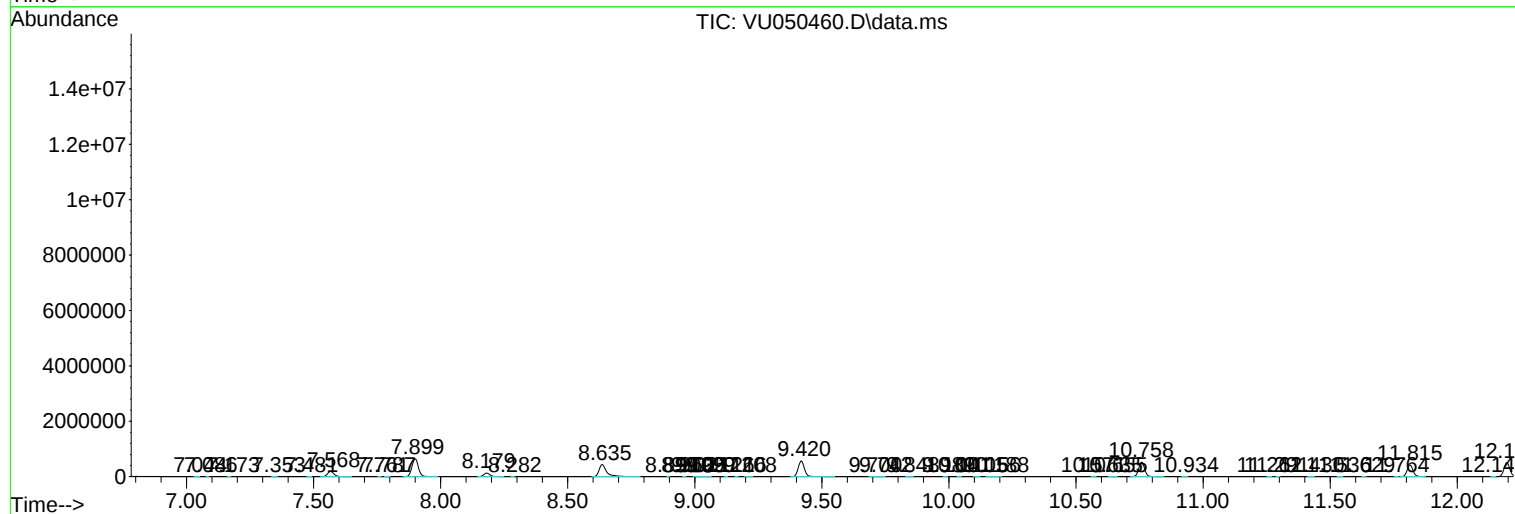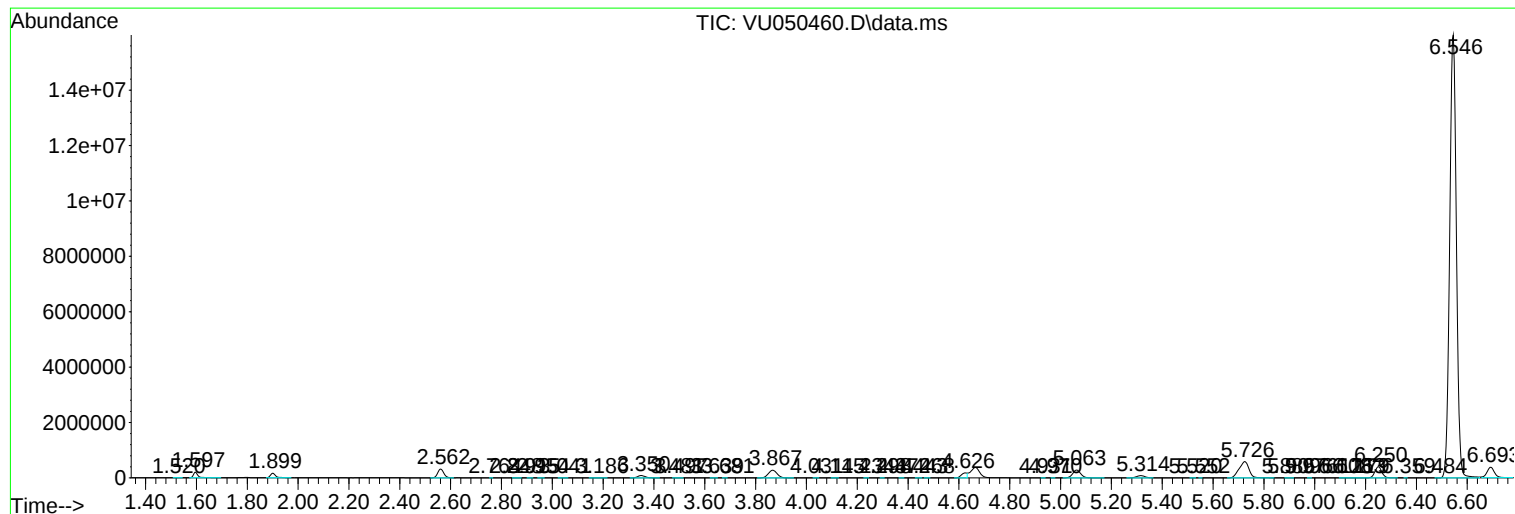

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050460.D
Acq On : 26 Aug 2022 16:25
Operator : SY/MD
Sample : N4322-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY178

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050460.D
Acq On : 26 Aug 2022 16:25
Operator : SY/MD
Sample : N4322-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY178

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------