

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050463.D
 Acq On : 26 Aug 2022 17:37
 Operator : SY/MD
 Sample : N4322-26
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY181

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	101	rBV	214170	250044	16.04%	2.317%
2	1.903	166	175	199	rVB	170743	232171	14.89%	2.152%
3	2.440	339	342	356	rVB7	2210	3549	0.23%	0.033%
4	2.562	366	380	394	rBV	314210	506779	32.51%	4.697%
5	2.768	436	444	455	rBV4	3283	6467	0.41%	0.060%
6	2.813	456	458	465	rVB	713	645	0.04%	0.006%
7	3.044	519	530	539	rBV5	1036	1828	0.12%	0.017%
8	3.189	564	575	586	rVB4	1064	2333	0.15%	0.022%
9	3.292	603	607	612	rVB	240	168	0.01%	0.002%
10	3.427	645	649	652	rVV	219	237	0.02%	0.002%
11	3.562	685	691	694	rBV2	165	169	0.01%	0.002%
12	3.787	757	761	763	rBV2	300	224	0.01%	0.002%
13	3.861	780	784	787	rBV3	568	526	0.03%	0.005%
14	3.928	801	805	809	rVB2	223	175	0.01%	0.002%
15	4.121	862	865	868	rBV	346	198	0.01%	0.002%
16	4.176	878	882	886	rBV2	229	217	0.01%	0.002%
17	4.333	929	931	935	rVB	357	207	0.01%	0.002%
18	4.562	996	1002	1007	rVB2	242	234	0.02%	0.002%
19	4.623	1007	1021	1049	rBV	163870	403101	25.86%	3.736%
20	5.063	1140	1158	1184	rBV	282849	618856	39.70%	5.735%
21	5.295	1220	1230	1239	rVB5	1354	2739	0.18%	0.025%
22	5.375	1248	1255	1260	rBV3	713	1166	0.07%	0.011%
23	5.726	1339	1364	1385	rBV2	577309	1558835	100.00%	14.446%
24	5.973	1438	1441	1446	rVB	450	350	0.02%	0.003%
25	6.034	1456	1460	1463	rBV4	343	276	0.02%	0.003%
26	6.105	1477	1482	1484	rBV2	405	314	0.02%	0.003%
27	6.157	1495	1498	1504	rBV2	359	412	0.03%	0.004%
28	6.250	1510	1527	1550	rBV	378523	718087	46.07%	6.655%
29	6.385	1567	1569	1573	rVB2	515	267	0.02%	0.002%
30	6.407	1573	1576	1578	rVB3	403	244	0.02%	0.002%
31	6.472	1593	1596	1600	rBV2	435	353	0.02%	0.003%
32	6.542	1608	1618	1630	rBV4	10051	19045	1.22%	0.176%
33	6.591	1630	1633	1638	rVB4	294	295	0.02%	0.003%
34	6.690	1649	1664	1691	rBV	370399	717897	46.05%	6.653%
35	6.845	1708	1712	1714	rBV3	418	307	0.02%	0.003%
36	6.903	1727	1730	1732	rBV3	243	170	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050463.D
 Acq On : 26 Aug 2022 17:37
 Operator : SY/MD
 Sample : N4322-26
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY181

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.915	1732	1734	1738	rVV2	273	226	0.01%	0.002%
38	6.938	1738	1741	1748	rVB2	258	260	0.02%	0.002%
39	6.989	1752	1757	1763	rBV	186	223	0.01%	0.002%
40	7.018	1763	1766	1771	rVB2	331	287	0.02%	0.003%
41	7.050	1771	1776	1778	rBV	294	232	0.01%	0.002%
42	7.189	1813	1819	1823	rVB2	543	635	0.04%	0.006%
43	7.433	1890	1895	1899	rBV2	172	197	0.01%	0.002%
44	7.568	1921	1937	1953	rBV	174534	306780	19.68%	2.843%
45	7.671	1966	1969	1973	rVB	433	281	0.02%	0.003%
46	7.710	1978	1981	1983	rBV2	585	411	0.03%	0.004%
47	7.793	2003	2007	2010	rBV2	313	304	0.02%	0.003%
48	7.825	2014	2017	2022	rVB3	335	272	0.02%	0.003%
49	7.899	2022	2040	2068	rBV	640859	1113743	71.45%	10.321%
50	8.179	2116	2127	2147	rBV	121847	204860	13.14%	1.899%
51	8.301	2160	2165	2168	rBV4	389	423	0.03%	0.004%
52	8.353	2179	2181	2184	rVB2	329	178	0.01%	0.002%
53	8.484	2218	2222	2225	rBV3	409	314	0.02%	0.003%
54	8.552	2237	2243	2244	rBV3	1773	1612	0.10%	0.015%
55	8.636	2256	2269	2318	rBV3	423420	874216	56.08%	8.102%
56	8.954	2366	2368	2375	rVB3	403	295	0.02%	0.003%
57	9.057	2396	2400	2403	rBV	211	180	0.01%	0.002%
58	9.095	2408	2412	2415	rBV2	262	198	0.01%	0.002%
59	9.124	2419	2421	2425	rVB2	310	177	0.01%	0.002%
60	9.160	2428	2432	2435	rVB3	506	351	0.02%	0.003%
61	9.198	2442	2444	2448	rBV2	281	237	0.02%	0.002%
62	9.288	2469	2472	2477	rBV2	246	211	0.01%	0.002%
63	9.317	2477	2481	2486	rBV	260	266	0.02%	0.002%
64	9.417	2498	2512	2530	rBV	542983	888869	57.02%	8.237%
65	9.574	2559	2561	2570	rVB4	557	584	0.04%	0.005%
66	9.703	2599	2601	2605	rVB3	395	217	0.01%	0.002%
67	9.793	2623	2629	2630	rBV2	294	214	0.01%	0.002%
68	9.906	2662	2664	2670	rBV2	205	166	0.01%	0.002%
69	9.941	2672	2675	2681	rVB	252	227	0.01%	0.002%
70	9.983	2681	2688	2692	rBV2	200	263	0.02%	0.002%
71	10.025	2698	2701	2707	rVB	348	341	0.02%	0.003%
72	10.092	2720	2722	2725	rVV	346	193	0.01%	0.002%
73	10.195	2748	2754	2757	rBV2	172	196	0.01%	0.002%
74	10.224	2757	2763	2766	rVB3	318	308	0.02%	0.003%
75	10.256	2766	2773	2777	rBV2	218	291	0.02%	0.003%
76	10.314	2787	2791	2796	rBV2	539	536	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050463.D
 Acq On : 26 Aug 2022 17:37
 Operator : SY/MD
 Sample : N4322-26
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY181

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.417	2820	2823	2829	rBV2	163	191	0.01%	0.002%
78	10.758	2915	2929	2951	rBV	523377	843262	54.10%	7.815%
79	11.098	3033	3035	3040	rVB2	278	200	0.01%	0.002%
80	11.475	3149	3152	3156	rBV3	379	296	0.02%	0.003%
81	11.539	3169	3172	3177	rBV	349	249	0.02%	0.002%
82	11.812	3244	3257	3277	rBV	391111	638621	40.97%	5.918%
83	12.066	3326	3336	3349	rBV5	5092	10065	0.65%	0.093%
84	12.195	3363	3376	3402	rBV	504478	844211	54.16%	7.824%
85	12.349	3420	3424	3426	rBV2	289	214	0.01%	0.002%
86	12.552	3484	3487	3492	rVB2	425	360	0.02%	0.003%
87	12.584	3493	3497	3502	rBV2	334	366	0.02%	0.003%
88	12.651	3515	3518	3520	rBV2	289	198	0.01%	0.002%
89	12.719	3536	3539	3540	rBV2	354	179	0.01%	0.002%
90	12.783	3557	3559	3561	rBV	295	180	0.01%	0.002%
91	12.912	3597	3599	3605	rVB	532	317	0.02%	0.003%
92	12.967	3612	3616	3620	rBV3	319	314	0.02%	0.003%
93	13.098	3650	3657	3658	rBV2	392	446	0.03%	0.004%
94	13.159	3674	3676	3679	rBV2	301	226	0.01%	0.002%
95	13.237	3697	3700	3702	rBV3	331	241	0.02%	0.002%
96	13.330	3725	3729	3732	rBV2	426	387	0.02%	0.004%
97	13.825	3881	3883	3885	rBV	391	234	0.02%	0.002%
98	15.282	4333	4336	4338	rBV2	585	380	0.02%	0.004%
99	15.439	4383	4385	4386	rBV2	512	220	0.01%	0.002%
100	15.552	4418	4420	4426	rBV4	704	516	0.03%	0.005%




Sum of corrected areas: 10790532

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050463.D
Acq On : 26 Aug 2022 17:37
Operator : SY/MD
Sample : N4322-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY181

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

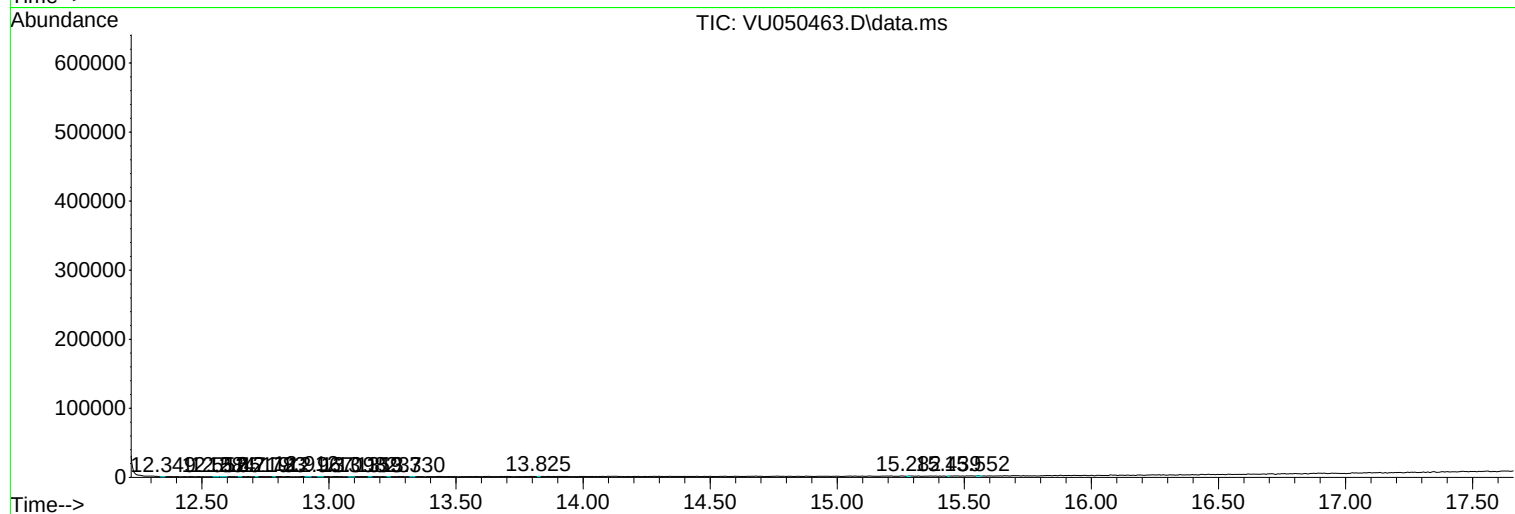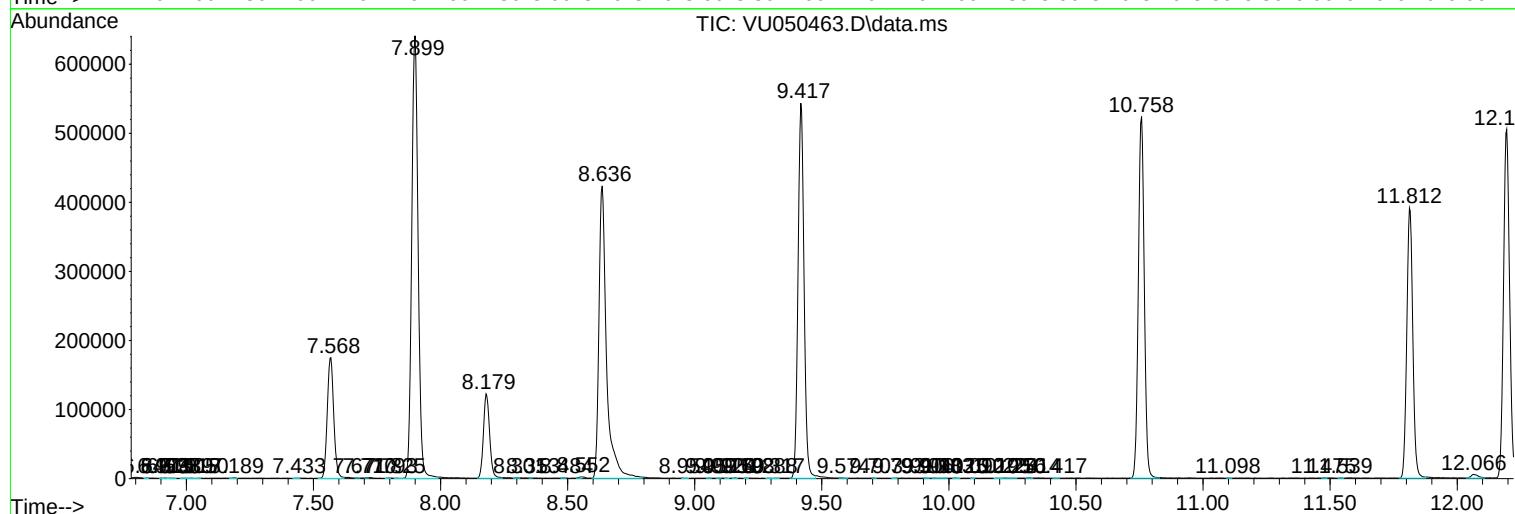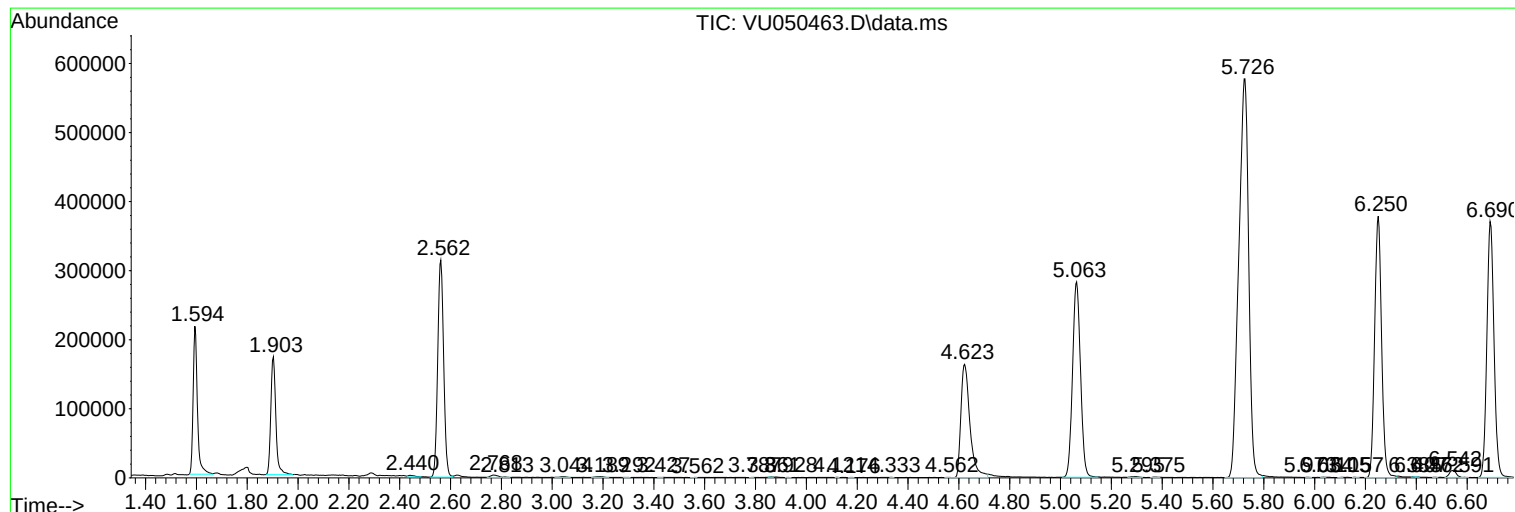

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050463.D
Acq On : 26 Aug 2022 17:37
Operator : SY/MD
Sample : N4322-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY181

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050463.D
Acq On : 26 Aug 2022 17:37
Operator : SY/MD
Sample : N4322-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY181

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc