

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050465.D
 Acq On : 26 Aug 2022 18:24
 Operator : SY/MD
 Sample : N4372-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV3	2945	2963	0.20%	0.028%
2	1.517	51	55	63	rBV2	3041	3870	0.26%	0.037%
3	1.594	72	79	100	rBV	200479	240982	15.96%	2.286%
4	1.903	166	175	193	rBV	160729	217362	14.40%	2.062%
5	2.562	367	380	396	rBV	292883	476789	31.58%	4.523%
6	2.732	430	433	434	rBV	470	219	0.01%	0.002%
7	2.764	435	443	457	rVB3	2423	5261	0.35%	0.050%
8	2.909	485	488	491	rBV2	250	186	0.01%	0.002%
9	3.012	516	520	522	rBV2	428	323	0.02%	0.003%
10	3.038	522	528	534	rBV4	1009	1195	0.08%	0.011%
11	3.147	559	562	565	rVV2	222	187	0.01%	0.002%
12	3.179	565	572	584	rVV4	1202	2643	0.18%	0.025%
13	3.298	606	609	611	rBV2	253	170	0.01%	0.002%
14	3.337	617	621	622	rBV2	299	208	0.01%	0.002%
15	3.350	622	625	630	rVB3	373	268	0.02%	0.003%
16	3.433	647	651	654	rVB2	338	272	0.02%	0.003%
17	3.517	671	677	680	rBV2	186	208	0.01%	0.002%
18	3.726	738	742	745	rBV2	275	185	0.01%	0.002%
19	3.822	770	772	776	rBV2	330	218	0.01%	0.002%
20	3.922	801	803	806	rVB	392	183	0.01%	0.002%
21	4.067	845	848	853	rVV2	216	237	0.02%	0.002%
22	4.334	928	931	934	rBV2	250	221	0.01%	0.002%
23	4.478	973	976	978	rBV3	275	183	0.01%	0.002%
24	4.523	983	990	992	rBV2	353	233	0.02%	0.002%
25	4.571	1000	1005	1008	rBV2	196	214	0.01%	0.002%
26	4.620	1008	1020	1057	rBV	159348	406086	26.90%	3.852%
27	5.063	1140	1158	1179	rBV	272318	595418	39.44%	5.649%
28	5.282	1220	1226	1227	rBV	911	691	0.05%	0.007%
29	5.372	1247	1254	1258	rBV	644	705	0.05%	0.007%
30	5.465	1278	1283	1286	rVB2	192	175	0.01%	0.002%
31	5.604	1323	1326	1330	rVB2	249	176	0.01%	0.002%
32	5.726	1342	1364	1400	rBV2	554542	1509620	100.00%	14.321%
33	6.128	1484	1489	1493	rBV3	714	550	0.04%	0.005%
34	6.147	1493	1495	1499	rBV2	251	195	0.01%	0.002%
35	6.250	1512	1527	1549	rBV	368168	701370	46.46%	6.654%
36	6.375	1562	1566	1571	rVB4	551	512	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050465.D
 Acq On : 26 Aug 2022 18:24
 Operator : SY/MD
 Sample : N4372-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.478	1596	1598	1602	rVB3	436	192	0.01%	0.002%
38	6.542	1603	1618	1637	rBV2	58345	112470	7.45%	1.067%
39	6.690	1649	1664	1692	rBV	356313	697479	46.20%	6.617%
40	6.864	1716	1718	1722	rVB2	581	349	0.02%	0.003%
41	6.899	1724	1729	1730	rBV2	282	171	0.01%	0.002%
42	6.957	1744	1747	1751	rVB2	208	197	0.01%	0.002%
43	7.012	1756	1764	1770	rVB2	173	239	0.02%	0.002%
44	7.186	1812	1818	1819	rBV	490	364	0.02%	0.003%
45	7.481	1907	1910	1915	rVB2	250	223	0.01%	0.002%
46	7.565	1920	1936	1955	rBV	167675	296460	19.64%	2.812%
47	7.706	1974	1980	1992	rVB6	936	1930	0.13%	0.018%
48	7.758	1992	1996	2000	rBV2	516	491	0.03%	0.005%
49	7.806	2009	2011	2016	rBV3	309	204	0.01%	0.002%
50	7.899	2025	2040	2069	rBV	619462	1065374	70.57%	10.107%
51	8.063	2088	2091	2096	rVB3	628	575	0.04%	0.005%
52	8.179	2115	2127	2149	rBV	115652	198618	13.16%	1.884%
53	8.378	2187	2189	2194	rBV3	192	172	0.01%	0.002%
54	8.459	2211	2214	2220	rBV2	314	340	0.02%	0.003%
55	8.581	2248	2252	2255	rBV2	350	259	0.02%	0.002%
56	8.636	2256	2269	2304	rBV3	403557	846451	56.07%	8.030%
57	8.973	2370	2374	2377	rVB2	294	225	0.01%	0.002%
58	9.111	2414	2417	2422	rBV3	224	226	0.01%	0.002%
59	9.263	2458	2464	2466	rBV2	307	312	0.02%	0.003%
60	9.337	2483	2487	2491	rBV2	250	251	0.02%	0.002%
61	9.417	2499	2512	2538	rBV	527003	881880	58.42%	8.366%
62	9.591	2564	2566	2570	rVB	413	208	0.01%	0.002%
63	9.645	2579	2583	2586	rVB2	349	308	0.02%	0.003%
64	9.674	2586	2592	2596	rBV	328	248	0.02%	0.002%
65	9.693	2596	2598	2602	rBV2	222	182	0.01%	0.002%
66	9.780	2621	2625	2632	rBV2	337	426	0.03%	0.004%
67	9.845	2641	2645	2649	rVB2	284	222	0.01%	0.002%
68	9.954	2674	2679	2682	rBV	392	331	0.02%	0.003%
69	10.063	2708	2713	2718	rBV2	206	279	0.02%	0.003%
70	10.128	2730	2733	2736	rBV	243	188	0.01%	0.002%
71	10.243	2765	2769	2773	rVB	319	281	0.02%	0.003%
72	10.272	2773	2778	2783	rBV	221	238	0.02%	0.002%
73	10.439	2826	2830	2838	rBV2	265	406	0.03%	0.004%
74	10.571	2866	2871	2873	rBV	235	188	0.01%	0.002%
75	10.639	2889	2892	2895	rBV2	289	233	0.02%	0.002%
76	10.758	2915	2929	2955	rBV	501885	822334	54.47%	7.801%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050465.D
 Acq On : 26 Aug 2022 18:24
 Operator : SY/MD
 Sample : N4372-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.263	3082	3086	3095	rVB	293	352	0.02%	0.003%
78	11.478	3151	3153	3157	rVB2	284	169	0.01%	0.002%
79	11.594	3185	3189	3192	rBV3	319	213	0.01%	0.002%
80	11.616	3193	3196	3201	rVB3	420	362	0.02%	0.003%
81	11.648	3201	3206	3210	rBV	336	343	0.02%	0.003%
82	11.812	3245	3257	3276	rBV	383989	626198	41.48%	5.941%
83	12.025	3315	3323	3328	rBV2	303	563	0.04%	0.005%
84	12.076	3330	3339	3348	rVV5	1600	2931	0.19%	0.028%
85	12.195	3363	3376	3402	rBV	485992	803540	53.23%	7.623%
86	12.725	3539	3541	3547	rBV3	256	215	0.01%	0.002%
87	12.816	3567	3569	3571	rBV2	298	175	0.01%	0.002%
88	12.870	3579	3586	3587	rBV2	325	351	0.02%	0.003%
89	12.925	3600	3603	3606	rBV3	235	171	0.01%	0.002%
90	13.012	3626	3630	3632	rBV3	340	268	0.02%	0.003%
91	13.044	3637	3640	3646	rBV2	444	551	0.04%	0.005%
92	13.098	3654	3657	3663	rVB3	317	293	0.02%	0.003%
93	13.124	3663	3665	3669	rBV3	364	227	0.02%	0.002%
94	13.176	3678	3681	3684	rBV2	249	210	0.01%	0.002%
95	13.275	3709	3712	3714	rBV	257	179	0.01%	0.002%
96	13.581	3805	3807	3810	rBV	351	245	0.02%	0.002%
97	13.626	3818	3821	3823	rBV	289	206	0.01%	0.002%
98	14.102	3966	3969	3974	rVB2	552	376	0.02%	0.004%
99	15.153	4293	4296	4297	rBV3	383	258	0.02%	0.002%
100	15.510	4405	4407	4414	rVB4	918	888	0.06%	0.008%




Sum of corrected areas: 10541086

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050465.D
Acq On : 26 Aug 2022 18:24
Operator : SY/MD
Sample : N4372-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

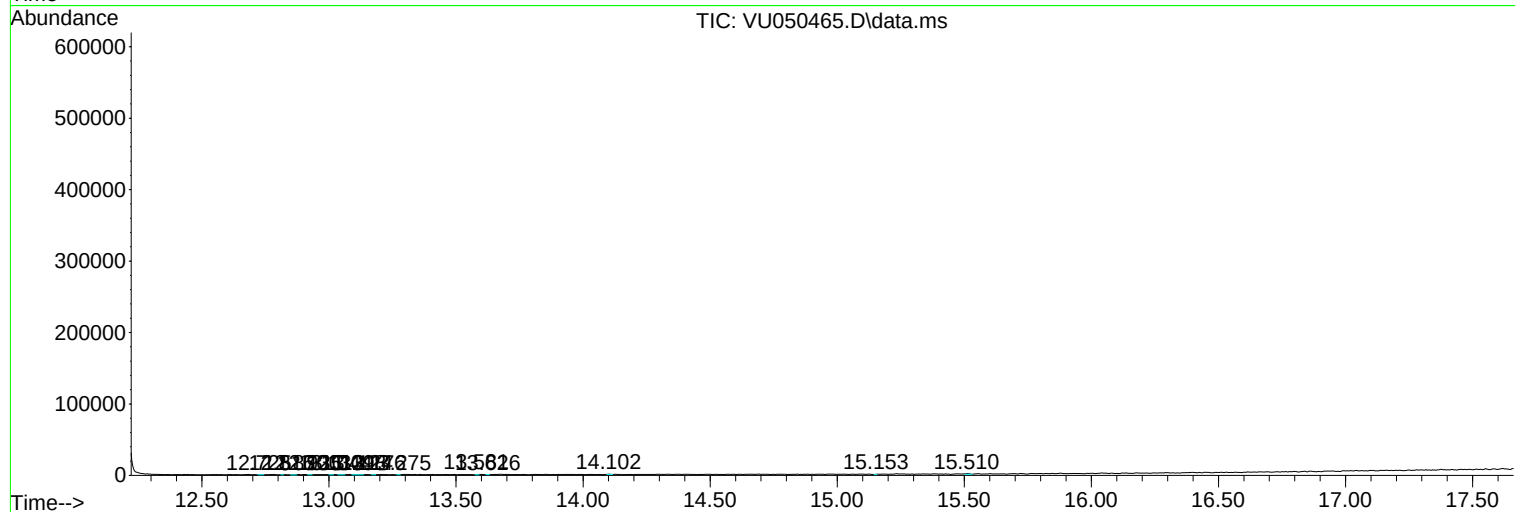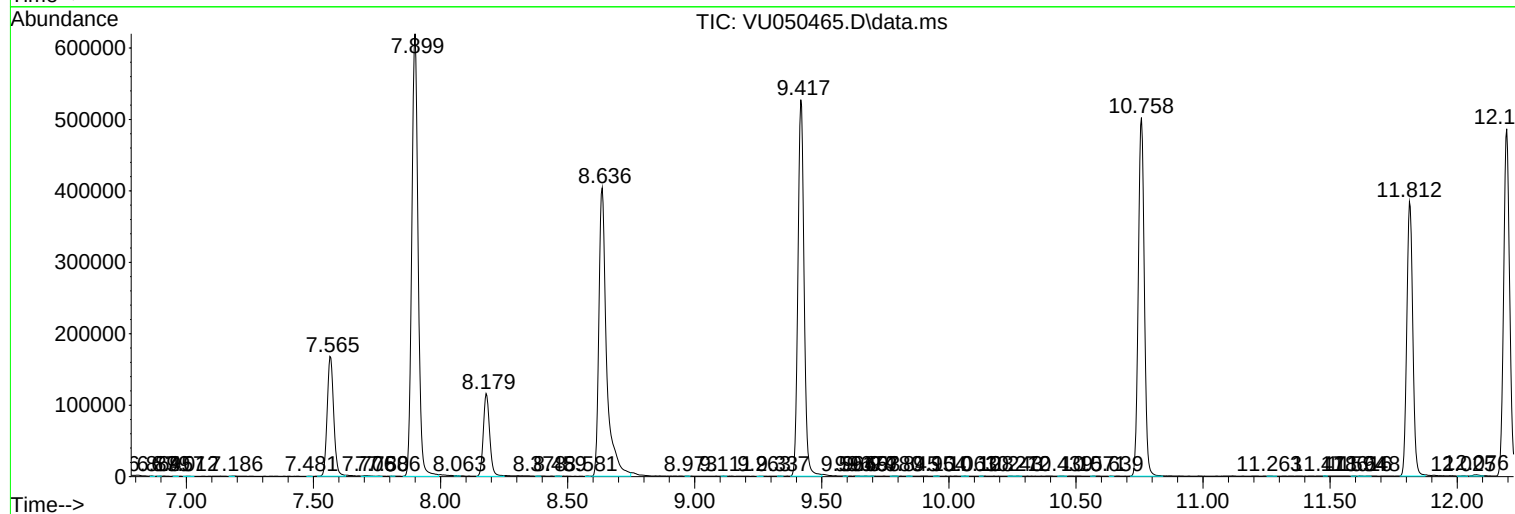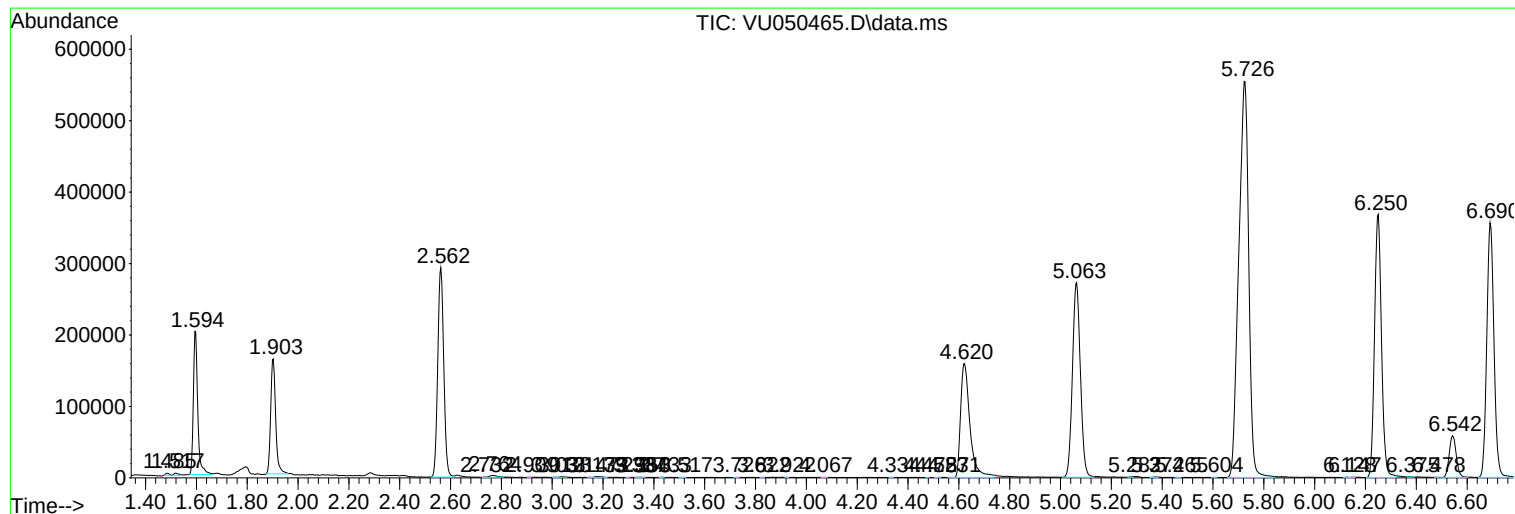

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050465.D
Acq On : 26 Aug 2022 18:24
Operator : SY/MD
Sample : N4372-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050465.D
Acq On : 26 Aug 2022 18:24
Operator : SY/MD
Sample : N4372-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc