

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050467.D
 Acq On : 26 Aug 2022 19:12
 Operator : SY/MD
 Sample : N4322-01ME
 Misc : 3.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY163ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.511	49	53	59	rVB2	3323	3314	0.20%	0.027%
2	1.591	71	78	87	rBV	78960	107977	6.60%	0.891%
3	1.874	162	166	176	rBV	32925	40341	2.46%	0.333%
4	2.520	355	367	386	rVB	234322	380525	23.25%	3.139%
5	2.649	399	407	409	rBV4	1958	2451	0.15%	0.020%
6	2.736	432	434	437	rBV2	386	266	0.02%	0.002%
7	2.932	493	495	497	rBV2	370	215	0.01%	0.002%
8	3.025	513	524	539	rBV2	11429	22833	1.40%	0.188%
9	3.112	548	551	554	rVB3	471	342	0.02%	0.003%
10	3.176	557	571	591	rBV	21143	54897	3.35%	0.453%
11	3.617	702	708	716	rBV2	365	463	0.03%	0.004%
12	3.668	719	724	725	rBV3	411	283	0.02%	0.002%
13	3.755	746	751	755	rVB2	293	274	0.02%	0.002%
14	3.829	768	774	778	rVB3	277	260	0.02%	0.002%
15	4.073	846	850	859	rBV	311	497	0.03%	0.004%
16	4.115	859	863	865	rVV	287	228	0.01%	0.002%
17	4.337	927	932	934	rBV2	345	238	0.01%	0.002%
18	4.372	938	943	946	rBV	298	242	0.01%	0.002%
19	4.494	977	981	984	rBV2	386	375	0.02%	0.003%
20	4.639	1012	1026	1090	rBV	224233	756145	46.20%	6.237%
21	4.883	1100	1102	1109	rVB4	597	547	0.03%	0.005%
22	4.916	1109	1112	1114	rBV	282	218	0.01%	0.002%
23	4.954	1121	1124	1128	rBV2	388	357	0.02%	0.003%
24	5.060	1140	1157	1182	rBV	315750	725841	44.35%	5.987%
25	5.282	1219	1226	1227	rBV3	1100	1179	0.07%	0.010%
26	5.372	1245	1254	1262	rVV9	1498	2436	0.15%	0.020%
27	5.443	1274	1276	1284	rVB2	328	299	0.02%	0.002%
28	5.488	1287	1290	1293	rBV	313	247	0.02%	0.002%
29	5.713	1339	1360	1388	rBV2	604964	1585934	96.90%	13.081%
30	5.977	1432	1442	1461	rBV4	10972	27529	1.68%	0.227%
31	6.243	1511	1525	1549	rBV	282334	567239	34.66%	4.679%
32	6.430	1578	1583	1590	rVB2	230	311	0.02%	0.003%
33	6.536	1603	1616	1629	rBV7	15596	31290	1.91%	0.258%
34	6.604	1629	1637	1649	rBV4	4316	8647	0.53%	0.071%
35	6.687	1649	1663	1680	rBV	396182	805491	49.21%	6.644%
36	6.800	1693	1698	1706	rVB7	1072	1553	0.09%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050467.D
 Acq On : 26 Aug 2022 19:12
 Operator : SY/MD
 Sample : N4322-01ME
 Misc : 3.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY163ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.970	1744	1751	1752	rBV2	389	356	0.02%	0.003%
38	7.063	1773	1780	1783	rBV2	346	331	0.02%	0.003%
39	7.231	1812	1832	1846	rBV7	5035	14675	0.90%	0.121%
40	7.282	1846	1848	1852	rVB3	515	371	0.02%	0.003%
41	7.304	1852	1855	1857	rBV3	644	425	0.03%	0.004%
42	7.395	1880	1883	1889	rBV2	252	290	0.02%	0.002%
43	7.565	1923	1936	1958	rBV	176695	335636	20.51%	2.768%
44	7.790	2003	2006	2008	rBV4	370	257	0.02%	0.002%
45	7.809	2008	2012	2016	rVB	517	467	0.03%	0.004%
46	7.896	2025	2039	2059	rBV	489625	872033	53.28%	7.193%
47	8.054	2086	2088	2090	rVB3	583	272	0.02%	0.002%
48	8.073	2090	2094	2104	rVB4	813	1158	0.07%	0.010%
49	8.182	2114	2128	2148	rBV	117982	233869	14.29%	1.929%
50	8.346	2173	2179	2180	rBV2	838	643	0.04%	0.005%
51	8.398	2192	2195	2197	rVB2	508	265	0.02%	0.002%
52	8.478	2216	2220	2227	rVB4	445	583	0.04%	0.005%
53	8.533	2233	2237	2243	rBV2	263	315	0.02%	0.003%
54	8.655	2258	2275	2309	rBV2	692327	1636740	100.00%	13.501%
55	8.954	2366	2368	2373	rVB2	417	291	0.02%	0.002%
56	9.002	2378	2383	2389	rVB4	503	645	0.04%	0.005%
57	9.034	2390	2393	2397	rBV4	333	235	0.01%	0.002%
58	9.115	2416	2418	2422	rVB3	367	221	0.01%	0.002%
59	9.144	2422	2427	2431	rBV2	546	665	0.04%	0.005%
60	9.166	2432	2434	2438	rVV	581	415	0.03%	0.003%
61	9.195	2440	2443	2447	rVB3	420	301	0.02%	0.002%
62	9.224	2447	2452	2455	rBV2	407	332	0.02%	0.003%
63	9.330	2480	2485	2489	rBV2	226	247	0.02%	0.002%
64	9.420	2496	2513	2534	rBV	382972	712132	43.51%	5.874%
65	9.565	2553	2558	2559	rBV2	493	317	0.02%	0.003%
66	9.578	2559	2562	2570	rVB4	865	943	0.06%	0.008%
67	9.697	2592	2599	2604	rBV5	1443	2018	0.12%	0.017%
68	9.755	2615	2617	2622	rVB2	316	215	0.01%	0.002%
69	9.986	2685	2689	2690	rBV2	316	218	0.01%	0.002%
70	10.105	2720	2726	2736	rVB3	1342	2118	0.13%	0.017%
71	10.240	2765	2768	2776	rVB2	311	269	0.02%	0.002%
72	10.375	2807	2810	2813	rBV	340	228	0.01%	0.002%
73	10.607	2877	2882	2885	rBV2	246	279	0.02%	0.002%
74	10.626	2885	2888	2892	rVV2	350	334	0.02%	0.003%
75	10.648	2892	2895	2902	rVV2	429	443	0.03%	0.004%
76	10.764	2914	2931	2951	rBV	886976	1467476	89.66%	12.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050467.D
 Acq On : 26 Aug 2022 19:12
 Operator : SY/MD
 Sample : N4322-01ME
 Misc : 3.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY163ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.896	2969	2972	2974	rBV3	623	377	0.02%	0.003%
78	11.012	3005	3008	3013	rBV2	238	223	0.01%	0.002%
79	11.063	3021	3024	3027	rVB	350	234	0.01%	0.002%
80	11.111	3037	3039	3040	rBV	451	220	0.01%	0.002%
81	11.253	3080	3083	3090	rBV2	400	329	0.02%	0.003%
82	11.468	3147	3150	3152	rBV2	641	407	0.02%	0.003%
83	11.510	3161	3163	3172	rVB	379	351	0.02%	0.003%
84	11.816	3246	3258	3279	rBV	349847	554016	33.85%	4.570%
85	12.198	3363	3377	3398	rBV	699393	1141092	69.72%	9.412%
86	12.578	3492	3495	3499	rBV2	347	216	0.01%	0.002%
87	12.677	3521	3526	3529	rBV3	286	295	0.02%	0.002%
88	12.764	3550	3553	3557	rBV2	445	412	0.03%	0.003%
89	12.896	3590	3594	3596	rBV4	343	276	0.02%	0.002%
90	13.028	3631	3635	3639	rBV3	233	236	0.01%	0.002%
91	13.079	3647	3651	3652	rBV	498	344	0.02%	0.003%
92	13.291	3714	3717	3722	rVV3	353	342	0.02%	0.003%
93	13.558	3797	3800	3802	rBV2	363	273	0.02%	0.002%
94	13.680	3835	3838	3841	rVB2	398	256	0.02%	0.002%
95	13.703	3842	3845	3849	rBV2	386	408	0.02%	0.003%
96	13.944	3918	3920	3927	rVB2	514	376	0.02%	0.003%
97	15.082	4271	4274	4278	rBV2	683	440	0.03%	0.004%
98	15.227	4316	4319	4328	rVB5	905	955	0.06%	0.008%
99	15.478	4393	4397	4400	rBV2	870	760	0.05%	0.006%
100	15.510	4405	4407	4413	rBV3	484	372	0.02%	0.003%




Sum of corrected areas: 12123522

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050467.D
Acq On : 26 Aug 2022 19:12
Operator : SY/MD
Sample : N4322-01ME
Misc : 3.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY163ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

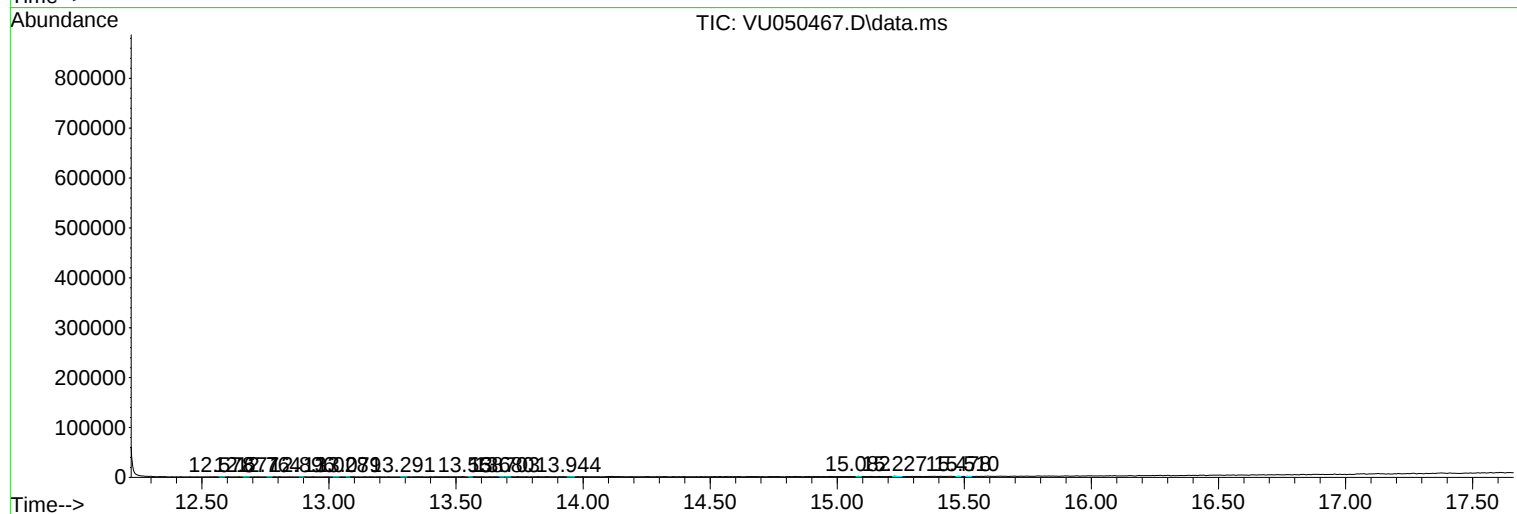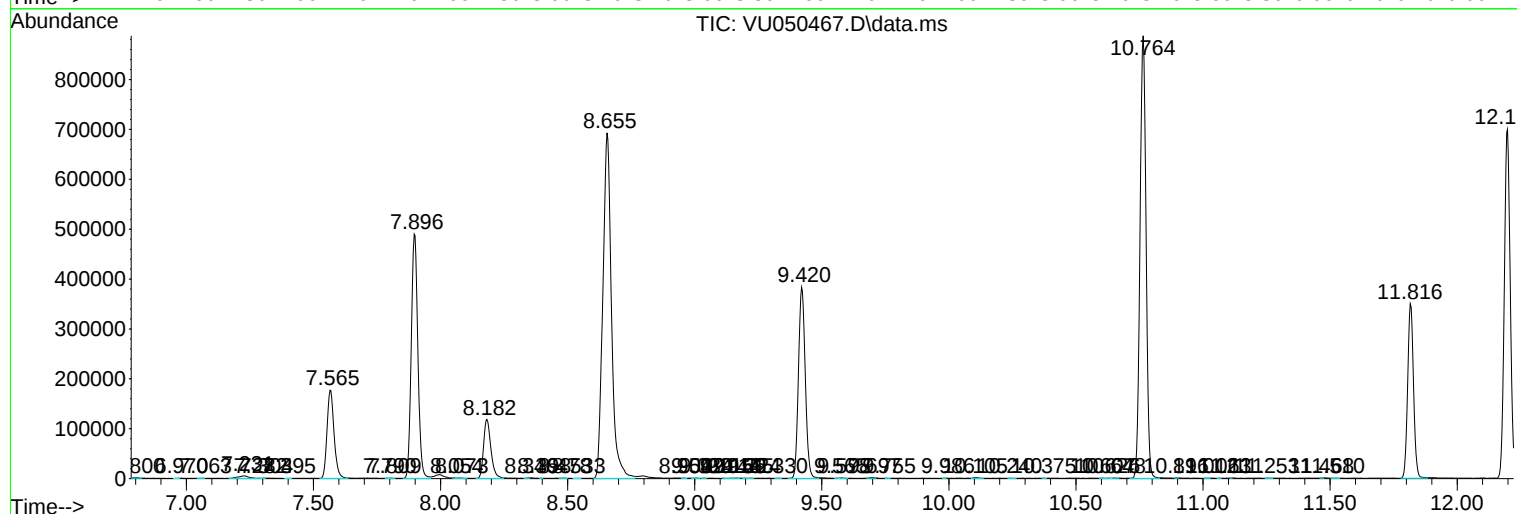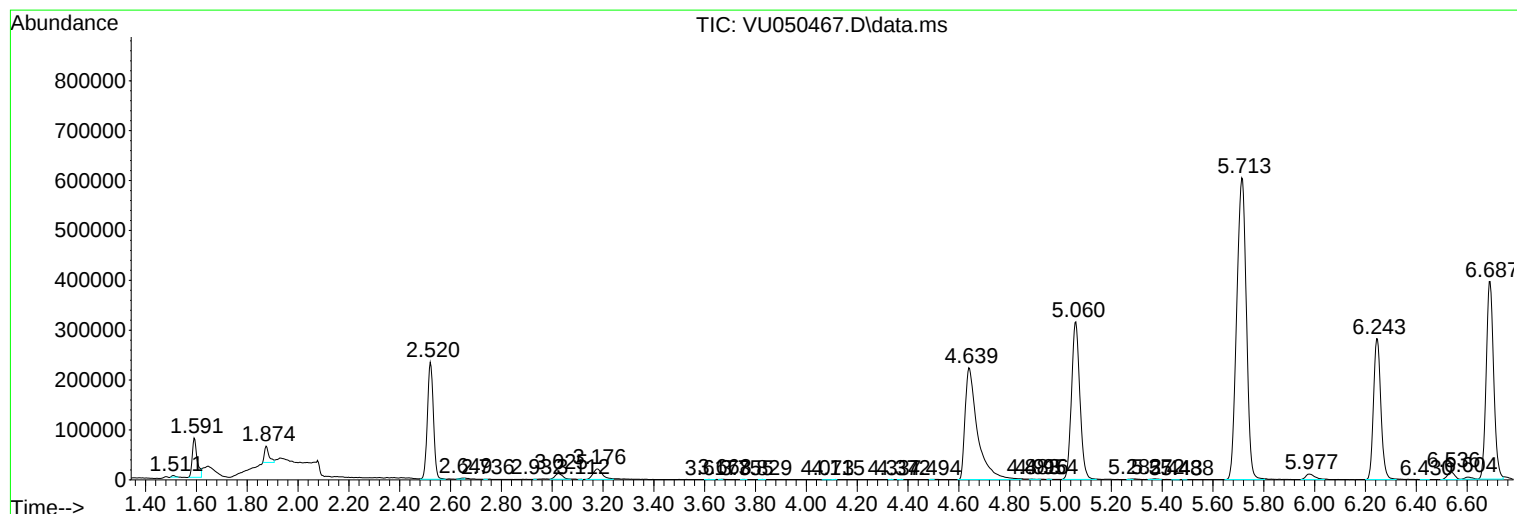

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050467.D
Acq On : 26 Aug 2022 19:12
Operator : SY/MD
Sample : N4322-01ME
Misc : 3.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY163ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
Data File : VU050467.D
Acq On : 26 Aug 2022 19:12
Operator : SY/MD
Sample : N4322-01ME
Misc : 3.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY163ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------